
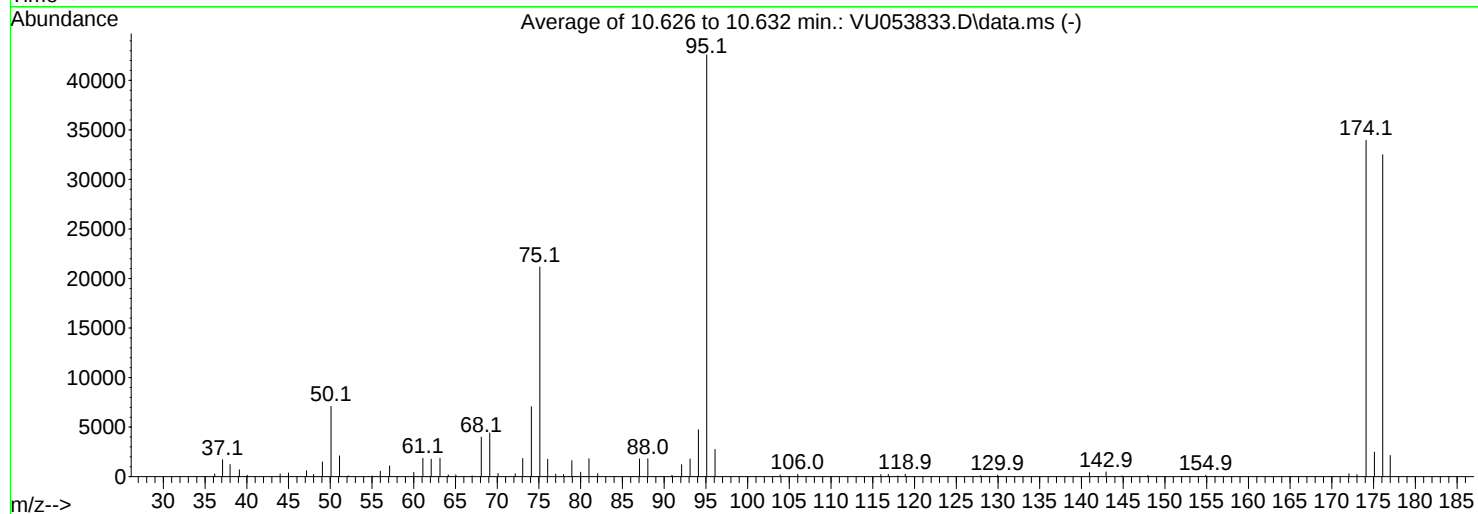


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053833.D
Acq On : 24 Apr 2023 10:35
Operator : JC/MD
Sample : BFB007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB007

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 26 05:09:52 2023

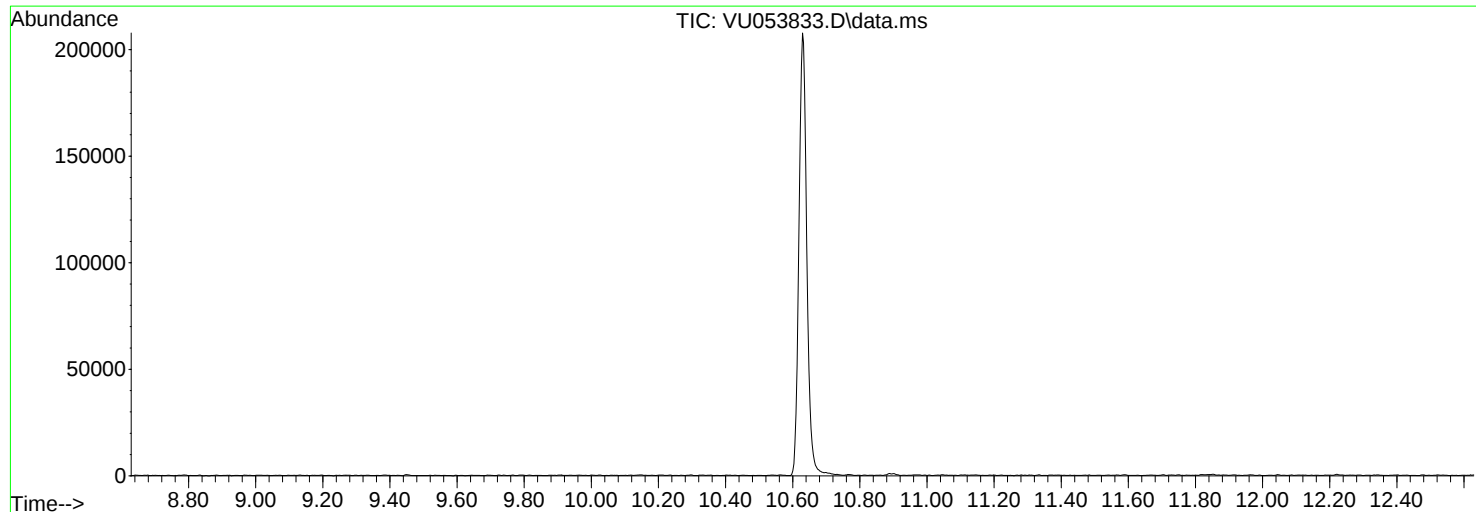

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7096	PASS
75	95	30	80	49.7	21168	PASS
95	95	100	100	100.0	42576	PASS
96	95	5	9	6.5	2748	PASS
173	174	0.00	2	0.6	206	PASS
174	95	50	120	79.8	33955	PASS
175	174	5	9	7.3	2481	PASS
176	174	95	101	95.7	32501	PASS
177	176	5	9	6.6	2135	PASS

m/z	Abundance
44.10	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.20	312.0
37.10	1805.0
38.00	1132.0
39.10	652.0
40.10	175.0
44.00	434.0
45.00	334.0
47.20	639.0
48.00	195.0
49.00	1359.0
50.10	6654.0
51.10	2046.0
56.00	634.0
57.10	945.0
60.00	458.0
61.10	1745.0
62.10	1662.0
63.20	1871.0
64.30	218.0
65.00	187.0
68.10	3594.0
69.10	4342.0
70.10	338.0
72.10	318.0
73.00	1810.0
74.10	6719.0
75.10	20912.0
76.10	1767.0
77.00	156.0
77.90	178.0
79.00	1528.0
80.00	411.0
81.00	1824.0
82.10	246.0
87.00	1902.0
88.10	1723.0
90.90	119.0
92.10	1145.0
93.10	1797.0
94.10	4660.0
95.10	41032.0
96.10	2717.0
97.00	107.0
103.90	161.0
106.00	265.0
115.90	209.0
116.90	224.0
118.90	234.0
129.90	107.0
140.90	408.0
143.00	470.0
144.80	123.0
148.00	109.0
154.90	145.0
172.10	244.0
173.10	195.0
174.10	31864.0
175.10	2299.0
176.10	30440.0
177.00	2072.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.10	298.0
37.10	1770.0
38.00	1282.0
39.10	701.0
40.10	136.0
44.00	452.0
45.00	380.0
47.20	627.0
48.00	251.0
49.00	1532.0
50.10	7335.0
51.10	2131.0
52.10	111.0
55.10	103.0
56.00	550.0
57.10	1102.0
60.00	460.0
61.10	1911.0
62.10	1819.0
63.10	1952.0
64.10	170.0
65.00	187.0
67.00	106.0
68.10	4076.0
69.10	4563.0
70.10	319.0
72.10	310.0
73.00	1932.0
74.10	7293.0
75.10	21816.0
76.00	1747.0
77.00	262.0
77.90	229.0
79.00	1698.0
80.00	470.0
81.00	1883.0
82.00	305.0
87.00	1867.0
88.00	1888.0
91.00	142.0
92.10	1264.0
93.10	1852.0
94.10	4855.0
95.10	44128.0
96.10	2852.0
103.90	174.0
106.00	259.0
115.90	213.0
116.90	228.0
118.00	117.0
118.90	254.0
127.90	113.0
130.00	159.0
140.90	419.0
142.90	514.0
144.90	114.0
148.00	117.0
154.90	150.0
172.00	291.0
173.00	203.0
174.10	34992.0
175.10	2592.0
176.10	33496.0
177.00	2204.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
36.10	214.0
37.10	1589.0
38.00	1295.0
39.10	723.0
40.00	115.0
44.00	388.0
45.00	377.0
47.10	521.0
48.00	230.0
49.10	1595.0
50.10	7300.0
51.10	2114.0
52.20	137.0
55.00	109.0
56.00	458.0
57.10	1189.0
60.00	395.0
61.10	1916.0
62.10	1799.0
63.10	1734.0
64.00	130.0
65.10	215.0
67.00	136.0
68.10	4317.0
69.10	4320.0
70.10	294.0
72.20	246.0
73.10	1761.0
74.10	7176.0
75.10	20776.0
76.10	1775.0
77.00	352.0
78.00	244.0
78.90	1618.0
80.00	462.0
81.00	1723.0
82.00	349.0
87.10	1634.0
88.00	1841.0
91.00	183.0
92.10	1243.0
93.10	1713.0
94.10	4699.0
95.10	42568.0
96.10	2675.0
103.90	224.0
106.00	192.0
116.00	191.0
116.80	253.0
118.00	142.0
118.90	232.0
127.90	168.0
130.00	179.0
141.00	426.0
142.90	467.0
147.90	113.0
154.90	124.0
172.00	348.0
172.90	219.0
174.10	35008.0
175.10	2553.0
176.10	33568.0
177.00	2130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007