


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042519\
Data File : VU031492.D
Acq On : 25 Apr 2019 08:37
Operator : JC/SP
Sample : BFB04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB04

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
Title : TRACE VOA SOM01.0
Last Update : Fri Apr 26 01:33:16 2019

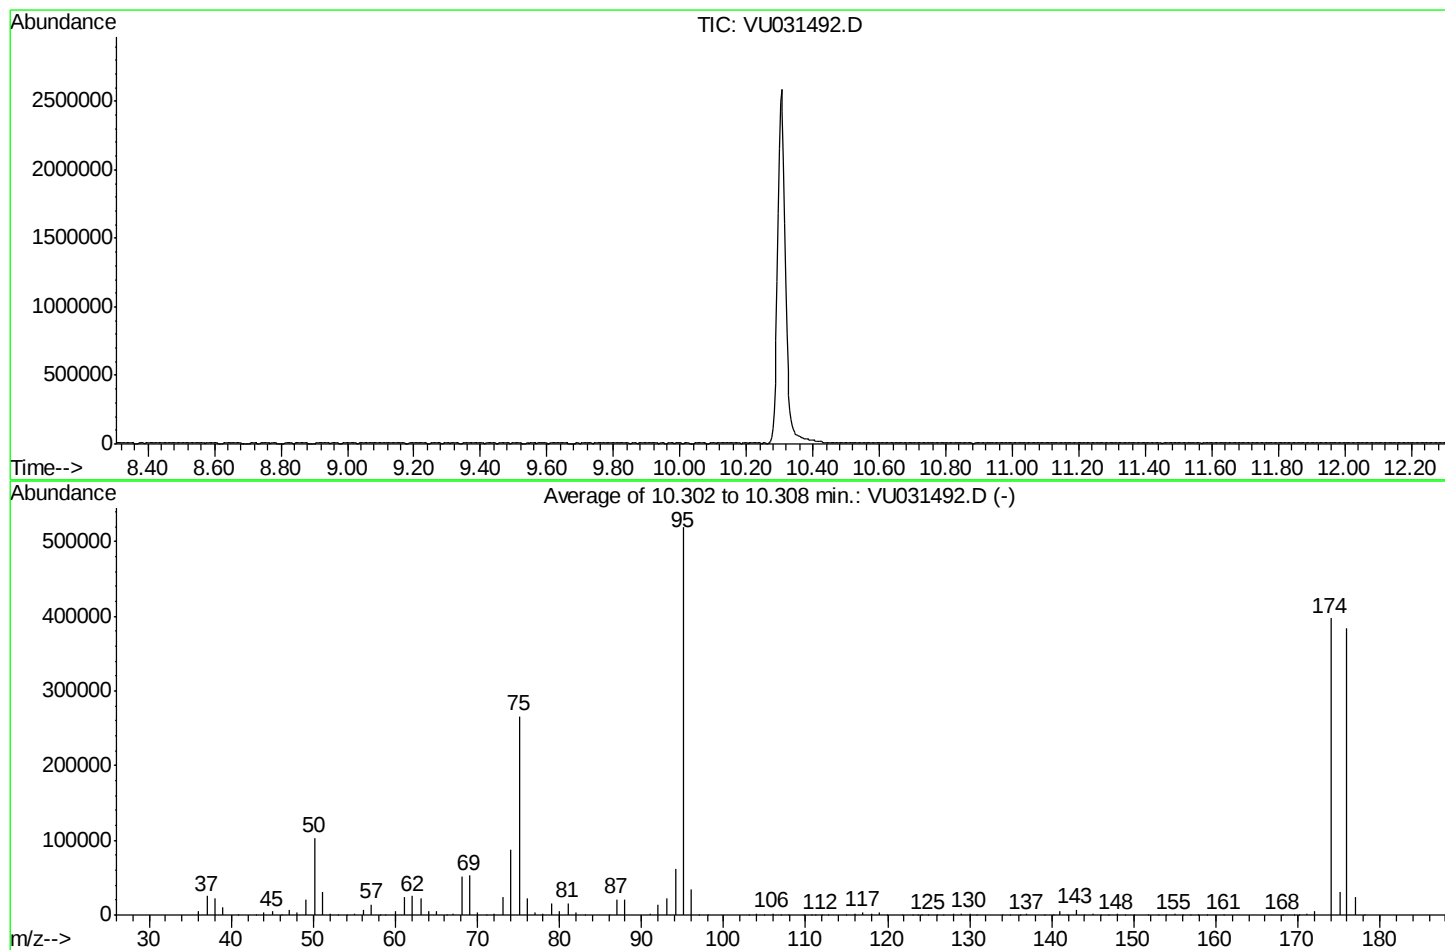

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	103208	PASS
75	95	30	80	51.3	266154	PASS
95	95	100	100	100.0	519168	PASS
96	95	5	9	6.6	34248	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.6	397632	PASS
175	174	5	9	7.6	30154	PASS
176	174	95	101	96.7	384533	PASS
177	176	5	9	6.3	24098	PASS

Scan 2851 (10.257 min): VU031492.D
BFB04

m/z	Abundance
39.00	202.0
40.00	4296.0
44.00	838.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	4980.0
37.00	25784.0
38.00	23024.0
39.00	10709.0
40.00	4217.0
43.10	241.0
44.00	3693.0
45.00	5233.0
46.10	1098.0
47.00	6907.0
48.00	3762.0
49.10	21616.0
50.10	105400.0
51.10	31248.0
52.10	1868.0
53.00	809.0
54.00	397.0
55.00	1265.0
56.00	6901.0
57.10	13529.0
58.10	542.0
58.80	134.0
60.10	5693.0
61.10	25224.0
62.10	25568.0
63.10	21840.0
64.10	4955.0
65.00	4666.0
66.20	747.0
67.00	1491.0
68.10	51552.0
69.10	52800.0
70.10	3983.0
71.00	238.0
72.10	2570.0
73.10	23896.0
74.10	87768.0
75.10	268544.0
76.10	22096.0
77.00	3074.0
78.00	2182.0
79.00	16976.0
80.00	4018.0
81.00	16141.0
82.00	3859.0
83.20	308.0
86.10	702.0
87.00	20912.0
88.00	20448.0
91.00	1934.0
92.00	14166.0
93.10	22384.0
94.10	60088.0
95.10	519232.0
96.10	34912.0
97.00	878.0
98.00	101.0
103.10	294.0
104.00	1877.0
105.00	622.0
106.00	2182.0
106.90	396.0
107.90	494.0
109.80	268.0
110.70	263.0
111.90	341.0
112.80	422.0
115.00	581.0
116.00	1792.0
117.00	3705.0
118.00	1745.0
119.00	3279.0
119.90	104.0
123.20	116.0
124.10	170.0
124.90	210.0
126.10	226.0
126.80	152.0
128.00	1696.0
129.00	1006.0
130.00	1852.0
130.90	765.0
134.00	108.0
134.90	731.0
136.10	104.0
137.00	1039.0
139.10	145.0
140.10	319.0
141.00	4807.0
141.90	780.0
143.00	7642.0
144.00	604.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

145.00	2879.0
146.00	922.0
146.90	282.0
148.00	1226.0
148.90	531.0
150.00	522.0
151.80	310.0
153.00	266.0
153.90	339.0
155.00	1323.0
155.90	212.0
156.90	752.0
157.90	132.0
158.90	558.0
161.00	599.0
168.20	131.0
169.60	128.0
170.10	130.0
171.10	1326.0
172.10	6177.0
174.00	386048.0
175.10	30856.0
176.00	372864.0
177.00	24600.0
178.10	563.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	5130.0
37.00	26096.0
38.00	23280.0
39.00	10181.0
40.00	4337.0
40.80	214.0
43.10	275.0
44.00	3872.0
45.00	5186.0
46.10	892.0
47.00	7021.0
48.00	3756.0
49.10	22048.0
50.10	107048.0
51.10	31472.0
52.10	1820.0
53.00	768.0
54.00	259.0
54.90	1211.0
56.00	7121.0
57.10	14202.0
58.10	517.0
58.80	183.0
60.10	5232.0
61.10	25688.0
62.10	26144.0
63.10	22656.0
64.10	4552.0
65.10	4756.0
66.20	840.0
67.00	1717.0
68.00	52832.0
69.10	54896.0
70.10	3736.0
71.10	201.0
72.10	2703.0
73.10	24080.0
74.10	90752.0
75.10	275520.0
76.10	22696.0
77.00	3114.0
78.00	2259.0
79.00	16664.0
80.00	4608.0
81.00	16369.0
82.00	3847.0
83.10	379.0
86.10	779.0
87.00	21912.0
88.00	21096.0
91.00	2041.0
92.00	14867.0
93.10	23304.0
94.10	63328.0
95.10	536640.0
96.10	35256.0
97.00	803.0
103.10	268.0
104.00	1983.0
105.00	616.0
106.00	2388.0
107.00	534.0
108.00	367.0
109.80	307.0
111.20	315.0
111.90	400.0
112.80	361.0
115.00	508.0
116.00	1946.0
117.00	3670.0
118.00	1839.0
119.00	3108.0
121.80	100.0
123.10	130.0
123.70	192.0
125.00	219.0
126.10	197.0
126.80	168.0
128.00	1906.0
129.00	1170.0
130.00	1904.0
130.90	706.0
135.00	754.0
137.00	1028.0
139.10	237.0
140.20	373.0
141.00	5201.0
141.90	846.0
143.00	7811.0
144.00	642.0
145.00	2623.0
146.00	912.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

146.90	352.0
148.00	1332.0
148.90	502.0
150.00	602.0
151.80	345.0
153.00	330.0
153.90	406.0
155.00	1362.0
155.90	200.0
156.90	888.0
157.90	193.0
158.90	638.0
161.00	594.0
168.10	158.0
169.60	130.0
170.10	167.0
171.10	1360.0
172.10	6160.0
174.00	410944.0
175.10	31112.0
176.00	398592.0
177.00	24864.0
178.10	734.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

m/z	Abundance
36.00	4796.0
37.00	23104.0
38.00	20864.0
39.10	8953.0
40.00	4321.0
40.80	309.0
43.00	346.0
44.00	3547.0
45.00	4573.0
46.10	719.0
47.00	6473.0
48.00	3263.0
49.10	20248.0
50.10	97176.0
51.10	28432.0
52.10	1522.0
53.00	695.0
53.90	132.0
54.90	1104.0
56.10	6531.0
57.10	13560.0
58.10	358.0
58.80	156.0
60.00	4172.0
61.10	23560.0
62.10	24288.0
63.10	20944.0
64.10	3649.0
65.10	4490.0
66.20	772.0
67.00	1664.0
68.00	49080.0
69.00	51712.0
70.00	3124.0
72.00	2634.0
73.10	21920.0
74.10	84976.0
75.10	254400.0
76.10	21168.0
77.00	2922.0
78.00	1911.0
79.00	14994.0
80.00	4654.0
81.00	15327.0
82.00	3530.0
83.00	431.0
86.10	768.0
87.00	20728.0
88.00	20152.0
91.00	1971.0
92.00	13701.0
93.10	22048.0
94.10	60088.0
95.10	501632.0
96.10	32576.0
97.10	717.0
103.10	219.0
103.90	1997.0
105.00	522.0
106.00	2269.0
107.00	521.0
108.00	275.0
109.80	346.0
111.10	401.0
111.90	372.0
112.80	307.0
115.10	349.0
116.00	1784.0
117.00	3354.0
118.00	1841.0
118.90	2867.0
121.80	108.0
123.00	154.0
123.70	161.0
125.00	175.0
126.00	157.0
126.90	138.0
128.00	1688.0
129.00	1200.0
130.00	1754.0
130.90	631.0
135.00	726.0
136.90	932.0
139.00	269.0
141.00	4697.0
141.90	725.0
143.00	7300.0
144.00	580.0
145.00	2195.0
146.00	802.0
147.00	351.0
148.00	1274.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04

148.90	322.0
150.00	540.0
151.80	242.0
153.00	288.0
153.90	465.0
155.00	1369.0
155.90	174.0
157.00	1015.0
157.90	249.0
159.00	591.0
160.80	446.0
161.10	445.0
168.10	133.0
169.60	104.0
170.10	164.0
171.10	1158.0
172.10	5718.0
174.00	395904.0
175.10	28496.0
176.00	382144.0
177.00	22832.0
178.10	698.0

Instrument :
MSVOA_U
ClientSampleId :
BFB04