

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048267.D
 Acq On : 25 Apr 2022 14:29
 Operator : SY/MD
 Sample : VU0425WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	51	rBV5	4968	7134	0.41%	0.053%
2	1.601	73	81	100	rBV	192043	254140	14.71%	1.900%
3	1.884	162	169	191	rVB	132979	212862	12.32%	1.592%
4	2.559	366	379	396	rBV	347303	577148	33.41%	4.315%
5	2.681	413	417	422	rVB3	393	335	0.02%	0.003%
6	2.723	425	430	432	rBV2	605	569	0.03%	0.004%
7	2.794	441	452	459	rBV6	1257	2927	0.17%	0.022%
8	2.845	465	468	474	rVB2	599	546	0.03%	0.004%
9	3.044	521	530	539	rBV4	2173	3975	0.23%	0.030%
10	3.138	555	559	560	rBV	439	309	0.02%	0.002%
11	3.186	561	574	585	rBV2	9787	21959	1.27%	0.164%
12	3.440	650	653	655	rBV	332	245	0.01%	0.002%
13	3.491	665	669	672	rVB2	358	261	0.02%	0.002%
14	3.581	693	697	704	rBV2	317	324	0.02%	0.002%
15	3.935	805	807	811	rVB2	315	223	0.01%	0.002%
16	4.144	869	872	882	rVB2	211	282	0.02%	0.002%
17	4.494	977	981	985	rBV2	296	208	0.01%	0.002%
18	4.620	1007	1020	1059	rBV	200042	505139	29.24%	3.777%
19	5.064	1141	1158	1181	rBV	305573	664883	38.49%	4.971%
20	5.195	1196	1199	1201	rBV	344	217	0.01%	0.002%
21	5.208	1201	1203	1208	rVB3	415	333	0.02%	0.002%
22	5.276	1222	1224	1226	rBV3	377	221	0.01%	0.002%
23	5.334	1233	1242	1245	rBV4	1313	2144	0.12%	0.016%
24	5.388	1257	1259	1264	rVB	350	219	0.01%	0.002%
25	5.501	1288	1294	1297	rBV2	209	207	0.01%	0.002%
26	5.723	1342	1363	1400	rBV2	643276	1727376	100.00%	12.916%
27	5.970	1435	1440	1445	rVV5	889	1172	0.07%	0.009%
28	6.031	1455	1459	1461	rBV2	310	235	0.01%	0.002%
29	6.247	1512	1526	1546	rBV	407284	773954	44.81%	5.787%
30	6.385	1566	1569	1572	rBV3	390	326	0.02%	0.002%
31	6.523	1605	1612	1613	rBV3	1788	1527	0.09%	0.011%
32	6.613	1638	1640	1644	rVB3	594	310	0.02%	0.002%
33	6.690	1649	1664	1688	rBV	399401	780736	45.20%	5.838%
34	6.954	1742	1746	1749	rBV	454	288	0.02%	0.002%
35	7.047	1769	1775	1776	rBV3	608	540	0.03%	0.004%
36	7.092	1785	1789	1791	rBV	320	295	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048267.D
 Acq On : 25 Apr 2022 14:29
 Operator : SY/MD
 Sample : VU0425WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	7.176	1804	1815	1833	rVV5	5482	12470	0.72%	0.093%
38	7.407	1884	1887	1893	rVB2	308	309	0.02%	0.002%
39	7.565	1920	1936	1961	rBV	214443	373910	21.65%	2.796%
40	7.658	1962	1965	1967	rBV2	324	234	0.01%	0.002%
41	7.687	1969	1974	1982	rVB4	2010	2956	0.17%	0.022%
42	7.800	1999	2009	2020	rBV6	3227	5457	0.32%	0.041%
43	7.896	2026	2039	2055	rBV	773367	1342062	77.69%	10.035%
44	8.179	2112	2127	2147	rBV	153596	257042	14.88%	1.922%
45	8.411	2197	2199	2203	rVV2	445	286	0.02%	0.002%
46	8.481	2211	2221	2225	rVB4	476	797	0.05%	0.006%
47	8.523	2231	2234	2237	rVB2	356	226	0.01%	0.002%
48	8.552	2237	2243	2245	rBV3	402	440	0.03%	0.003%
49	8.636	2256	2269	2302	rBV	657365	1237820	71.66%	9.255%
50	8.845	2332	2334	2339	rVB4	401	254	0.01%	0.002%
51	8.883	2342	2346	2352	rVB3	369	398	0.02%	0.003%
52	8.938	2358	2363	2366	rBB3	281	244	0.01%	0.002%
53	9.015	2384	2387	2393	rBV2	287	215	0.01%	0.002%
54	9.099	2410	2413	2418	rVB	324	233	0.01%	0.002%
55	9.157	2429	2431	2435	rBV3	285	267	0.02%	0.002%
56	9.218	2447	2450	2453	rVB2	384	224	0.01%	0.002%
57	9.237	2453	2456	2461	rVB3	313	244	0.01%	0.002%
58	9.417	2499	2512	2544	rBV	629458	1050659	60.82%	7.856%
59	9.571	2554	2560	2567	rBV5	1117	1569	0.09%	0.012%
60	9.639	2577	2581	2589	rVB3	257	296	0.02%	0.002%
61	9.674	2589	2592	2593	rBV	598	306	0.02%	0.002%
62	9.700	2593	2600	2605	rVB3	1507	2107	0.12%	0.016%
63	9.793	2627	2629	2634	rVB	298	214	0.01%	0.002%
64	9.867	2648	2652	2655	rBV2	424	279	0.02%	0.002%
65	9.906	2658	2664	2668	rVB2	305	332	0.02%	0.002%
66	10.005	2690	2695	2697	rBV	250	243	0.01%	0.002%
67	10.105	2720	2726	2737	rVB6	1458	2486	0.14%	0.019%
68	10.160	2737	2743	2744	rBV	267	210	0.01%	0.002%
69	10.208	2756	2758	2765	rVB2	267	238	0.01%	0.002%
70	10.372	2805	2809	2812	rBV2	312	253	0.01%	0.002%
71	10.488	2838	2845	2856	rVB4	1080	1722	0.10%	0.013%
72	10.642	2888	2893	2895	rVV2	519	555	0.03%	0.004%
73	10.671	2896	2902	2910	rVB3	3336	4652	0.27%	0.035%
74	10.758	2916	2929	2947	rBV	706410	1132955	65.59%	8.471%
75	10.867	2959	2963	2966	rBV3	801	645	0.04%	0.005%
76	10.922	2978	2980	2985	rVB2	489	271	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048267.D
 Acq On : 25 Apr 2022 14:29
 Operator : SY/MD
 Sample : VU0425WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK111

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.092	3028	3033	3038	rVV3	840	819	0.05%	0.006%
78	11.211	3066	3070	3072	rBV2	296	224	0.01%	0.002%
79	11.468	3138	3150	3160	rBV5	3418	6658	0.39%	0.050%
80	11.549	3172	3175	3179	rVB2	348	220	0.01%	0.002%
81	11.693	3215	3220	3226	rVB4	1430	1559	0.09%	0.012%
82	11.748	3231	3237	3245	rVB2	1975	2743	0.16%	0.021%
83	11.812	3245	3257	3283	rBV	641150	1016796	58.86%	7.603%
84	12.047	3327	3330	3336	rBV3	416	488	0.03%	0.004%
85	12.195	3361	3376	3394	rBV	806340	1314855	76.12%	9.831%
86	12.439	3449	3452	3455	rVB2	341	253	0.01%	0.002%
87	12.459	3455	3458	3462	rVB3	322	236	0.01%	0.002%
88	12.488	3462	3467	3468	rBV2	382	331	0.02%	0.002%
89	12.639	3511	3514	3522	rVB3	509	454	0.03%	0.003%
90	12.745	3544	3547	3550	rBV2	296	284	0.02%	0.002%
91	12.771	3550	3555	3560	rBV2	992	1278	0.07%	0.010%
92	12.906	3593	3597	3600	rBV	403	394	0.02%	0.003%
93	13.002	3623	3627	3632	rBV6	755	771	0.04%	0.006%
94	13.221	3689	3695	3705	rBV5	2787	4558	0.26%	0.034%
95	13.848	3881	3890	3899	rBV2	5884	9284	0.54%	0.069%
96	13.928	3912	3915	3916	rBV	420	240	0.01%	0.002%
97	14.092	3957	3966	3978	rBV	13220	20534	1.19%	0.154%
98	14.333	4033	4041	4054	rVB3	6854	10778	0.62%	0.081%
99	15.057	4263	4266	4267	rBV2	579	336	0.02%	0.003%
100	15.471	4393	4395	4396	rBV	659	286	0.02%	0.002%




Sum of corrected areas: 13374028

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048267.D
Acq On : 25 Apr 2022 14:29
Operator : SY/MD
Sample : VU0425WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

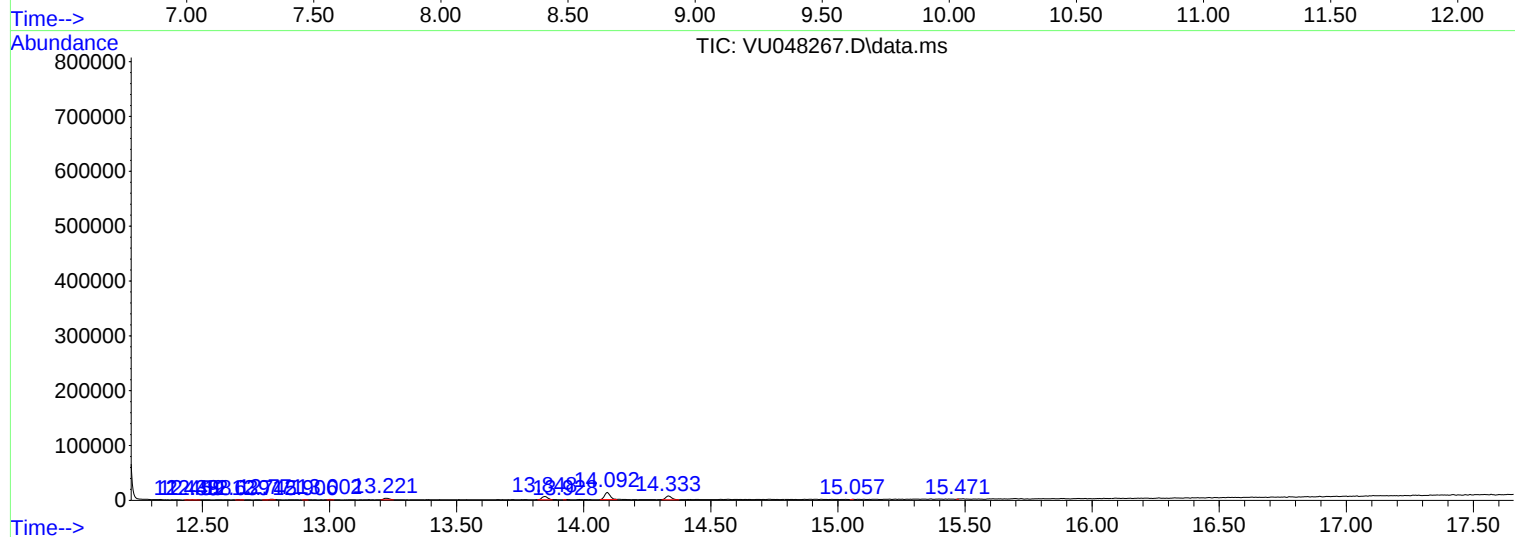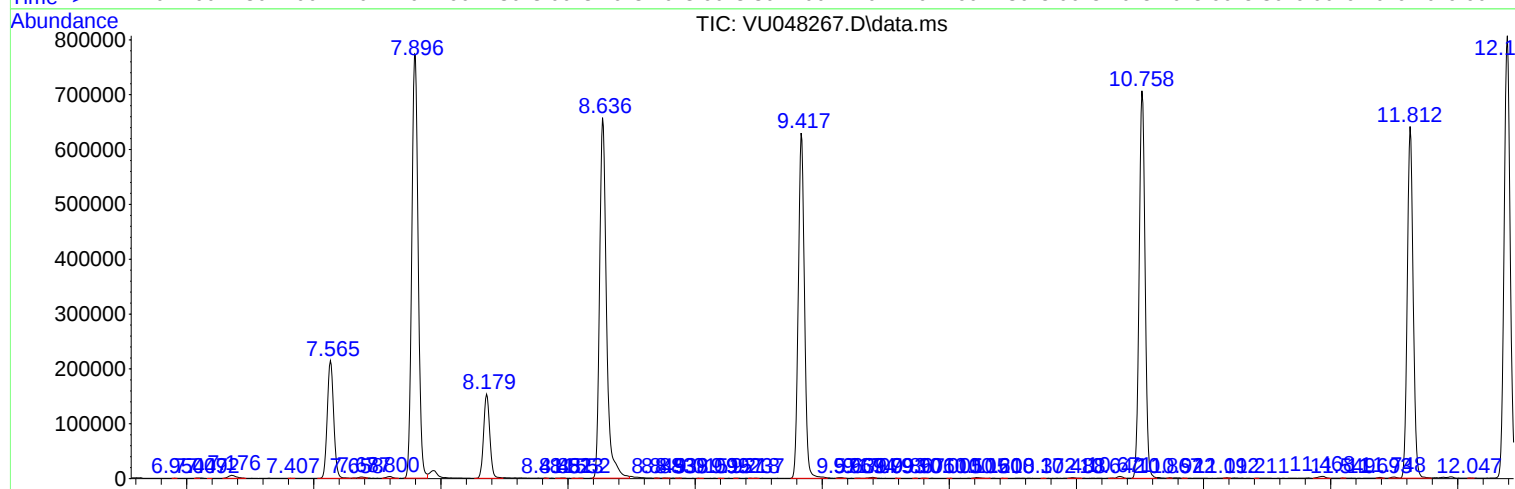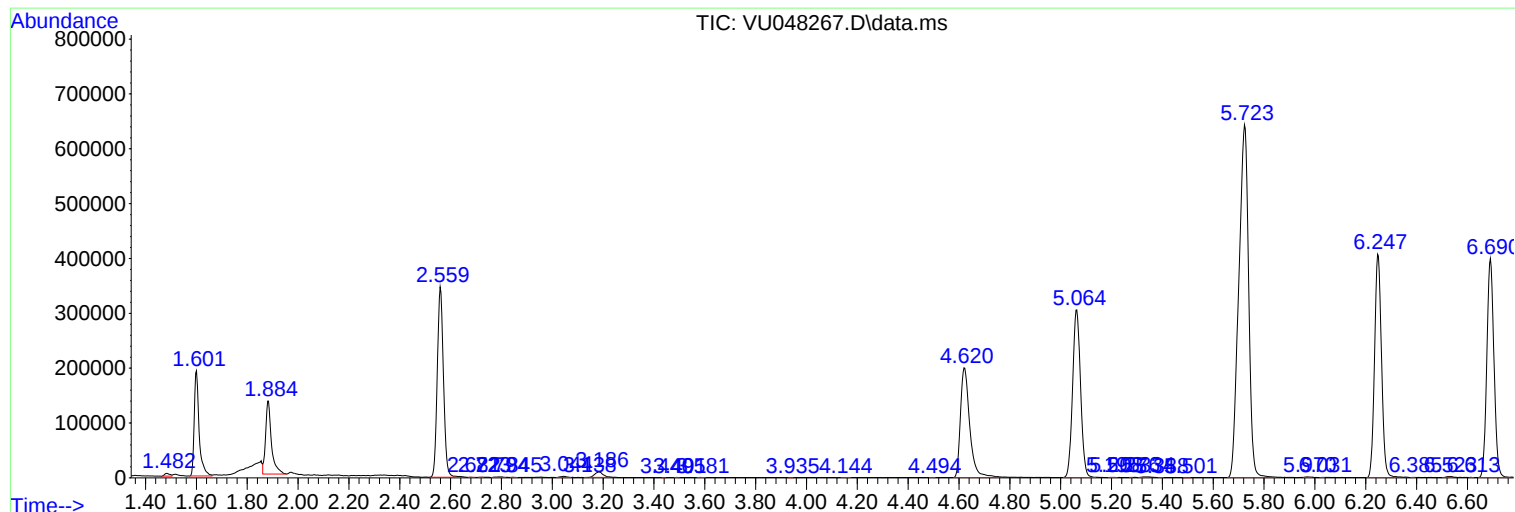

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048267.D
Acq On : 25 Apr 2022 14:29
Operator : SY/MD
Sample : VU0425WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048267.D
Acq On : 25 Apr 2022 14:29
Operator : SY/MD
Sample : VU0425WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK111

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------