

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048272.D
 Acq On : 25 Apr 2022 16:52
 Operator : SY/MD
 Sample : VIBLK067
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048272.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	39	44	51	rBV3	5719	8450	0.47%	0.061%
2	1.601	73	81	101	rBV	197416	256185	14.38%	1.855%
3	1.880	162	168	194	rVB	141793	232812	13.06%	1.686%
4	2.559	367	379	395	rBV	350508	588115	33.00%	4.258%
5	2.720	426	429	433	rBV4	465	392	0.02%	0.003%
6	2.787	444	450	455	rBV2	1738	2216	0.12%	0.016%
7	2.916	487	490	492	rVB2	311	207	0.01%	0.001%
8	2.938	492	497	498	rBV3	446	331	0.02%	0.002%
9	3.044	519	530	549	rBV2	12549	26706	1.50%	0.193%
10	3.183	560	573	591	rBV	12672	29439	1.65%	0.213%
11	3.292	603	607	610	rBV	530	343	0.02%	0.002%
12	3.346	621	624	626	rBV4	661	449	0.03%	0.003%
13	3.475	660	664	665	rBV2	364	268	0.02%	0.002%
14	3.520	675	678	681	rBV	359	270	0.02%	0.002%
15	3.674	717	726	727	rBV3	453	560	0.03%	0.004%
16	3.739	742	746	753	rVB2	579	576	0.03%	0.004%
17	3.784	753	760	764	rBV	239	301	0.02%	0.002%
18	3.819	769	771	774	rVB2	333	204	0.01%	0.001%
19	3.941	804	809	814	rVB3	363	382	0.02%	0.003%
20	4.083	849	853	858	rVB2	290	235	0.01%	0.002%
21	4.170	876	880	888	rVB3	316	316	0.02%	0.002%
22	4.337	929	932	937	rVV2	225	208	0.01%	0.002%
23	4.363	938	940	952	rVB2	406	541	0.03%	0.004%
24	4.411	952	955	958	rBV2	351	289	0.02%	0.002%
25	4.517	984	988	991	rBV2	281	255	0.01%	0.002%
26	4.620	1006	1020	1062	rBV	205576	527086	29.58%	3.816%
27	4.819	1079	1082	1089	rVB3	512	493	0.03%	0.004%
28	4.980	1130	1132	1139	rVB2	363	298	0.02%	0.002%
29	5.060	1139	1157	1178	rBV	315952	691939	38.83%	5.010%
30	5.285	1223	1227	1228	rBV	577	387	0.02%	0.003%
31	5.340	1235	1244	1258	rVB5	1562	3820	0.21%	0.028%
32	5.523	1296	1301	1302	rBV	313	220	0.01%	0.002%
33	5.533	1302	1304	1307	rVB	404	198	0.01%	0.001%
34	5.723	1340	1363	1404	rBV2	661149	1782078	100.00%	12.902%
35	5.961	1432	1437	1438	rBV3	1153	860	0.05%	0.006%
36	6.041	1455	1462	1466	rBV4	579	670	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048272.D
 Acq On : 25 Apr 2022 16:52
 Operator : SY/MD
 Sample : VIBLK067
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.247	1511	1526	1554	rBV	424351	805839	45.22%	5.834%
38	6.494	1598	1603	1605	rBV3	293	247	0.01%	0.002%
39	6.536	1605	1616	1627	rVB7	2482	5212	0.29%	0.038%
40	6.578	1627	1629	1630	rBV7	575	261	0.01%	0.002%
41	6.597	1633	1635	1648	rVB6	883	1340	0.08%	0.010%
42	6.690	1649	1664	1692	rBV	418171	812989	45.62%	5.886%
43	6.806	1692	1700	1708	rVB4	1770	2775	0.16%	0.020%
44	6.848	1708	1713	1716	rBV3	347	367	0.02%	0.003%
45	6.948	1741	1744	1749	rBV	272	230	0.01%	0.002%
46	7.051	1772	1776	1780	rVB2	703	661	0.04%	0.005%
47	7.337	1861	1865	1869	rBV2	393	268	0.02%	0.002%
48	7.565	1923	1936	1963	rBV	219952	379431	21.29%	2.747%
49	7.690	1967	1975	1986	rVB3	2576	4522	0.25%	0.033%
50	7.751	1989	1994	1998	rBV3	200	236	0.01%	0.002%
51	7.800	1998	2009	2020	rVB4	4299	8229	0.46%	0.060%
52	7.848	2020	2024	2025	rBV2	395	227	0.01%	0.002%
53	7.899	2025	2040	2055	rBV	770636	1347002	75.59%	9.752%
54	8.179	2115	2127	2144	rBV	149556	250635	14.06%	1.815%
55	8.404	2193	2197	2203	rVV4	513	483	0.03%	0.003%
56	8.478	2218	2220	2227	rVB2	595	460	0.03%	0.003%
57	8.552	2239	2243	2248	rVB3	1269	1261	0.07%	0.009%
58	8.581	2248	2252	2256	rBV2	321	201	0.01%	0.001%
59	8.639	2256	2270	2301	rBV	653469	1255392	70.45%	9.089%
60	8.877	2339	2344	2350	rVB2	447	401	0.02%	0.003%
61	9.073	2402	2405	2408	rBV2	271	212	0.01%	0.002%
62	9.118	2414	2419	2422	rBV4	212	229	0.01%	0.002%
63	9.240	2453	2457	2460	rVB3	365	318	0.02%	0.002%
64	9.417	2498	2512	2534	rBV	638894	1073982	60.27%	7.775%
65	9.555	2552	2555	2556	rBV2	430	245	0.01%	0.002%
66	9.571	2557	2560	2568	rVB3	1737	1871	0.10%	0.014%
67	9.645	2580	2583	2586	rBV2	370	296	0.02%	0.002%
68	9.697	2590	2599	2610	rBV2	2970	4636	0.26%	0.034%
69	9.960	2674	2681	2682	rBV	175	213	0.01%	0.002%
70	9.999	2688	2693	2698	rBV2	416	401	0.02%	0.003%
71	10.111	2716	2728	2737	rVV5	3166	6062	0.34%	0.044%
72	10.292	2782	2784	2788	rBV2	342	240	0.01%	0.002%
73	10.488	2834	2845	2853	rBV3	2406	3730	0.21%	0.027%
74	10.603	2877	2881	2885	rBV2	320	248	0.01%	0.002%
75	10.671	2891	2902	2910	rBV3	3223	4707	0.26%	0.034%
76	10.758	2916	2929	2947	rBV	691036	1129333	63.37%	8.176%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048272.D
 Acq On : 25 Apr 2022 16:52
 Operator : SY/MD
 Sample : VIBLK067
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK067

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.867	2960	2963	2965	rBV4	403	288	0.02%	0.002%
78	10.899	2970	2973	2977	rVB3	1117	819	0.05%	0.006%
79	11.018	3008	3010	3014	rVB2	343	206	0.01%	0.001%
80	11.092	3026	3033	3036	rBV4	1548	1845	0.10%	0.013%
81	11.153	3050	3052	3056	rVB2	431	225	0.01%	0.002%
82	11.295	3093	3096	3098	rBV	360	207	0.01%	0.001%
83	11.468	3138	3150	3161	rBV4	6629	11957	0.67%	0.087%
84	11.581	3182	3185	3194	rVB4	673	659	0.04%	0.005%
85	11.693	3215	3220	3227	rVB4	1523	1746	0.10%	0.013%
86	11.745	3227	3236	3245	rBV3	5822	8891	0.50%	0.064%
87	11.812	3245	3257	3277	rBV	653597	1049485	58.89%	7.598%
88	11.970	3302	3306	3315	rVB5	2395	3556	0.20%	0.026%
89	12.195	3359	3376	3393	rBV	788854	1290564	72.42%	9.343%
90	12.359	3425	3427	3432	rBV4	358	354	0.02%	0.003%
91	12.693	3527	3531	3533	rBV2	235	204	0.01%	0.001%
92	12.771	3548	3555	3566	rBV4	1299	2372	0.13%	0.017%
93	13.002	3621	3627	3630	rBV	1555	1612	0.09%	0.012%
94	13.224	3687	3696	3705	rBV4	8707	13557	0.76%	0.098%
95	13.841	3878	3888	3898	rBV3	21651	33891	1.90%	0.245%
96	13.931	3910	3916	3919	rBV2	687	738	0.04%	0.005%
97	14.089	3955	3965	3981	rBV	51803	84881	4.76%	0.615%
98	14.330	4031	4040	4054	rVB2	25411	40105	2.25%	0.290%
99	14.581	4115	4118	4126	rBV3	527	550	0.03%	0.004%
100	14.635	4133	4135	4139	rBV2	499	296	0.02%	0.002%




Sum of corrected areas: 13812499

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048272.D
Acq On : 25 Apr 2022 16:52
Operator : SY/MD
Sample : VIBLK067
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

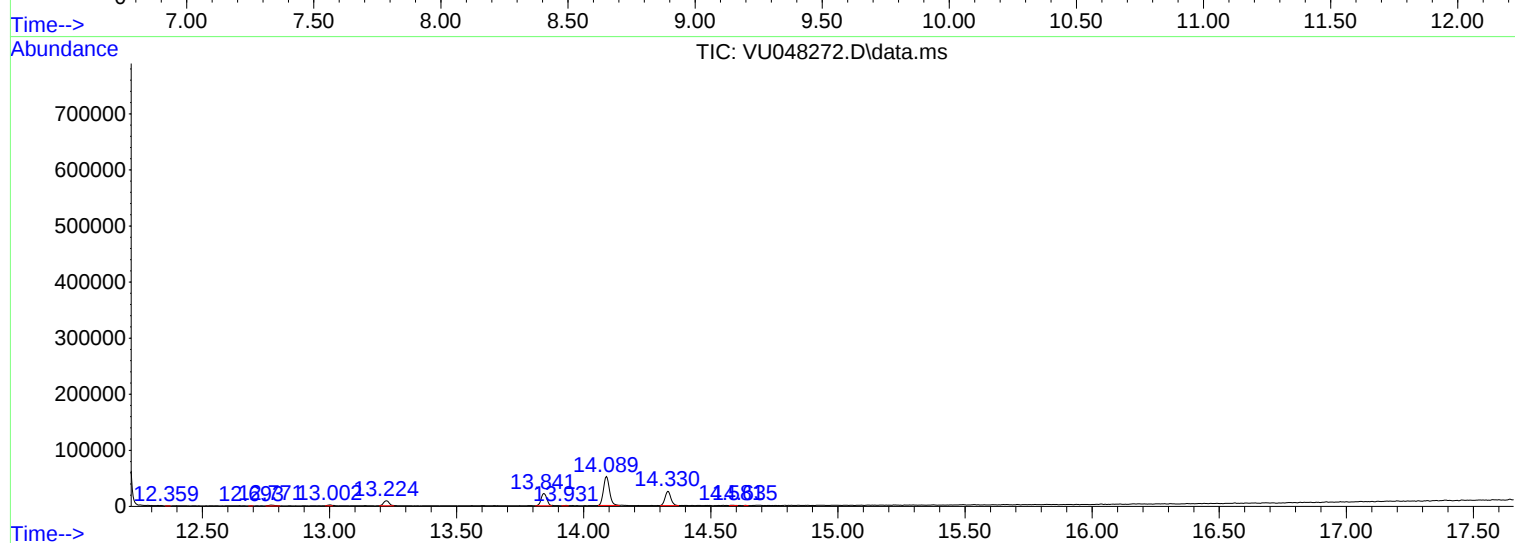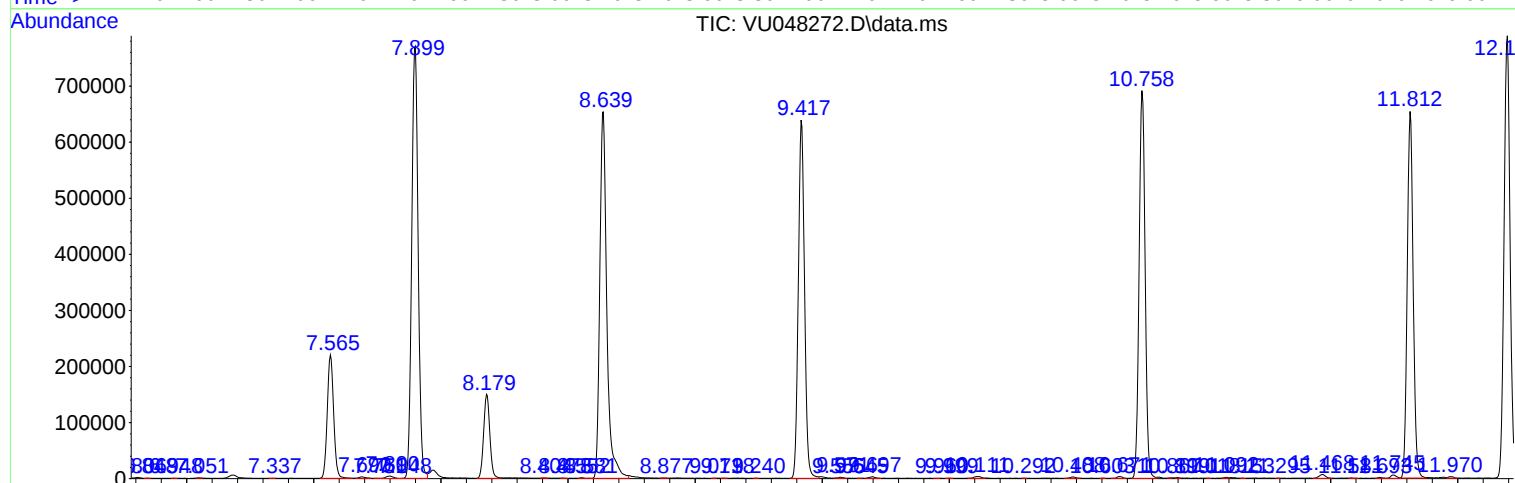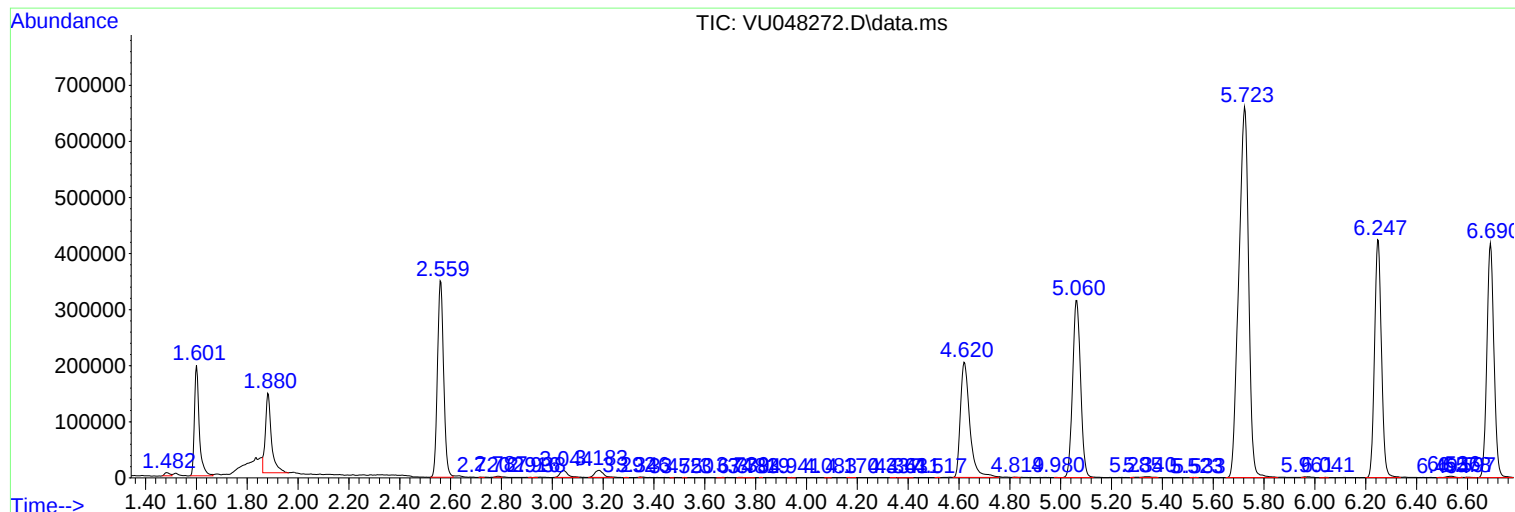

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048272.D
Acq On : 25 Apr 2022 16:52
Operator : SY/MD
Sample : VIBLK067
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048272.D
Acq On : 25 Apr 2022 16:52
Operator : SY/MD
Sample : VIBLK067
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK067

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------