

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048273.D
 Acq On : 25 Apr 2022 17:16
 Operator : SY/MD
 Sample : N2488-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048273.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	38	45	51	rBV4	6436	10010	0.57%	0.071%
2	1.601	73	81	101	rBV	189891	246722	14.15%	1.760%
3	1.880	162	168	190	rVB	133001	212593	12.19%	1.517%
4	2.559	367	379	396	rBV	354291	592574	33.98%	4.227%
5	2.768	440	444	445	rBV3	822	448	0.03%	0.003%
6	2.922	488	492	495	rBV2	346	282	0.02%	0.002%
7	2.948	495	500	501	rBV3	733	636	0.04%	0.005%
8	2.983	509	511	515	rVB	328	202	0.01%	0.001%
9	3.015	516	521	523	rBV2	375	381	0.02%	0.003%
10	3.083	539	542	547	rVB2	372	257	0.01%	0.002%
11	3.112	547	551	553	rBV2	307	282	0.02%	0.002%
12	3.183	559	573	590	rBV	16469	38254	2.19%	0.273%
13	3.350	618	625	627	rBV4	1158	1219	0.07%	0.009%
14	3.784	753	760	762	rVV2	233	270	0.02%	0.002%
15	3.797	762	764	769	rVB	441	273	0.02%	0.002%
16	3.906	796	798	802	rVB	311	229	0.01%	0.002%
17	3.941	802	809	813	rBV2	322	405	0.02%	0.003%
18	4.131	866	868	874	rVB3	282	243	0.01%	0.002%
19	4.176	874	882	885	rBV2	232	300	0.02%	0.002%
20	4.623	1007	1021	1043	rBV	194165	492283	28.23%	3.512%
21	5.064	1141	1158	1179	rBV	308733	683546	39.19%	4.876%
22	5.282	1221	1226	1227	rBV2	482	323	0.02%	0.002%
23	5.334	1235	1242	1251	rVB5	1756	2908	0.17%	0.021%
24	5.527	1292	1302	1307	rBV3	715	1102	0.06%	0.008%
25	5.723	1340	1363	1393	rBV2	641807	1743977	100.00%	12.442%
26	5.967	1432	1439	1456	rVB5	2559	5248	0.30%	0.037%
27	6.041	1456	1462	1467	rVB3	646	746	0.04%	0.005%
28	6.073	1467	1472	1476	rBV2	258	214	0.01%	0.002%
29	6.112	1477	1484	1490	rVB4	575	693	0.04%	0.005%
30	6.144	1490	1494	1496	rBV	419	290	0.02%	0.002%
31	6.247	1511	1526	1546	rBV	443071	840610	48.20%	5.997%
32	6.372	1562	1565	1568	rBV3	295	205	0.01%	0.001%
33	6.408	1574	1576	1582	rVB3	355	318	0.02%	0.002%
34	6.530	1606	1614	1616	rBV5	2201	2704	0.16%	0.019%
35	6.597	1631	1635	1646	rVB4	1794	2235	0.13%	0.016%
36	6.690	1647	1664	1682	rBV	406539	791902	45.41%	5.649%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048273.D
 Acq On : 25 Apr 2022 17:16
 Operator : SY/MD
 Sample : N2488-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.793	1692	1696	1698	rBV3	937	862	0.05%	0.006%
38	6.835	1708	1709	1715	rVB2	476	343	0.02%	0.002%
39	7.047	1766	1775	1781	rBV3	824	1088	0.06%	0.008%
40	7.105	1790	1793	1795	rBV2	383	262	0.02%	0.002%
41	7.179	1800	1816	1831	rBV3	5912	13190	0.76%	0.094%
42	7.321	1853	1860	1862	rBV2	220	270	0.02%	0.002%
43	7.420	1889	1891	1898	rVB3	412	349	0.02%	0.002%
44	7.469	1902	1906	1911	rBV2	230	217	0.01%	0.002%
45	7.565	1923	1936	1957	rBV	214826	380229	21.80%	2.713%
46	7.690	1967	1975	1986	rVB5	2341	4141	0.24%	0.030%
47	7.800	2001	2009	2019	rVB5	2090	3586	0.21%	0.026%
48	7.896	2023	2039	2055	rBV	796665	1380594	79.16%	9.849%
49	8.179	2115	2127	2145	rBV	151143	258300	14.81%	1.843%
50	8.472	2207	2218	2229	rBV2	12036	22049	1.26%	0.157%
51	8.559	2237	2245	2251	rVB7	1452	2067	0.12%	0.015%
52	8.639	2254	2270	2303	rBV	636864	1229241	70.48%	8.769%
53	8.919	2354	2357	2359	rBV	656	444	0.03%	0.003%
54	8.951	2365	2367	2375	rVB3	390	481	0.03%	0.003%
55	9.076	2402	2406	2408	rVB2	389	280	0.02%	0.002%
56	9.163	2428	2433	2439	rBV5	540	628	0.04%	0.004%
57	9.340	2486	2488	2491	rVB2	489	276	0.02%	0.002%
58	9.417	2499	2512	2540	rBV	638175	1152659	66.09%	8.223%
59	9.568	2555	2559	2566	rVB2	1906	2051	0.12%	0.015%
60	9.639	2578	2581	2587	rBV3	563	508	0.03%	0.004%
61	9.694	2590	2598	2608	rBV4	2805	4268	0.24%	0.030%
62	9.806	2631	2633	2637	rVB	336	233	0.01%	0.002%
63	10.102	2717	2725	2729	rBV4	2266	2924	0.17%	0.021%
64	10.295	2781	2785	2790	rBV2	401	434	0.02%	0.003%
65	10.375	2804	2810	2812	rBV	367	383	0.02%	0.003%
66	10.449	2830	2833	2837	rBV2	355	254	0.01%	0.002%
67	10.488	2837	2845	2853	rBV3	1817	2403	0.14%	0.017%
68	10.671	2892	2902	2909	rBV2	3529	4791	0.27%	0.034%
69	10.758	2915	2929	2949	rBV	707710	1136350	65.16%	8.107%
70	10.893	2959	2971	2987	rVB	21084	35430	2.03%	0.253%
71	11.063	3021	3024	3026	rBV2	340	261	0.01%	0.002%
72	11.092	3029	3033	3035	rVV	981	961	0.06%	0.007%
73	11.118	3039	3041	3049	rVB4	915	832	0.05%	0.006%
74	11.208	3066	3069	3072	rBV	425	262	0.02%	0.002%
75	11.308	3097	3100	3105	rVB2	303	273	0.02%	0.002%
76	11.420	3131	3135	3137	rVB2	592	415	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048273.D
 Acq On : 25 Apr 2022 17:16
 Operator : SY/MD
 Sample : N2488-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.465	3137	3149	3161	rBV7	4256	7738	0.44%	0.055%
78	11.571	3178	3182	3190	rVB3	688	668	0.04%	0.005%
79	11.645	3202	3205	3208	rVB3	386	277	0.02%	0.002%
80	11.697	3208	3221	3227	rBV5	1863	2919	0.17%	0.021%
81	11.748	3227	3237	3245	rBV	16856	26304	1.51%	0.188%
82	11.812	3245	3257	3281	rVB	646840	1116259	64.01%	7.963%
83	11.973	3302	3307	3319	rVB3	2930	4022	0.23%	0.029%
84	12.073	3324	3338	3343	rBV7	2025	3763	0.22%	0.027%
85	12.195	3361	3376	3398	rBV	803363	1374032	78.79%	9.802%
86	12.401	3438	3440	3443	rBV2	695	329	0.02%	0.002%
87	12.452	3451	3456	3460	rVB3	399	438	0.03%	0.003%
88	12.488	3465	3467	3475	rVB4	385	345	0.02%	0.002%
89	12.600	3499	3502	3508	rVB3	600	617	0.04%	0.004%
90	12.636	3508	3513	3517	rBV3	604	660	0.04%	0.005%
91	12.713	3532	3537	3543	rBV3	462	678	0.04%	0.005%
92	12.771	3547	3555	3566	rVB	8634	13763	0.79%	0.098%
93	12.999	3624	3626	3631	rVB4	485	361	0.02%	0.003%
94	13.221	3689	3695	3705	rVB5	4718	7293	0.42%	0.052%
95	13.529	3786	3791	3794	rBV2	441	435	0.02%	0.003%
96	13.841	3878	3888	3901	rBV2	44352	69254	3.97%	0.494%
97	14.089	3955	3965	3978	rBV	17141	29411	1.69%	0.210%
98	14.333	4030	4041	4055	rBV2	22622	37548	2.15%	0.268%
99	14.504	4092	4094	4095	rBV2	416	204	0.01%	0.001%
100	14.809	4187	4189	4193	rBV3	528	468	0.03%	0.003%




Sum of corrected areas: 14017259

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048273.D
Acq On : 25 Apr 2022 17:16
Operator : SY/MD
Sample : N2488-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

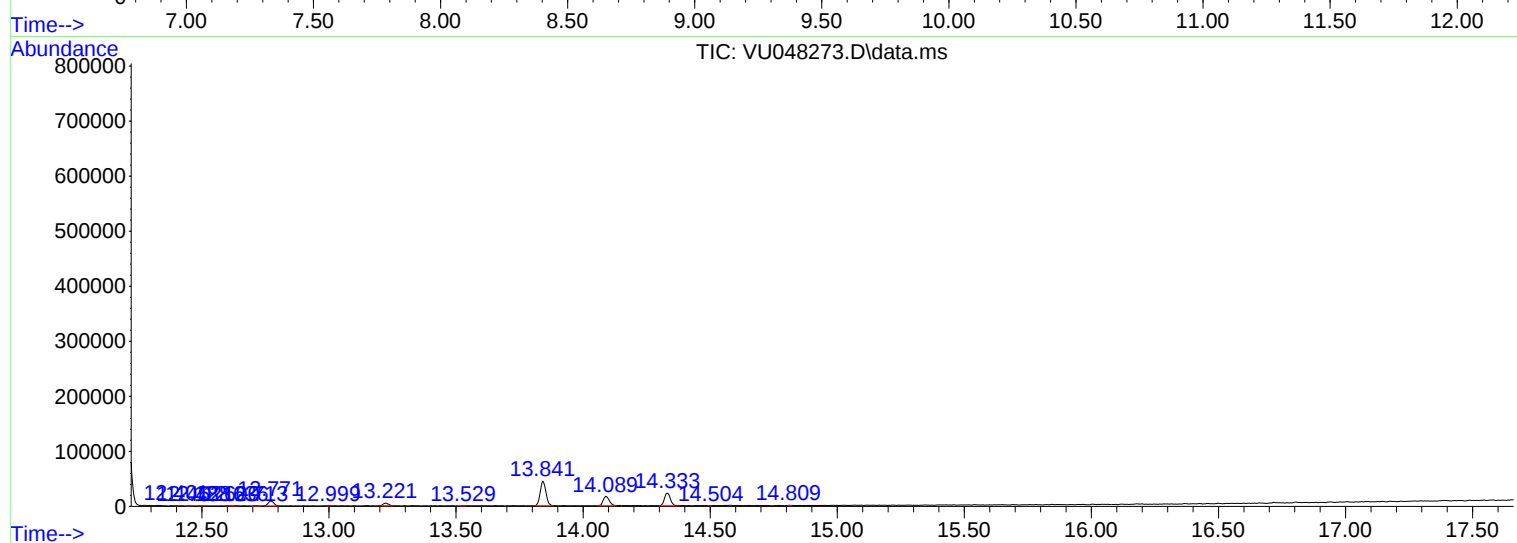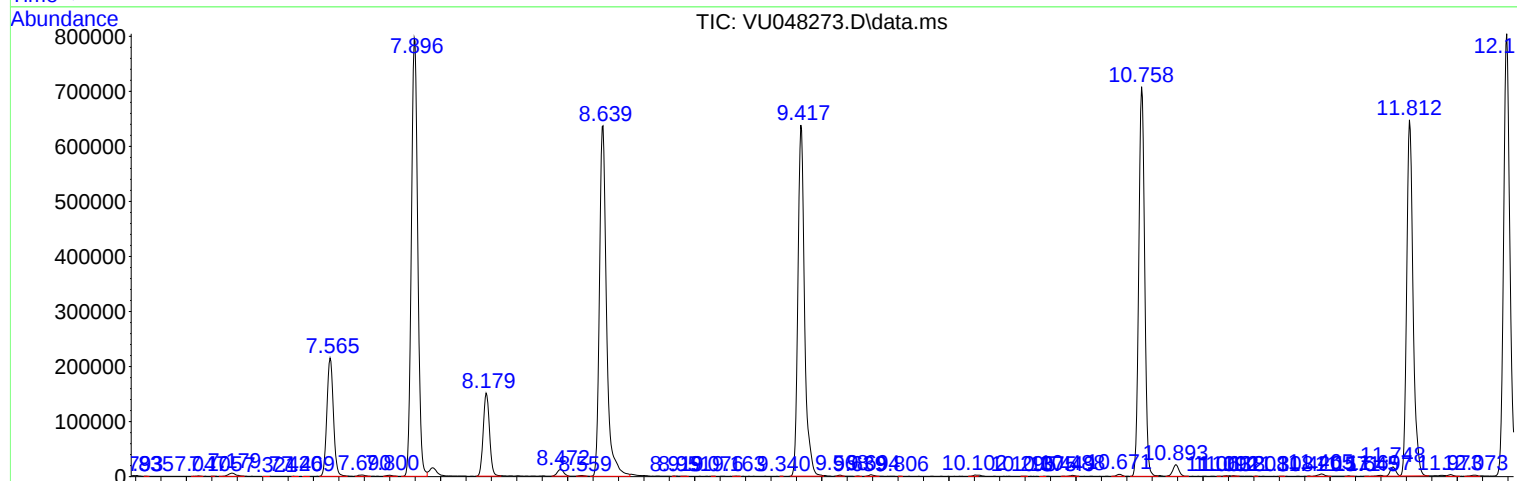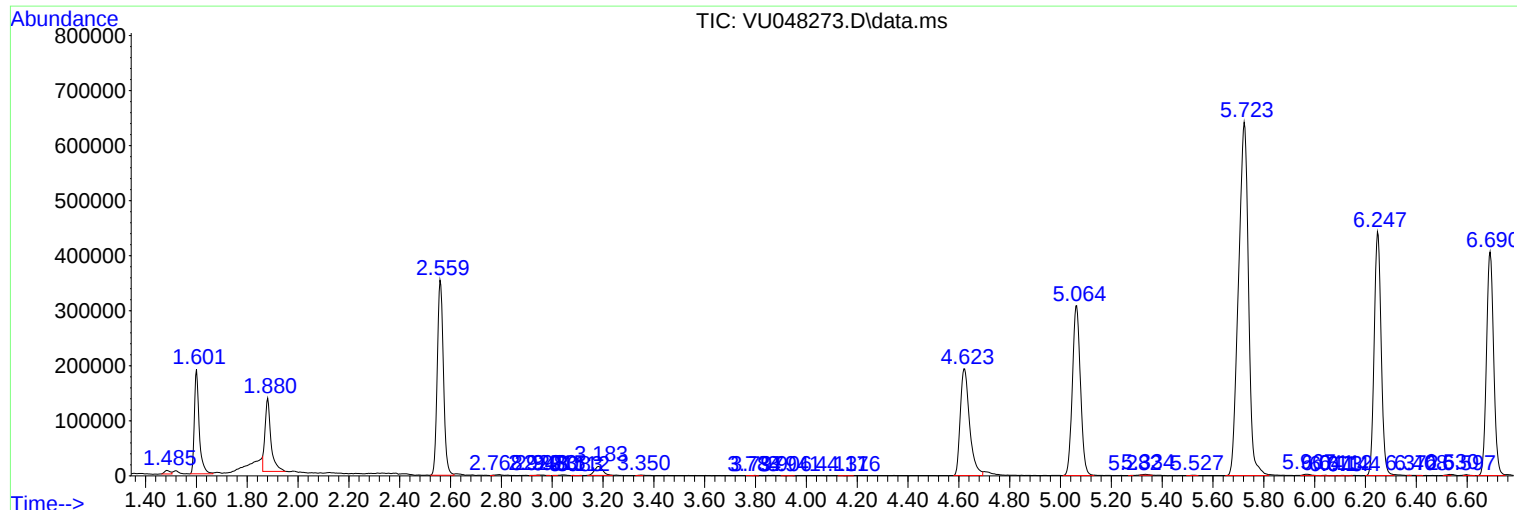

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048273.D
Acq On : 25 Apr 2022 17:16
Operator : SY/MD
Sample : N2488-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048273.D
Acq On : 25 Apr 2022 17:16
Operator : SY/MD
Sample : N2488-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------