

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048275.D
 Acq On : 25 Apr 2022 18:04
 Operator : SY/MD
 Sample : N2486-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048275.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	41	45	52	rVB3	4266	4279	0.24%	0.032%
2	1.601	73	81	100	rBV	205845	259764	14.69%	1.944%
3	1.896	165	173	186	rBV	140660	201061	11.37%	1.505%
4	2.562	368	380	399	rBV	356997	591862	33.46%	4.430%
5	2.729	429	432	434	rBV	424	304	0.02%	0.002%
6	2.774	444	446	448	rBV	404	224	0.01%	0.002%
7	2.938	495	497	499	rBV2	343	199	0.01%	0.001%
8	2.951	499	501	507	rVB3	452	372	0.02%	0.003%
9	3.044	520	530	538	rBV5	2321	3879	0.22%	0.029%
10	3.189	563	575	590	rVB2	3080	7446	0.42%	0.056%
11	3.600	699	703	708	rBV3	228	253	0.01%	0.002%
12	3.678	725	727	735	rBV	215	198	0.01%	0.001%
13	3.848	777	780	783	rBV	282	223	0.01%	0.002%
14	3.867	783	786	790	rVV2	244	217	0.01%	0.002%
15	4.031	834	837	842	rBV	239	280	0.02%	0.002%
16	4.099	852	858	861	rBV2	336	423	0.02%	0.003%
17	4.327	925	929	932	rVB2	274	255	0.01%	0.002%
18	4.346	932	935	937	rBV	272	217	0.01%	0.002%
19	4.504	980	984	989	rBV2	225	258	0.01%	0.002%
20	4.620	1006	1020	1047	rBV	211916	508596	28.75%	3.807%
21	4.851	1090	1092	1101	rVB2	312	258	0.01%	0.002%
22	5.063	1140	1158	1180	rBV	315635	681416	38.52%	5.101%
23	5.279	1222	1225	1227	rBV2	419	327	0.02%	0.002%
24	5.334	1234	1242	1251	rVB3	1820	2976	0.17%	0.022%
25	5.523	1296	1301	1306	rBV2	249	234	0.01%	0.002%
26	5.652	1337	1341	1342	rBV	258	203	0.01%	0.002%
27	5.726	1342	1364	1394	rVV2	655729	1768829	100.00%	13.241%
28	5.980	1435	1443	1449	rVB5	1008	1483	0.08%	0.011%
29	6.047	1462	1464	1469	rVB2	386	291	0.02%	0.002%
30	6.115	1481	1485	1492	rBV6	498	699	0.04%	0.005%
31	6.250	1512	1527	1557	rBV	448355	846717	47.87%	6.338%
32	6.465	1590	1594	1598	rVB2	395	351	0.02%	0.003%
33	6.491	1598	1602	1605	rBV2	377	301	0.02%	0.002%
34	6.530	1606	1614	1622	rVV7	1412	2584	0.15%	0.019%
35	6.575	1626	1628	1632	rBV3	431	268	0.02%	0.002%
36	6.690	1649	1664	1684	rBV	405724	795232	44.96%	5.953%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048275.D
 Acq On : 25 Apr 2022 18:04
 Operator : SY/MD
 Sample : N2486-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.806	1697	1700	1709	rVB5	1652	1892	0.11%	0.014%
38	6.890	1723	1726	1730	rVB2	324	248	0.01%	0.002%
39	6.915	1730	1734	1737	rVB2	361	292	0.02%	0.002%
40	6.938	1737	1741	1745	rBV2	206	198	0.01%	0.001%
41	7.041	1767	1773	1774	rBV2	491	353	0.02%	0.003%
42	7.096	1788	1790	1794	rVB	331	194	0.01%	0.001%
43	7.186	1804	1818	1829	rBV4	4564	9975	0.56%	0.075%
44	7.243	1834	1836	1842	rVB2	564	590	0.03%	0.004%
45	7.279	1842	1847	1850	rBV2	361	383	0.02%	0.003%
46	7.382	1874	1879	1882	rBV2	316	307	0.02%	0.002%
47	7.565	1917	1936	1954	rBV	215558	374776	21.19%	2.805%
48	7.690	1967	1975	1992	rVB5	2787	5431	0.31%	0.041%
49	7.761	1992	1997	1998	rBV2	281	290	0.02%	0.002%
50	7.793	2001	2007	2012	rBV3	793	935	0.05%	0.007%
51	7.899	2025	2040	2055	rBV	797703	1371333	77.53%	10.265%
52	8.179	2115	2127	2146	rBV	147443	246721	13.95%	1.847%
53	8.324	2170	2172	2175	rVB2	400	189	0.01%	0.001%
54	8.359	2182	2183	2189	rVB2	567	310	0.02%	0.002%
55	8.517	2230	2232	2237	rVB3	289	203	0.01%	0.002%
56	8.632	2255	2268	2301	rBV	634310	1161228	65.65%	8.692%
57	8.874	2339	2343	2346	rBV	397	351	0.02%	0.003%
58	8.983	2374	2377	2379	rBV2	333	257	0.01%	0.002%
59	9.025	2387	2390	2399	rVB3	300	376	0.02%	0.003%
60	9.073	2402	2405	2408	rBV2	470	342	0.02%	0.003%
61	9.121	2415	2420	2424	rBV3	387	392	0.02%	0.003%
62	9.163	2429	2433	2437	rVB3	539	536	0.03%	0.004%
63	9.230	2449	2454	2459	rVV3	506	425	0.02%	0.003%
64	9.417	2498	2512	2536	rBV	655403	1090516	61.65%	8.163%
65	9.632	2577	2579	2583	rBV2	299	205	0.01%	0.002%
66	9.652	2583	2585	2591	rVB2	469	281	0.02%	0.002%
67	9.690	2592	2597	2607	rVV4	1368	2086	0.12%	0.016%
68	9.732	2608	2610	2618	rVB3	392	292	0.02%	0.002%
69	9.796	2622	2630	2635	rBV2	268	490	0.03%	0.004%
70	9.883	2655	2657	2662	rBV2	227	200	0.01%	0.001%
71	10.105	2720	2726	2730	rVV4	562	635	0.04%	0.005%
72	10.153	2739	2741	2747	rVB3	329	202	0.01%	0.002%
73	10.214	2752	2760	2763	rBV3	646	789	0.04%	0.006%
74	10.279	2776	2780	2783	rBV2	328	291	0.02%	0.002%
75	10.671	2896	2902	2911	rVB3	3093	4256	0.24%	0.032%
76	10.758	2916	2929	2952	rBV	666525	1072526	60.63%	8.028%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048275.D
 Acq On : 25 Apr 2022 18:04
 Operator : SY/MD
 Sample : N2486-21
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.857	2958	2960	2963	rBV3	436	300	0.02%	0.002%
78	10.893	2964	2971	2982	rVB3	2767	4446	0.25%	0.033%
79	11.005	3003	3006	3010	rVB2	478	352	0.02%	0.003%
80	11.092	3030	3033	3037	rVV2	562	417	0.02%	0.003%
81	11.291	3092	3095	3099	rVB2	419	281	0.02%	0.002%
82	11.407	3129	3131	3139	rVB4	562	582	0.03%	0.004%
83	11.459	3139	3147	3148	rBV3	2659	2633	0.15%	0.020%
84	11.578	3181	3184	3192	rVB4	656	629	0.04%	0.005%
85	11.693	3216	3220	3228	rVB3	1163	1443	0.08%	0.011%
86	11.745	3231	3236	3244	rVB4	1374	2162	0.12%	0.016%
87	11.812	3244	3257	3277	rBV	654120	1024676	57.93%	7.670%
88	11.970	3302	3306	3318	rVB7	2313	3397	0.19%	0.025%
89	12.195	3362	3376	3396	rBV	772305	1256766	71.05%	9.408%
90	12.330	3416	3418	3425	rVB4	1039	939	0.05%	0.007%
91	12.639	3510	3514	3521	rVB3	925	1140	0.06%	0.009%
92	12.680	3521	3527	3529	rBV3	460	481	0.03%	0.004%
93	12.771	3551	3555	3567	rVB4	2081	2778	0.16%	0.021%
94	13.227	3691	3697	3706	rVB5	1050	1433	0.08%	0.011%
95	13.301	3716	3720	3725	rBV3	342	419	0.02%	0.003%
96	13.848	3882	3890	3901	rVB3	6331	9188	0.52%	0.069%
97	14.095	3960	3967	3976	rBV2	3076	4486	0.25%	0.034%
98	14.333	4035	4041	4051	rVB6	3598	5499	0.31%	0.041%
99	14.520	4097	4099	4105	rVB3	444	334	0.02%	0.003%
100	14.571	4112	4115	4119	rBV3	534	441	0.02%	0.003%




Sum of corrected areas: 13358997

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048275.D
Acq On : 25 Apr 2022 18:04
Operator : SY/MD
Sample : N2486-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

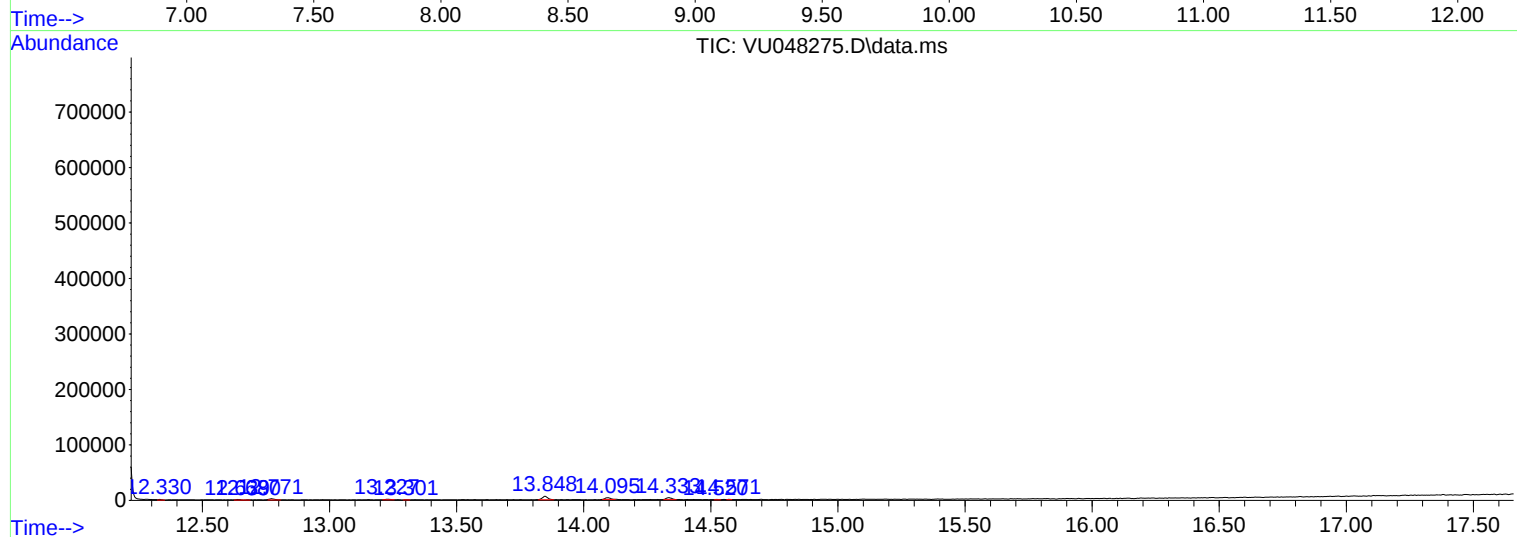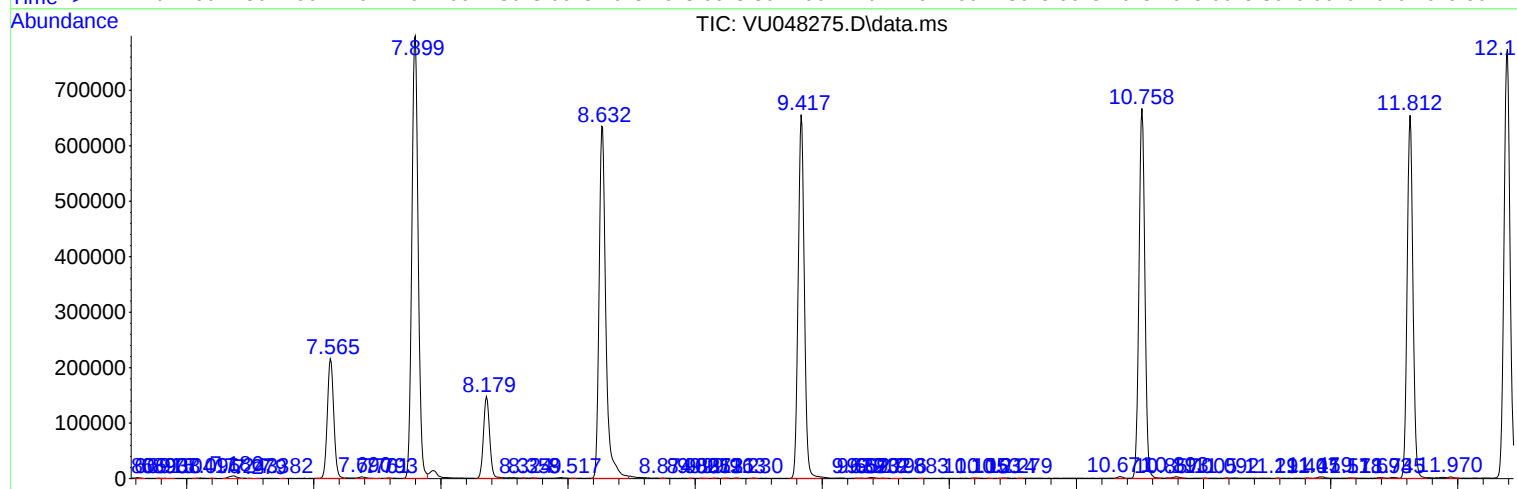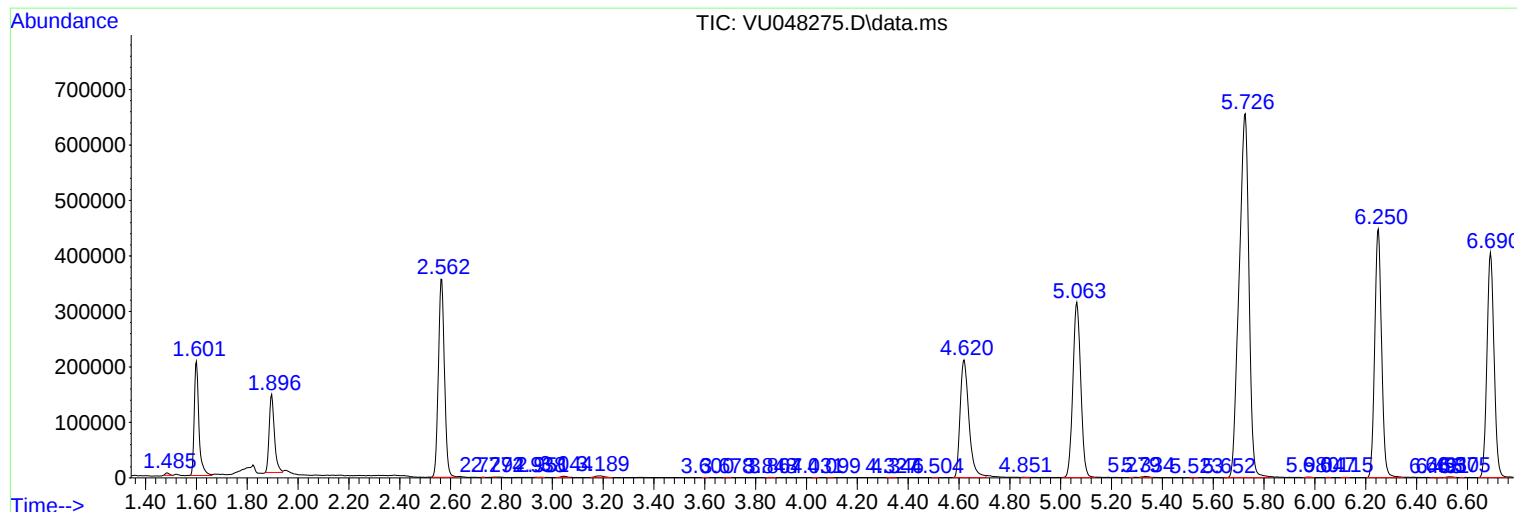

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048275.D
Acq On : 25 Apr 2022 18:04
Operator : SY/MD
Sample : N2486-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048275.D
Acq On : 25 Apr 2022 18:04
Operator : SY/MD
Sample : N2486-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------