

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048276.D
 Acq On : 25 Apr 2022 18:28
 Operator : SY/MD
 Sample : N2488-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048276.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	39	46	52	rBV3	5090	8137	0.49%	0.063%
2	1.600	73	81	98	rBV	190345	242052	14.43%	1.870%
3	1.890	163	171	187	rVB	132182	194953	11.62%	1.506%
4	2.562	367	380	397	rBV	336080	555145	33.10%	4.289%
5	2.678	414	416	420	rVB2	697	454	0.03%	0.004%
6	2.729	429	432	435	rBV3	258	183	0.01%	0.001%
7	2.745	435	437	440	rVB	433	216	0.01%	0.002%
8	3.047	522	531	545	rVV4	2110	3795	0.23%	0.029%
9	3.186	561	574	587	rBV	7270	16983	1.01%	0.131%
10	3.250	592	594	598	rVB2	538	268	0.02%	0.002%
11	3.346	621	624	628	rBV2	291	270	0.02%	0.002%
12	3.604	701	704	709	rVB2	386	315	0.02%	0.002%
13	3.944	808	810	813	rVV	303	207	0.01%	0.002%
14	4.057	841	845	847	rBV2	332	269	0.02%	0.002%
15	4.153	869	875	877	rBV	194	196	0.01%	0.002%
16	4.260	903	908	911	rBV2	237	183	0.01%	0.001%
17	4.517	982	988	991	rBV2	246	235	0.01%	0.002%
18	4.620	1006	1020	1046	rBV	212179	508996	30.35%	3.932%
19	4.819	1079	1082	1087	rBV4	445	428	0.03%	0.003%
20	5.063	1140	1158	1177	rBV	295496	642982	38.34%	4.967%
21	5.208	1201	1203	1206	rVB2	392	201	0.01%	0.002%
22	5.240	1210	1213	1216	rBV	367	207	0.01%	0.002%
23	5.285	1222	1227	1232	rBV2	767	952	0.06%	0.007%
24	5.311	1232	1235	1236	rVV	558	382	0.02%	0.003%
25	5.340	1236	1244	1257	rVB4	1566	3429	0.20%	0.026%
26	5.722	1341	1363	1399	rBV2	621765	1677040	100.00%	12.956%
27	5.964	1433	1438	1445	rBV4	758	935	0.06%	0.007%
28	6.041	1455	1462	1468	rVB4	506	703	0.04%	0.005%
29	6.083	1471	1475	1479	rVB2	264	237	0.01%	0.002%
30	6.115	1479	1485	1489	rBV3	508	510	0.03%	0.004%
31	6.166	1497	1501	1505	rVB2	358	322	0.02%	0.002%
32	6.250	1512	1527	1546	rBV	419274	794476	47.37%	6.138%
33	6.523	1606	1612	1615	rBV3	1479	1773	0.11%	0.014%
34	6.581	1627	1630	1632	rBV3	460	279	0.02%	0.002%
35	6.690	1649	1664	1690	rBV	395294	766655	45.71%	5.923%
36	6.816	1700	1703	1707	rVV3	1091	1039	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048276.D
 Acq On : 25 Apr 2022 18:28
 Operator : SY/MD
 Sample : N2488-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.835	1707	1709	1714	rVB2	445	393	0.02%	0.003%
38	6.941	1737	1742	1745	rBV	292	308	0.02%	0.002%
39	6.999	1755	1760	1765	rBV3	250	257	0.02%	0.002%
40	7.054	1768	1777	1782	rVV3	750	1154	0.07%	0.009%
41	7.179	1805	1816	1832	rVV5	4550	10188	0.61%	0.079%
42	7.288	1846	1850	1854	rBV2	297	320	0.02%	0.002%
43	7.459	1902	1903	1909	rVB2	282	192	0.01%	0.001%
44	7.565	1924	1936	1954	rBV	207359	362304	21.60%	2.799%
45	7.642	1958	1960	1964	rVB2	505	338	0.02%	0.003%
46	7.690	1967	1975	1984	rVV4	2148	3377	0.20%	0.026%
47	7.790	2001	2006	2007	rBV4	655	601	0.04%	0.005%
48	7.828	2015	2018	2021	rVB	303	197	0.01%	0.002%
49	7.896	2021	2039	2055	rBV	746696	1297793	77.39%	10.026%
50	8.118	2103	2108	2110	rVB2	382	310	0.02%	0.002%
51	8.179	2115	2127	2145	rBV	146830	248180	14.80%	1.917%
52	8.369	2183	2186	2190	rVB4	388	217	0.01%	0.002%
53	8.414	2198	2200	2203	rVB3	423	213	0.01%	0.002%
54	8.494	2222	2225	2229	rVB3	374	289	0.02%	0.002%
55	8.552	2241	2243	2247	rBV2	258	184	0.01%	0.001%
56	8.636	2255	2269	2301	rBV	648863	1217094	72.57%	9.403%
57	8.880	2342	2345	2349	rVB	345	187	0.01%	0.001%
58	8.925	2355	2359	2361	rBV2	419	341	0.02%	0.003%
59	9.002	2380	2383	2386	rVB2	313	221	0.01%	0.002%
60	9.166	2427	2434	2438	rVB3	516	609	0.04%	0.005%
61	9.198	2438	2444	2451	rBV2	269	437	0.03%	0.003%
62	9.417	2496	2512	2535	rBV	637128	1052701	62.77%	8.133%
63	9.574	2557	2561	2567	rVV3	881	920	0.05%	0.007%
64	9.603	2567	2570	2574	rVB	369	193	0.01%	0.001%
65	9.697	2592	2599	2608	rVB3	1516	2088	0.12%	0.016%
66	9.774	2620	2623	2629	rVB3	302	311	0.02%	0.002%
67	9.848	2643	2646	2652	rVB2	415	330	0.02%	0.003%
68	10.031	2695	2703	2706	rBV2	226	328	0.02%	0.003%
69	10.111	2720	2728	2730	rBV5	631	660	0.04%	0.005%
70	10.169	2742	2746	2751	rBV2	352	299	0.02%	0.002%
71	10.230	2762	2765	2768	rBV	289	187	0.01%	0.001%
72	10.250	2768	2771	2778	rVB2	283	269	0.02%	0.002%
73	10.330	2793	2796	2804	rBV2	233	330	0.02%	0.003%
74	10.552	2863	2865	2871	rVB	370	239	0.01%	0.002%
75	10.671	2894	2902	2910	rVB4	2697	3880	0.23%	0.030%
76	10.758	2916	2929	2948	rBV	681427	1084022	64.64%	8.375%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048276.D
 Acq On : 25 Apr 2022 18:28
 Operator : SY/MD
 Sample : N2488-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.889	2968	2970	2978	rVB4	920	1023	0.06%	0.008%
78	10.925	2978	2981	2985	rVB3	461	315	0.02%	0.002%
79	11.118	3037	3041	3048	rBV5	860	1035	0.06%	0.008%
80	11.150	3048	3051	3057	rVB2	463	450	0.03%	0.003%
81	11.272	3086	3089	3090	rBV	336	176	0.01%	0.001%
82	11.462	3138	3148	3159	rBV7	2242	3908	0.23%	0.030%
83	11.693	3212	3220	3227	rBV4	1130	1698	0.10%	0.013%
84	11.748	3232	3237	3244	rVV4	861	1130	0.07%	0.009%
85	11.812	3244	3257	3283	rVV	614287	983397	58.64%	7.597%
86	11.941	3293	3297	3300	rBV4	786	714	0.04%	0.006%
87	12.086	3340	3342	3344	rVB2	515	262	0.02%	0.002%
88	12.105	3344	3348	3349	rBV2	459	339	0.02%	0.003%
89	12.195	3360	3376	3402	rBV	754323	1215268	72.47%	9.388%
90	12.394	3436	3438	3444	rVB	488	327	0.02%	0.003%
91	12.680	3523	3527	3529	rBV2	326	246	0.01%	0.002%
92	12.774	3550	3556	3563	rVB3	1181	1646	0.10%	0.013%
93	12.896	3592	3594	3601	rVB2	521	540	0.03%	0.004%
94	12.931	3601	3605	3607	rBV2	544	463	0.03%	0.004%
95	13.848	3884	3890	3901	rVB6	2440	3839	0.23%	0.030%
96	14.098	3959	3968	3985	rBV3	2863	5737	0.34%	0.044%
97	14.192	3995	3997	3999	rBV	470	262	0.02%	0.002%
98	14.333	4035	4041	4051	rVB5	1675	2826	0.17%	0.022%
99	14.703	4153	4156	4159	rBV	580	283	0.02%	0.002%
100	14.722	4159	4162	4165	rBV2	582	480	0.03%	0.004%




Sum of corrected areas: 12944232

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048276.D
Acq On : 25 Apr 2022 18:28
Operator : SY/MD
Sample : N2488-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

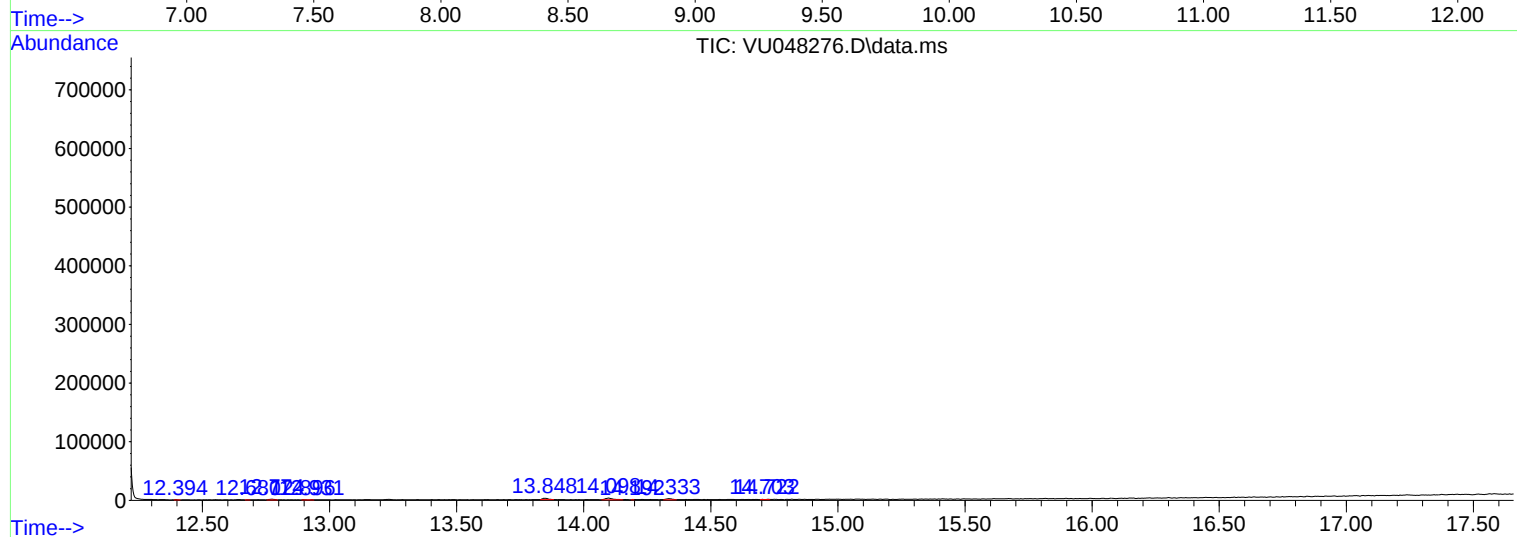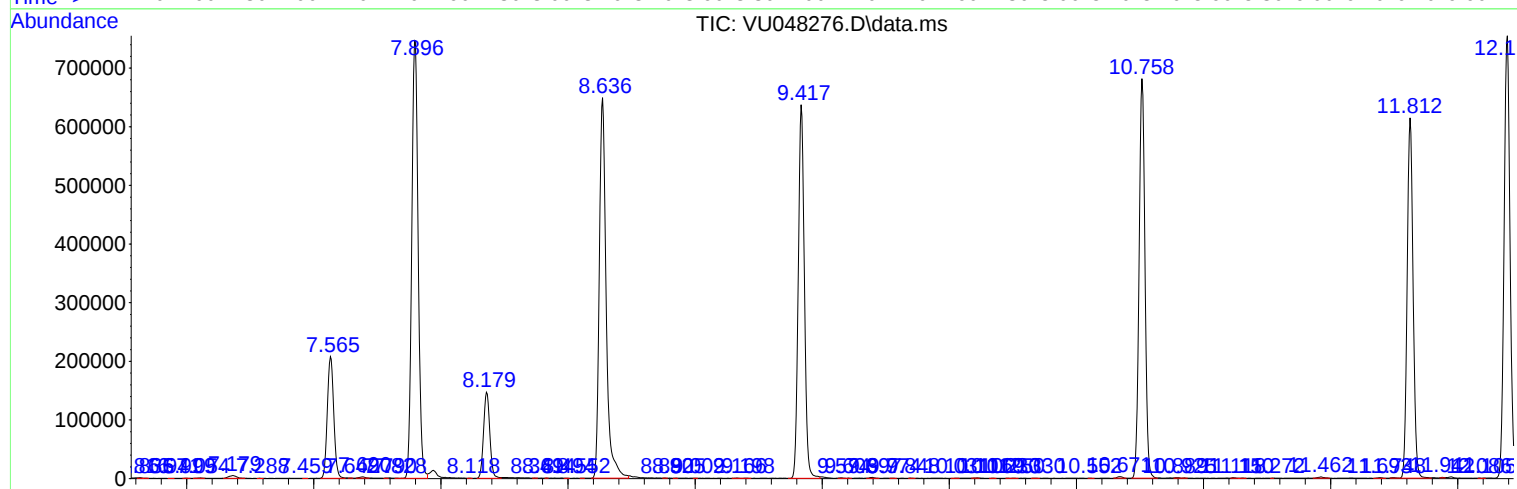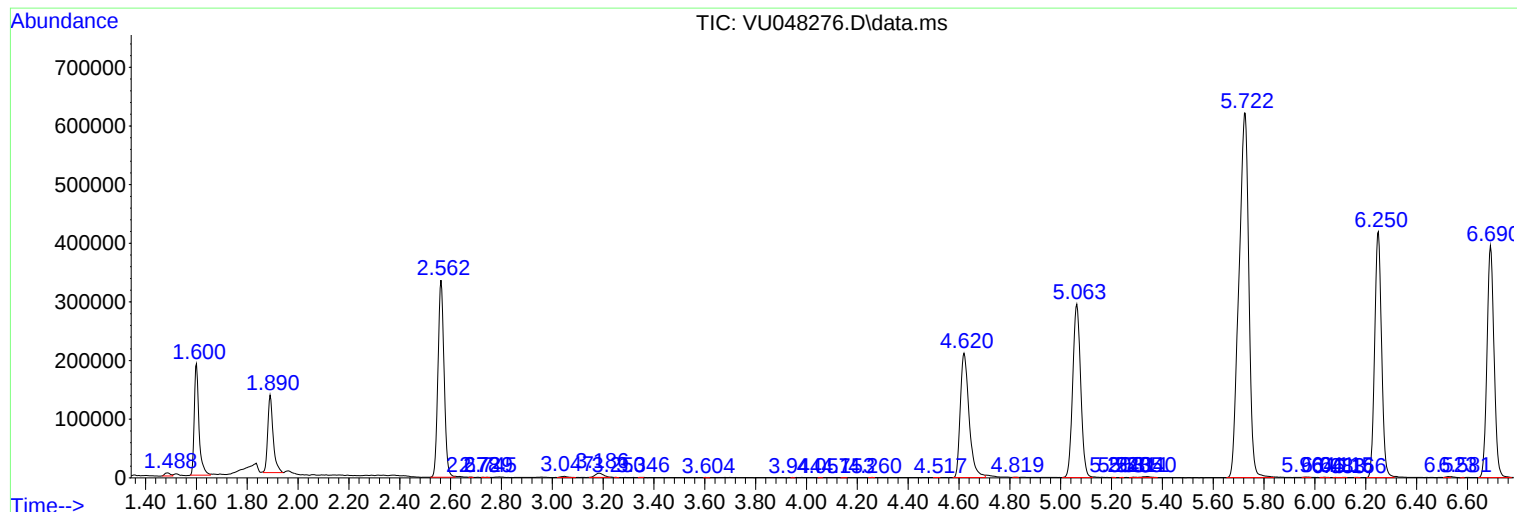

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048276.D
Acq On : 25 Apr 2022 18:28
Operator : SY/MD
Sample : N2488-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048276.D
Acq On : 25 Apr 2022 18:28
Operator : SY/MD
Sample : N2488-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------