

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048281.D
 Acq On : 25 Apr 2022 20:27
 Operator : SY/MD
 Sample : N2518-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXER7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	38	44	51	rBV2	6363	9012	0.55%	0.070%
2	1.601	73	81	101	rBV	181059	236692	14.36%	1.839%
3	1.884	162	169	191	rVB	125517	203613	12.35%	1.582%
4	2.504	359	362	367	rVB	415	334	0.02%	0.003%
5	2.559	367	379	396	rBV	326612	544700	33.04%	4.232%
6	2.784	441	449	458	rVB5	911	1520	0.09%	0.012%
7	2.832	461	464	467	rVB3	380	240	0.01%	0.002%
8	2.855	467	471	476	rVB4	441	390	0.02%	0.003%
9	2.893	480	483	486	rBV3	412	299	0.02%	0.002%
10	2.948	496	500	503	rBV4	520	492	0.03%	0.004%
11	3.038	523	528	529	rBV2	632	441	0.03%	0.003%
12	3.134	554	558	561	rVB	350	261	0.02%	0.002%
13	3.183	561	573	586	rBV	5211	11710	0.71%	0.091%
14	3.404	637	642	645	rVV2	185	191	0.01%	0.001%
15	3.466	656	661	666	rBV2	302	320	0.02%	0.002%
16	3.597	698	702	706	rBV2	309	290	0.02%	0.002%
17	3.655	716	720	723	rBV2	344	271	0.02%	0.002%
18	4.256	901	907	909	rBV2	202	232	0.01%	0.002%
19	4.501	980	983	988	rVB3	276	214	0.01%	0.002%
20	4.620	1006	1020	1047	rBV	189040	480973	29.17%	3.737%
21	4.854	1089	1093	1095	rVB2	299	211	0.01%	0.002%
22	5.060	1141	1157	1183	rBV	311362	679537	41.22%	5.280%
23	5.224	1205	1208	1211	rVB	393	226	0.01%	0.002%
24	5.298	1220	1231	1234	rBV3	667	1078	0.07%	0.008%
25	5.337	1234	1243	1246	rBV5	1087	1517	0.09%	0.012%
26	5.723	1341	1363	1388	rBV2	619745	1648650	100.00%	12.810%
27	5.973	1432	1441	1452	rVB3	1927	3783	0.23%	0.029%
28	6.083	1472	1475	1479	rVB2	223	198	0.01%	0.002%
29	6.118	1484	1486	1490	rVB2	330	246	0.01%	0.002%
30	6.247	1508	1526	1558	rBV	416834	798502	48.43%	6.205%
31	6.369	1561	1564	1569	rVV3	425	399	0.02%	0.003%
32	6.436	1582	1585	1589	rVB2	389	300	0.02%	0.002%
33	6.459	1589	1592	1595	rBV2	357	312	0.02%	0.002%
34	6.526	1607	1613	1621	rBV4	1320	2083	0.13%	0.016%
35	6.594	1629	1634	1644	rVB5	1084	1627	0.10%	0.013%
36	6.690	1644	1664	1685	rBV	398216	774869	47.00%	6.021%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048281.D
 Acq On : 25 Apr 2022 20:27
 Operator : SY/MD
 Sample : N2518-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXER7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.803	1694	1699	1711	rVB4	1048	2029	0.12%	0.016%
38	6.935	1737	1740	1744	rVB	279	239	0.01%	0.002%
39	7.060	1773	1779	1784	rVB3	569	681	0.04%	0.005%
40	7.182	1803	1817	1835	rBV7	4418	10437	0.63%	0.081%
41	7.565	1923	1936	1960	rVV	197547	342283	20.76%	2.660%
42	7.690	1966	1975	1989	rVB6	2392	4883	0.30%	0.038%
43	7.745	1989	1992	1997	rBV2	297	281	0.02%	0.002%
44	7.771	1997	2000	2004	rVB3	263	198	0.01%	0.002%
45	7.803	2004	2010	2012	rBV3	515	557	0.03%	0.004%
46	7.896	2024	2039	2055	rBV	728510	1263543	76.64%	9.818%
47	8.179	2115	2127	2146	rVV	138511	236338	14.34%	1.836%
48	8.324	2170	2172	2176	rVB2	541	291	0.02%	0.002%
49	8.362	2182	2184	2189	rVB3	429	279	0.02%	0.002%
50	8.469	2211	2217	2232	rVB3	3031	5799	0.35%	0.045%
51	8.555	2240	2244	2248	rVB3	451	331	0.02%	0.003%
52	8.636	2256	2269	2304	rBV	630659	1182892	71.75%	9.191%
53	9.115	2414	2418	2422	rBV3	212	202	0.01%	0.002%
54	9.163	2431	2433	2436	rVB2	485	208	0.01%	0.002%
55	9.231	2449	2454	2456	rBV2	284	252	0.02%	0.002%
56	9.417	2498	2512	2542	rBV	621614	1030719	62.52%	8.009%
57	9.652	2580	2585	2588	rVB3	166	196	0.01%	0.002%
58	9.697	2588	2599	2608	rBV3	1193	1891	0.11%	0.015%
59	9.796	2628	2630	2637	rVB3	220	247	0.01%	0.002%
60	9.864	2649	2651	2655	rVB2	334	199	0.01%	0.002%
61	9.912	2659	2666	2668	rBV2	195	190	0.01%	0.001%
62	9.951	2674	2678	2681	rBV2	292	275	0.02%	0.002%
63	10.095	2718	2723	2726	rBV2	578	533	0.03%	0.004%
64	10.169	2743	2746	2751	rBV	283	267	0.02%	0.002%
65	10.308	2785	2789	2794	rVB	264	207	0.01%	0.002%
66	10.417	2818	2823	2826	rBV2	298	306	0.02%	0.002%
67	10.488	2841	2845	2848	rVB2	271	229	0.01%	0.002%
68	10.671	2893	2902	2909	rVV3	2791	3851	0.23%	0.030%
69	10.758	2916	2929	2952	rBV	680200	1096152	66.49%	8.517%
70	10.893	2958	2971	2987	rVB	5606	10409	0.63%	0.081%
71	10.957	2988	2991	2993	rBV3	284	194	0.01%	0.002%
72	11.002	3001	3005	3010	rVB3	311	345	0.02%	0.003%
73	11.034	3010	3015	3018	rBV3	372	381	0.02%	0.003%
74	11.092	3029	3033	3034	rBV	361	222	0.01%	0.002%
75	11.118	3037	3041	3042	rBV2	493	433	0.03%	0.003%
76	11.153	3048	3052	3057	rVB2	517	388	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048281.D
 Acq On : 25 Apr 2022 20:27
 Operator : SY/MD
 Sample : N2518-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXER7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.205	3065	3068	3072	rBV2	326	265	0.02%	0.002%
78	11.320	3098	3104	3111	rVB2	342	419	0.03%	0.003%
79	11.414	3129	3133	3137	rBV2	575	395	0.02%	0.003%
80	11.456	3137	3146	3148	rBV4	1719	2122	0.13%	0.016%
81	11.571	3179	3182	3189	rVV2	495	475	0.03%	0.004%
82	11.697	3213	3221	3227	rBV3	871	1410	0.09%	0.011%
83	11.751	3232	3238	3239	rBV2	606	555	0.03%	0.004%
84	11.812	3244	3257	3279	rBV	633744	1010677	61.30%	7.853%
85	12.009	3316	3318	3324	rVB2	431	339	0.02%	0.003%
86	12.073	3332	3338	3339	rBV2	345	288	0.02%	0.002%
87	12.115	3346	3351	3352	rBV2	398	328	0.02%	0.003%
88	12.195	3357	3376	3394	rBV	761353	1239591	75.19%	9.632%
89	12.481	3463	3465	3470	rVB2	412	275	0.02%	0.002%
90	12.529	3476	3480	3481	rBV	332	262	0.02%	0.002%
91	12.568	3489	3492	3495	rBV2	292	224	0.01%	0.002%
92	12.636	3508	3513	3514	rBV2	534	441	0.03%	0.003%
93	12.771	3549	3555	3565	rVB3	2524	3902	0.24%	0.030%
94	13.099	3654	3657	3661	rBV2	283	195	0.01%	0.002%
95	13.227	3692	3697	3702	rBV3	544	653	0.04%	0.005%
96	13.295	3715	3718	3721	rBV2	384	269	0.02%	0.002%
97	13.674	3832	3836	3837	rBV	380	237	0.01%	0.002%
98	14.256	4014	4017	4020	rBV3	335	237	0.01%	0.002%
99	14.330	4035	4040	4041	rBV2	700	555	0.03%	0.004%
100	15.491	4399	4401	4404	rBV3	816	413	0.03%	0.003%




Sum of corrected areas: 12869617

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048281.D
Acq On : 25 Apr 2022 20:27
Operator : SY/MD
Sample : N2518-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXER7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

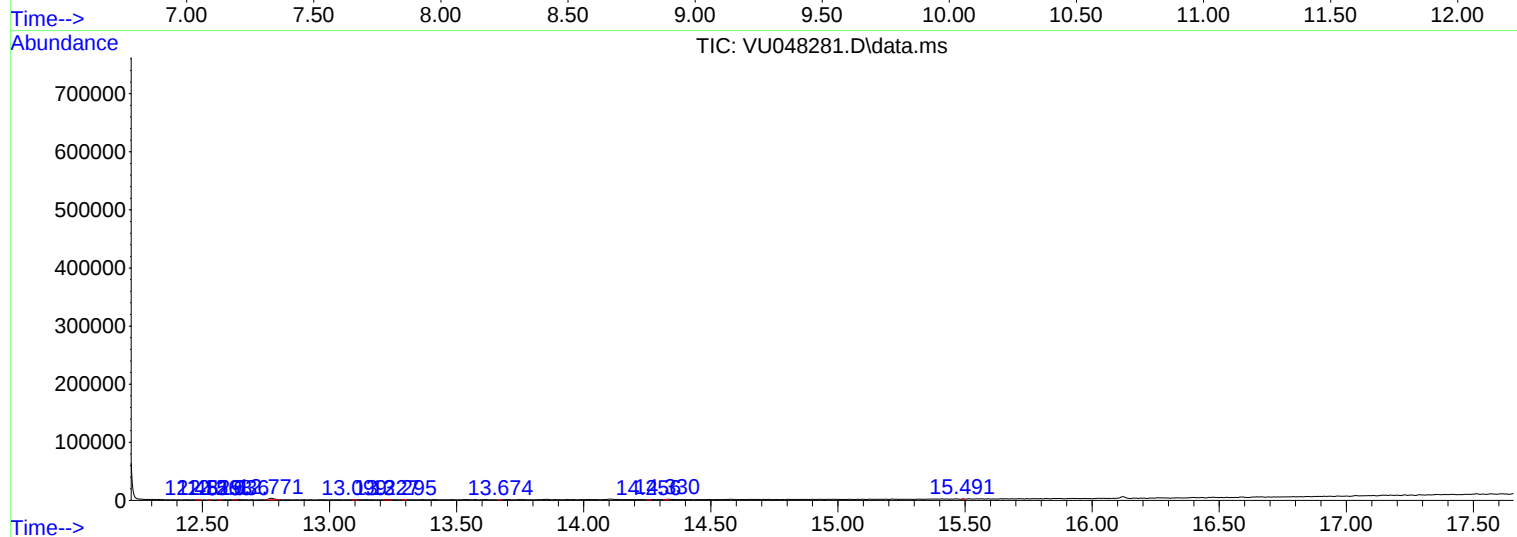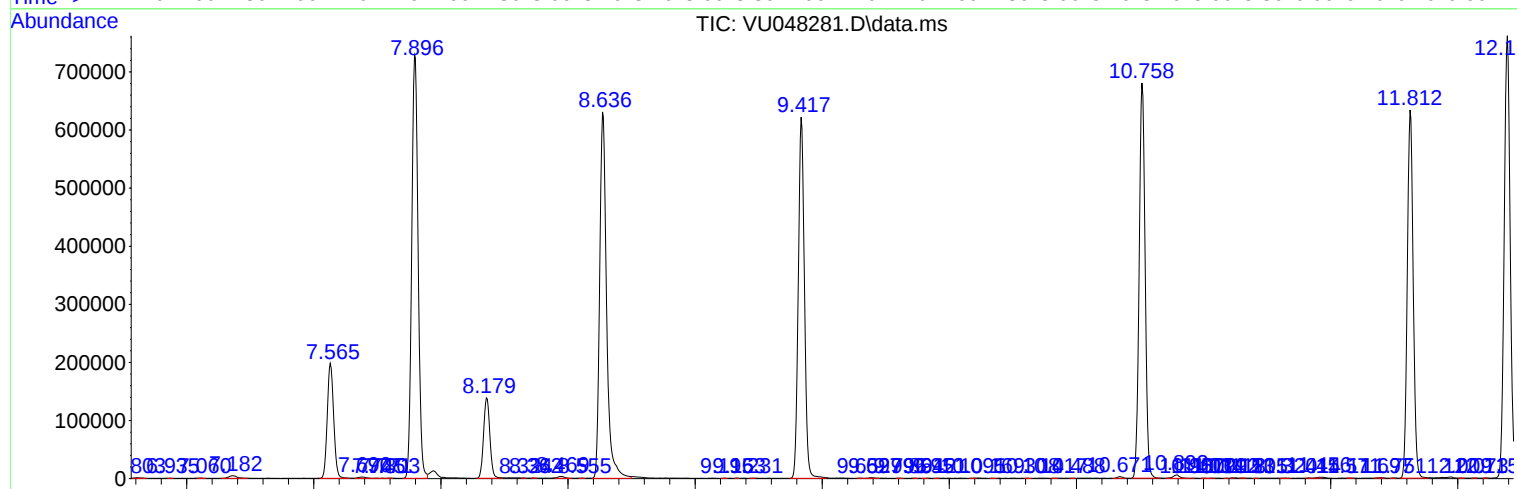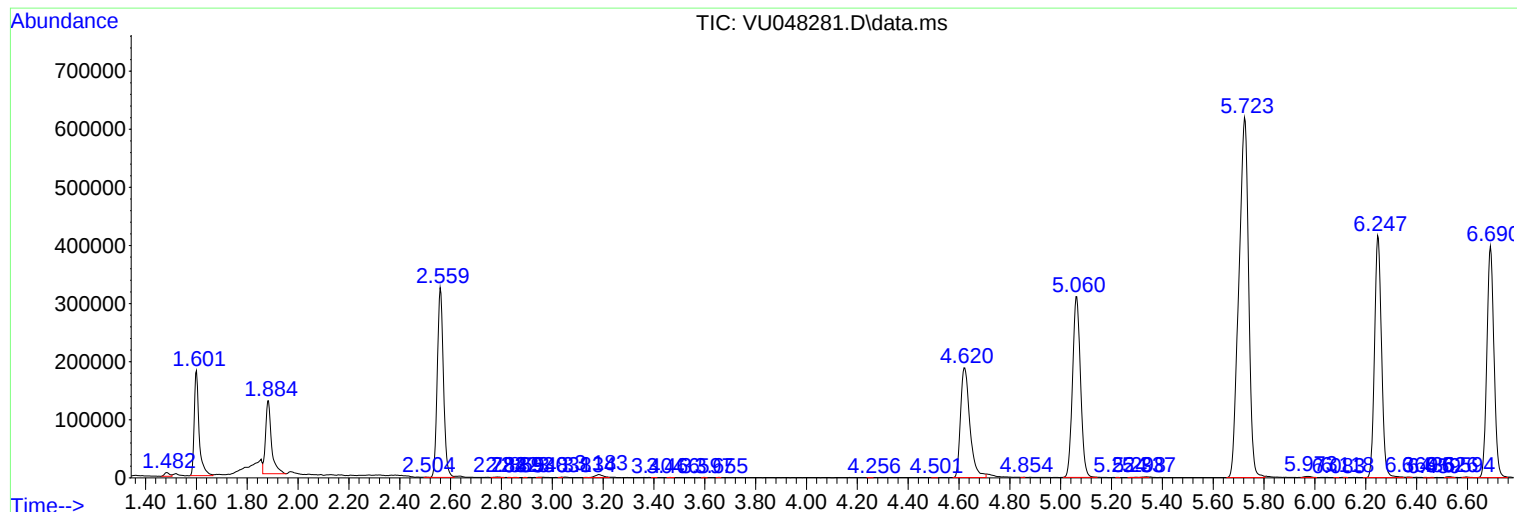

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048281.D
Acq On : 25 Apr 2022 20:27
Operator : SY/MD
Sample : N2518-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXER7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048281.D
Acq On : 25 Apr 2022 20:27
Operator : SY/MD
Sample : N2518-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXER7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------