

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048284.D
 Acq On : 25 Apr 2022 21:39
 Operator : SY/MD
 Sample : N2518-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.359	3	6	19	rVB2	8550	9503	0.55%	0.075%
2	1.488	40	46	51	rBV2	6480	8113	0.47%	0.064%
3	1.600	73	81	103	rBV	183627	235696	13.73%	1.854%
4	1.903	169	175	195	rVB	150712	219027	12.75%	1.723%
5	2.565	368	381	402	rBV	338158	568550	33.11%	4.472%
6	2.735	432	434	441	rVB3	426	383	0.02%	0.003%
7	2.832	461	464	467	rBV2	383	293	0.02%	0.002%
8	2.887	479	481	485	rVB2	424	244	0.01%	0.002%
9	3.041	523	529	534	rBV6	1054	1565	0.09%	0.012%
10	3.137	552	559	563	rBV2	704	811	0.05%	0.006%
11	3.186	568	574	584	rVV2	737	1420	0.08%	0.011%
12	3.613	704	707	712	rVV3	289	288	0.02%	0.002%
13	3.797	760	764	768	rVB2	239	194	0.01%	0.002%
14	3.935	802	807	813	rBV2	363	496	0.03%	0.004%
15	4.215	892	894	897	rVB2	264	166	0.01%	0.001%
16	4.629	1009	1023	1067	rBV	185507	500982	29.17%	3.940%
17	5.067	1141	1159	1184	rBV	302741	666011	38.78%	5.238%
18	5.234	1207	1211	1213	rBV2	311	254	0.01%	0.002%
19	5.279	1222	1225	1226	rBV	490	243	0.01%	0.002%
20	5.330	1238	1241	1244	rBV3	292	222	0.01%	0.002%
21	5.375	1251	1255	1256	rBV	453	278	0.02%	0.002%
22	5.578	1313	1318	1322	rBV2	264	317	0.02%	0.002%
23	5.726	1341	1364	1379	rBV2	643074	1717224	100.00%	13.506%
24	5.973	1435	1441	1445	rBV5	1309	1822	0.11%	0.014%
25	6.092	1472	1478	1481	rBV3	314	298	0.02%	0.002%
26	6.118	1481	1486	1487	rBV2	351	286	0.02%	0.002%
27	6.163	1498	1500	1502	rBV	278	184	0.01%	0.001%
28	6.250	1512	1527	1554	rBV	443243	844396	49.17%	6.641%
29	6.530	1606	1614	1621	rBV5	1571	2783	0.16%	0.022%
30	6.584	1625	1631	1632	rBV3	494	375	0.02%	0.003%
31	6.690	1649	1664	1692	rBV	410610	809425	47.14%	6.366%
32	7.005	1757	1762	1765	rBV2	214	238	0.01%	0.002%
33	7.189	1810	1819	1835	rVV3	4610	9301	0.54%	0.073%
34	7.346	1865	1868	1872	rVB2	269	167	0.01%	0.001%
35	7.439	1895	1897	1903	rVB2	234	175	0.01%	0.001%
36	7.565	1923	1936	1960	rBV	194719	350291	20.40%	2.755%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048284.D
 Acq On : 25 Apr 2022 21:39
 Operator : SY/MD
 Sample : N2518-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	7.690	1970	1975	1986	rVB5	2632	4094	0.24%	0.032%
38	7.735	1986	1989	1992	rBV2	396	267	0.02%	0.002%
39	7.751	1992	1994	1997	rVB2	339	199	0.01%	0.002%
40	7.771	1997	2000	2001	rBV	286	165	0.01%	0.001%
41	7.899	2026	2040	2055	rBV	752889	1301328	75.78%	10.235%
42	8.179	2115	2127	2147	rBV	136184	234406	13.65%	1.844%
43	8.433	2202	2206	2208	rBV2	342	231	0.01%	0.002%
44	8.475	2213	2219	2227	rVB3	2007	2682	0.16%	0.021%
45	8.578	2241	2251	2258	rVV	11930	18973	1.10%	0.149%
46	8.639	2258	2270	2308	rVB	597524	1095677	63.81%	8.618%
47	8.880	2343	2345	2348	rBV2	305	208	0.01%	0.002%
48	8.967	2369	2372	2376	rVB2	390	255	0.01%	0.002%
49	9.012	2382	2386	2388	rBV2	296	223	0.01%	0.002%
50	9.057	2397	2400	2401	rBV	405	206	0.01%	0.002%
51	9.108	2414	2416	2419	rBV2	342	215	0.01%	0.002%
52	9.156	2429	2431	2432	rBV	392	168	0.01%	0.001%
53	9.288	2468	2472	2480	rVB2	433	514	0.03%	0.004%
54	9.417	2499	2512	2537	rBV	623645	1042765	60.72%	8.201%
55	9.568	2552	2559	2561	rBV3	1206	1254	0.07%	0.010%
56	9.616	2568	2574	2579	rBV	483	688	0.04%	0.005%
57	9.639	2579	2581	2585	rVV2	462	368	0.02%	0.003%
58	9.690	2591	2597	2608	rVV2	1580	2845	0.17%	0.022%
59	10.086	2716	2720	2721	rBV	306	193	0.01%	0.002%
60	10.279	2777	2780	2786	rBV	344	285	0.02%	0.002%
61	10.446	2830	2832	2834	rBV	264	165	0.01%	0.001%
62	10.542	2859	2862	2864	rBV2	264	164	0.01%	0.001%
63	10.674	2894	2903	2910	rVB4	2525	3518	0.20%	0.028%
64	10.758	2916	2929	2949	rVV	639907	1027707	59.85%	8.083%
65	10.864	2960	2962	2964	rVV2	355	222	0.01%	0.002%
66	10.893	2964	2971	2981	rVB2	4451	6723	0.39%	0.053%
67	10.992	3000	3002	3005	rVV2	312	166	0.01%	0.001%
68	11.079	3026	3029	3031	rBV	239	182	0.01%	0.001%
69	11.118	3037	3041	3048	rVB2	823	944	0.05%	0.007%
70	11.246	3078	3081	3084	rBV2	312	241	0.01%	0.002%
71	11.346	3109	3112	3114	rVB	286	164	0.01%	0.001%
72	11.417	3129	3134	3138	rBV4	403	426	0.02%	0.003%
73	11.459	3141	3147	3148	rBV2	1380	1171	0.07%	0.009%
74	11.523	3164	3167	3169	rBV2	247	185	0.01%	0.001%
75	11.578	3181	3184	3189	rVB2	626	601	0.03%	0.005%
76	11.603	3189	3192	3195	rBV2	286	261	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048284.D
 Acq On : 25 Apr 2022 21:39
 Operator : SY/MD
 Sample : N2518-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.658	3206	3209	3212	rBV2	268	169	0.01%	0.001%
78	11.700	3215	3222	3226	rVV3	1104	1234	0.07%	0.010%
79	11.725	3226	3230	3233	rVB3	306	243	0.01%	0.002%
80	11.751	3233	3238	3243	rVB2	571	528	0.03%	0.004%
81	11.812	3245	3257	3280	rBV	574823	904090	52.65%	7.111%
82	11.970	3304	3306	3315	rVB7	1932	2261	0.13%	0.018%
83	12.066	3327	3336	3352	rBV8	3726	8286	0.48%	0.065%
84	12.195	3362	3376	3396	rBV	655833	1086937	63.30%	8.549%
85	12.330	3415	3418	3420	rBV2	576	378	0.02%	0.003%
86	12.439	3450	3452	3456	rVB2	379	211	0.01%	0.002%
87	12.478	3462	3464	3468	rBV	346	209	0.01%	0.002%
88	12.500	3468	3471	3473	rVV2	361	259	0.02%	0.002%
89	12.533	3477	3481	3483	rBV2	300	249	0.01%	0.002%
90	12.700	3528	3533	3537	rVB4	310	279	0.02%	0.002%
91	12.722	3537	3540	3543	rBV2	309	241	0.01%	0.002%
92	12.777	3549	3557	3564	rBV	1845	2685	0.16%	0.021%
93	12.954	3610	3612	3615	rBV	316	197	0.01%	0.002%
94	13.031	3631	3636	3639	rBV3	435	555	0.03%	0.004%
95	13.150	3670	3673	3677	rBV2	473	403	0.02%	0.003%
96	13.381	3743	3745	3747	rBV2	355	192	0.01%	0.002%
97	13.668	3831	3834	3837	rBV2	471	348	0.02%	0.003%
98	14.089	3961	3965	3966	rBV2	594	460	0.03%	0.004%
99	14.671	4143	4146	4151	rBV	501	434	0.03%	0.003%
100	14.819	4188	4192	4193	rBV3	537	412	0.02%	0.003%




Sum of corrected areas: 12714330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048284.D
Acq On : 25 Apr 2022 21:39
Operator : SY/MD
Sample : N2518-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

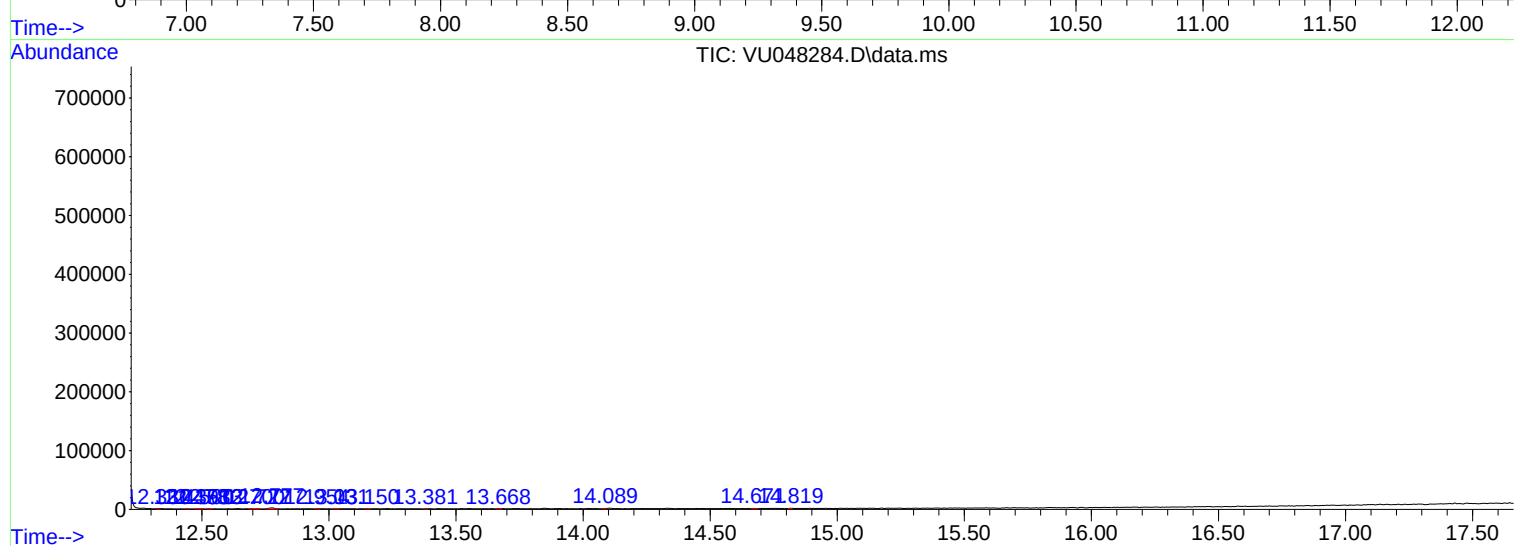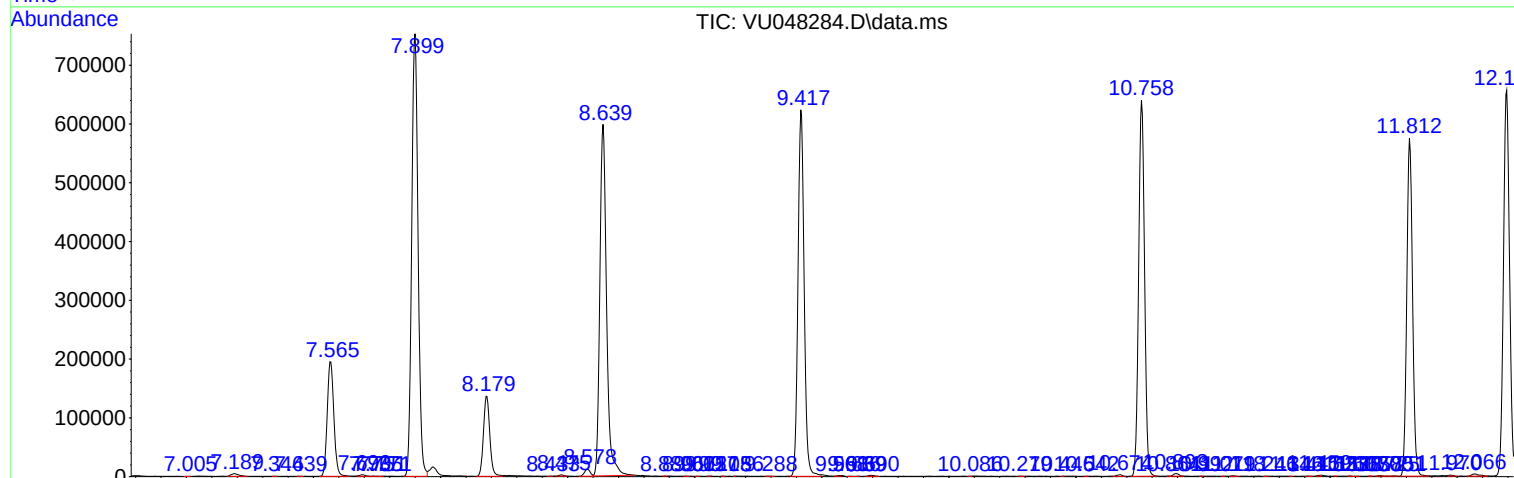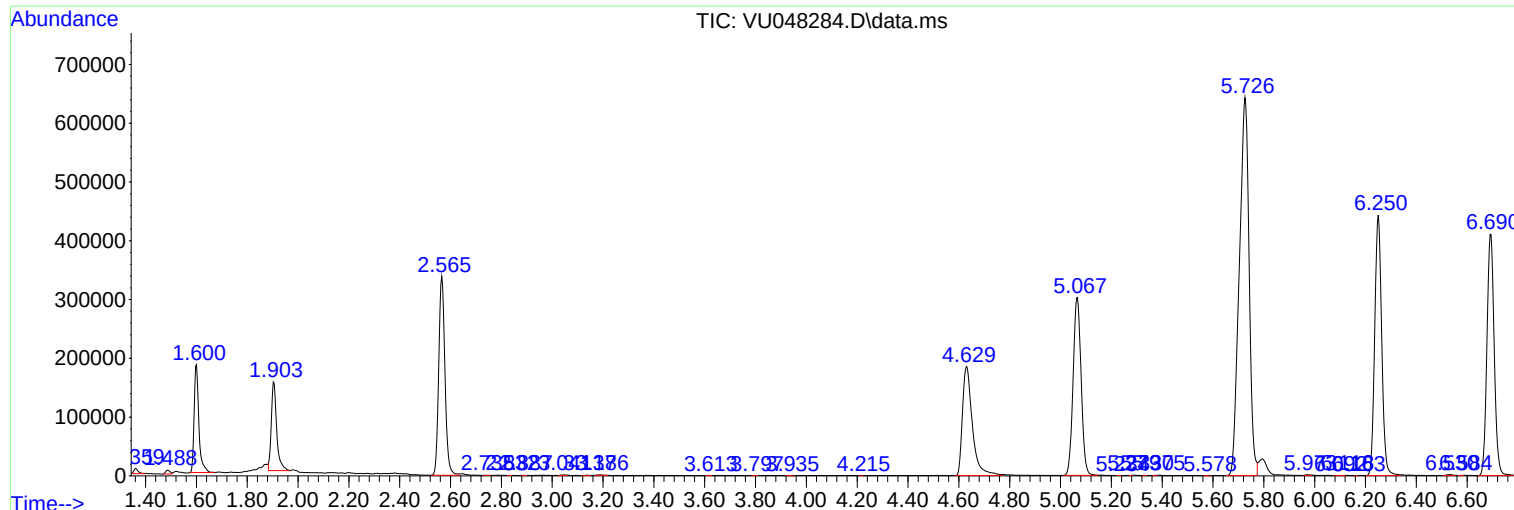

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048284.D
Acq On : 25 Apr 2022 21:39
Operator : SY/MD
Sample : N2518-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
Data File : VU048284.D
Acq On : 25 Apr 2022 21:39
Operator : SY/MD
Sample : N2518-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc