


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042522\
 Data File : VU048258.D
 Acq On : 25 Apr 2022 08:48
 Operator : SY/MD
 Sample : BFB072
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB072

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 26 02:41:26 2022

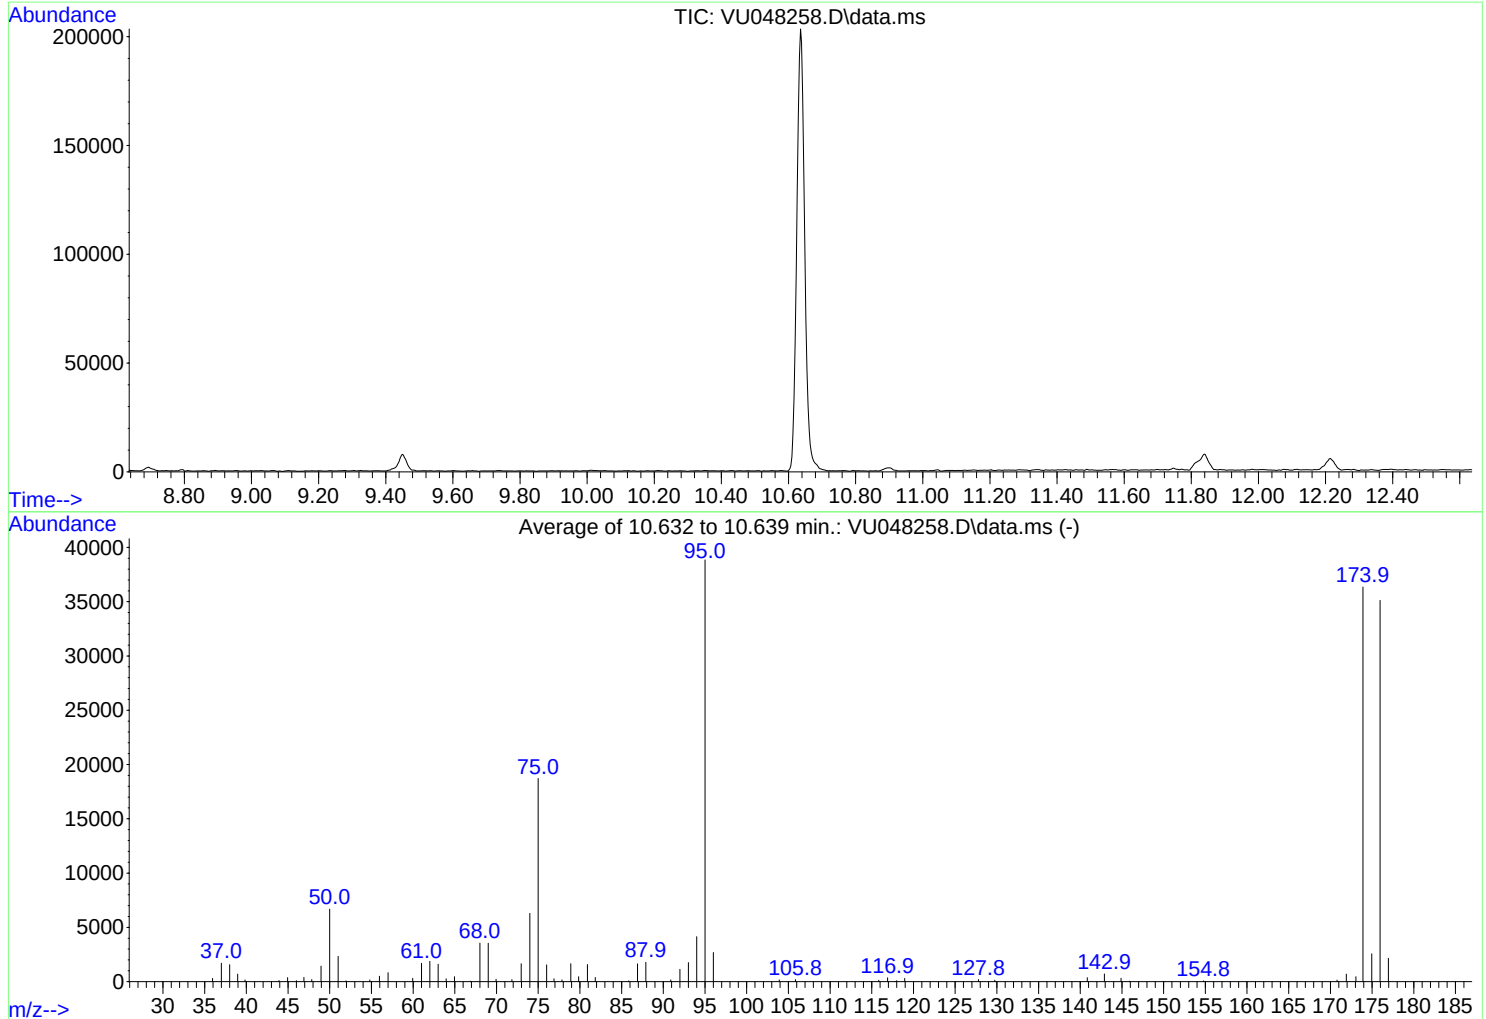

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	6677	PASS
75	95	30	80	48.2	18715	PASS
95	95	100	100	100.0	38856	PASS
96	95	5	9	6.9	2676	PASS
173	174	0.00	2	1.3	464	PASS
174	95	50	120	93.5	36344	PASS
175	174	5	9	7.0	2562	PASS
176	174	95	101	96.6	35125	PASS
177	176	5	9	6.1	2150	PASS

m/z	Abundance
43.90	364.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
35.90	264.0
37.00	1684.0
38.00	1585.0
38.90	663.0
39.90	154.0
43.90	476.0
45.00	314.0
46.90	367.0
47.90	240.0
49.00	1353.0
50.00	6734.0
51.00	2211.0
52.00	122.0
54.80	161.0
56.00	527.0
57.00	833.0
60.00	307.0
61.00	1690.0
62.00	1805.0
63.00	1648.0
63.90	277.0
64.90	441.0
68.00	3455.0
69.00	3502.0
69.90	195.0
71.90	209.0
73.00	1607.0
74.00	6092.0
75.00	18096.0
76.00	1587.0
76.90	274.0
77.90	169.0
78.90	1598.0
79.90	430.0
80.90	1616.0
81.90	371.0
85.80	124.0
86.90	1593.0
87.90	1747.0
90.90	189.0
92.00	1157.0
93.00	1626.0
94.00	4090.0
95.00	37936.0
96.00	2544.0
104.00	147.0
105.90	195.0
115.90	122.0
116.90	340.0
117.80	101.0
118.90	300.0
127.70	187.0
129.80	145.0
140.90	316.0
142.90	646.0
144.90	283.0
145.90	118.0
154.80	104.0
170.80	126.0
171.90	692.0
173.10	398.0
173.90	33904.0
174.90	2627.0
175.90	33760.0
176.90	2053.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
36.00	304.0
37.00	1783.0
38.00	1567.0
39.00	706.0
39.90	178.0
43.90	475.0
44.90	391.0
46.00	142.0
46.90	413.0
47.80	190.0
48.90	1484.0
50.00	6945.0
51.00	2413.0
51.90	109.0
54.80	177.0
56.00	512.0
57.00	835.0
60.00	322.0
61.00	1748.0
62.00	1890.0
63.00	1643.0
64.00	261.0
65.00	454.0
68.00	3669.0
69.00	3634.0
69.90	221.0
71.90	206.0
73.00	1727.0
74.00	6506.0
75.00	19288.0
76.00	1604.0
76.90	276.0
77.90	172.0
78.90	1712.0
79.80	474.0
80.90	1645.0
81.80	383.0
85.90	112.0
86.90	1668.0
87.90	1876.0
90.90	176.0
92.00	1197.0
93.00	1831.0
94.00	4192.0
95.00	40064.0
96.00	2779.0
103.90	158.0
105.80	199.0
115.90	139.0
116.90	374.0
118.00	126.0
119.00	305.0
127.80	172.0
129.70	151.0
140.80	385.0
142.90	757.0
144.90	329.0
154.80	102.0
170.80	161.0
171.90	706.0
173.00	478.0
173.90	37536.0
175.00	2670.0
175.90	36176.0
177.00	2206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072

m/z	Abundance
36.00	302.0
37.00	1621.0
38.00	1515.0
39.00	727.0
39.80	170.0
43.90	452.0
44.90	412.0
46.00	128.0
46.90	414.0
47.90	143.0
48.90	1453.0
50.00	6352.0
51.00	2346.0
54.80	160.0
55.90	481.0
57.00	805.0
59.90	289.0
61.00	1656.0
62.00	1934.0
63.00	1527.0
64.00	250.0
65.00	468.0
66.90	114.0
68.00	3542.0
69.00	3473.0
70.00	245.0
71.80	175.0
72.90	1610.0
74.00	6278.0
75.00	18760.0
76.00	1473.0
76.90	252.0
77.80	160.0
78.90	1664.0
79.90	483.0
80.90	1472.0
81.80	396.0
86.90	1636.0
87.90	1738.0
90.90	136.0
92.00	1064.0
93.00	1801.0
94.00	4128.0
95.00	38568.0
96.00	2704.0
103.80	166.0
105.80	186.0
115.80	127.0
116.90	356.0
118.00	139.0
119.00	258.0
127.90	226.0
129.70	126.0
140.80	384.0
142.90	730.0
144.90	336.0
170.80	171.0
171.90	663.0
173.00	516.0
173.90	37592.0
174.90	2388.0
176.00	35440.0
177.00	2191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB072