

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
 Data File : VU053879.D
 Acq On : 25 Apr 2023 13:14
 Operator : JC/MD
 Sample : VIBLK157
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK157

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	92	rBV	50219	59210	15.42%	1.765%
2	1.916	169	179	194	rBV	43618	58367	15.20%	1.740%
3	2.565	370	381	400	rVB	84537	139759	36.40%	4.165%
4	3.044	517	530	549	rVB2	16104	31962	8.32%	0.953%
5	4.636	1014	1025	1053	rBV2	38371	120081	31.27%	3.579%
6	5.057	1142	1156	1175	rVB2	77345	170037	44.28%	5.068%
7	5.723	1343	1363	1400	rBV2	148436	383996	100.00%	11.445%
8	6.247	1512	1526	1542	rBV	156229	300736	78.32%	8.963%
9	6.539	1606	1617	1633	rBV7	10538	20762	5.41%	0.619%
10	6.687	1650	1663	1679	rBV	90489	176223	45.89%	5.252%
11	7.562	1924	1935	1949	rBV	43716	76312	19.87%	2.274%
12	7.893	2024	2038	2060	rBV	184753	328736	85.61%	9.798%
13	8.176	2116	2126	2141	rBV	25440	42868	11.16%	1.278%
14	8.468	2207	2217	2230	rBV4	5579	10266	2.67%	0.306%
15	8.549	2234	2242	2254	rVB5	4887	7558	1.97%	0.225%
16	8.632	2255	2268	2298	rBV	160244	310654	80.90%	9.259%
17	9.414	2494	2511	2528	rBV	216098	367441	95.69%	10.951%
18	10.751	2915	2927	2944	rBV	62826	104916	27.32%	3.127%
19	10.890	2960	2970	2981	rBV2	6940	11347	2.95%	0.338%
20	11.809	3243	3256	3279	rBV	220673	361883	94.24%	10.786%
21	12.189	3361	3374	3398	rBV	165590	272075	70.85%	8.109%




Sum of corrected areas: 3355189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053879.D
Acq On : 25 Apr 2023 13:14
Operator : JC/MD
Sample : VIBLK157
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

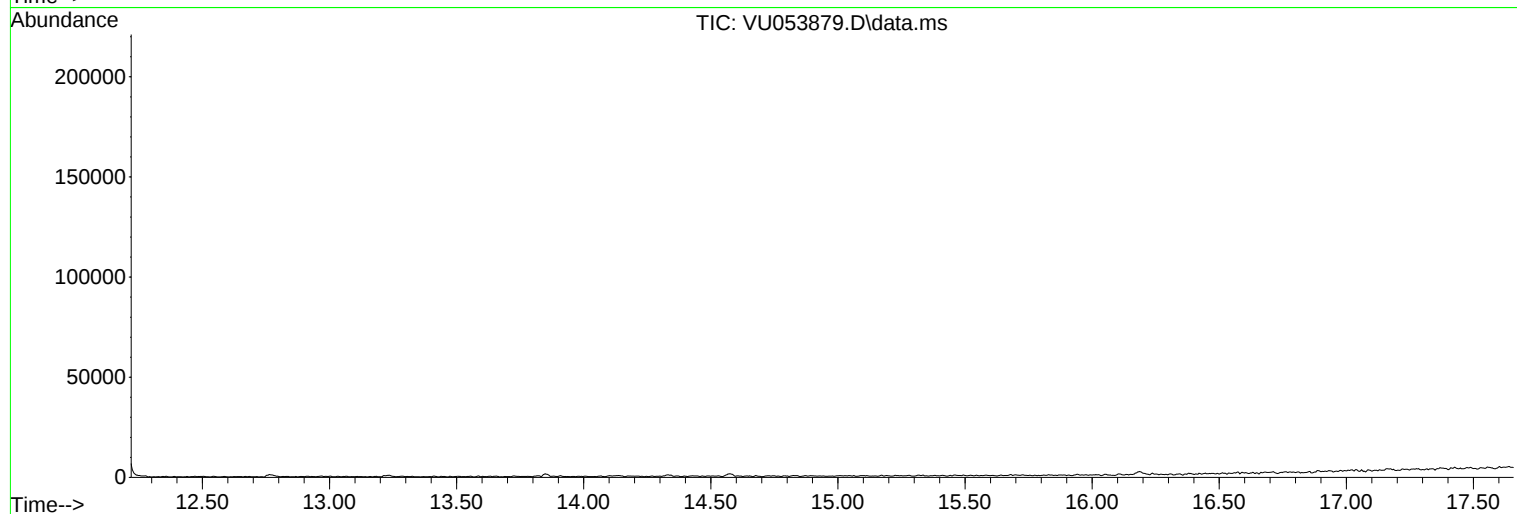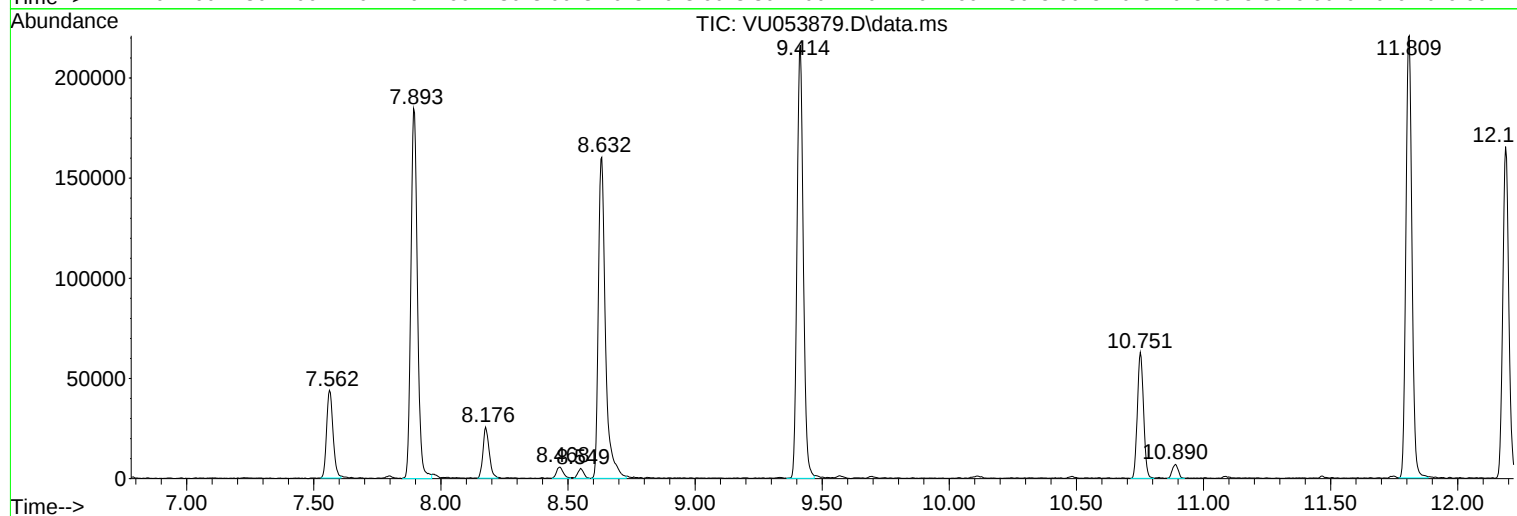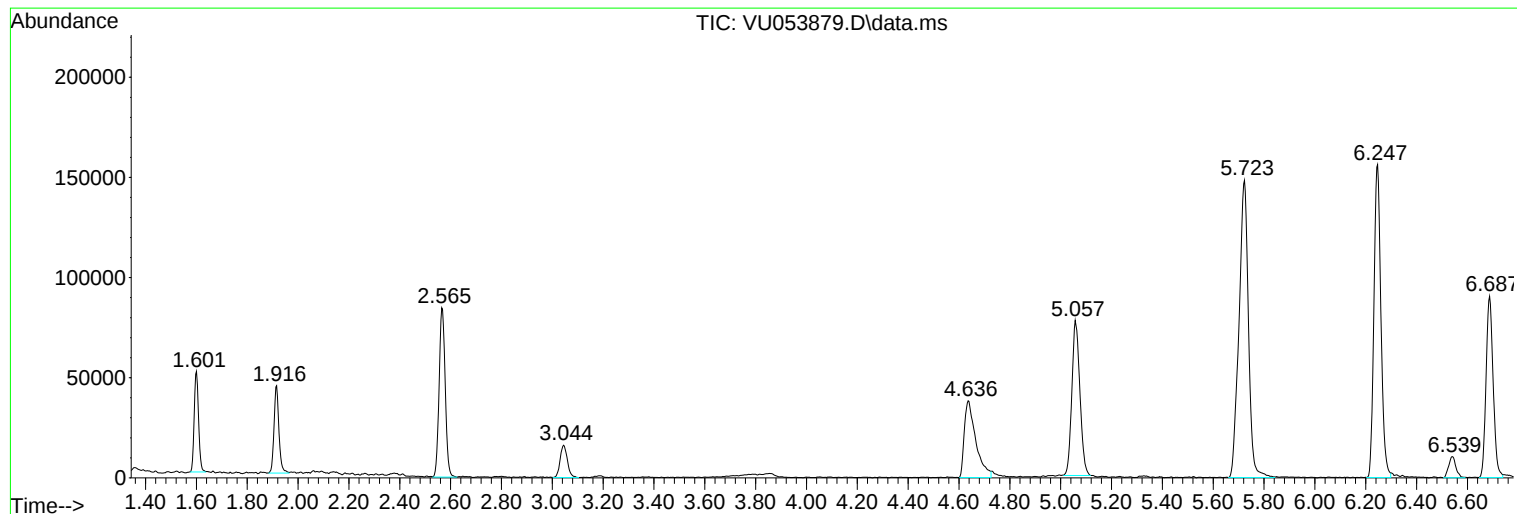

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053879.D
Acq On : 25 Apr 2023 13:14
Operator : JC/MD
Sample : VIBLK157
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053879.D
Acq On : 25 Apr 2023 13:14
Operator : JC/MD
Sample : VIBLK157
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK157

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------