

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
 Data File : VU053882.D
 Acq On : 25 Apr 2023 14:25
 Operator : JC/MD
 Sample : 02433-20 20X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE55

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053882.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rBV	46734	55621	9.65%	1.439%
2	1.912	171	178	192	rBV	41578	56548	9.81%	1.463%
3	2.565	368	381	395	rBV	81372	131990	22.91%	3.416%
4	3.044	519	530	542	rBV3	8517	15423	2.68%	0.399%
5	4.632	1012	1024	1054	rBV	43413	134247	23.30%	3.474%
6	5.057	1142	1156	1183	rVB	77948	172359	29.91%	4.461%
7	5.722	1342	1363	1386	rBV3	142436	373782	64.87%	9.673%
8	6.243	1510	1525	1551	rBV	151760	297446	51.62%	7.698%
9	6.539	1608	1617	1629	rBV4	10389	19516	3.39%	0.505%
10	6.687	1648	1663	1681	rBV	90137	176501	30.63%	4.568%
11	7.562	1922	1935	1955	rBV	42305	76161	13.22%	1.971%
12	7.893	2023	2038	2058	rBV	177128	313030	54.33%	8.101%
13	8.176	2116	2126	2141	rBV2	24445	41861	7.26%	1.083%
14	8.465	2209	2216	2229	rVB3	5710	9623	1.67%	0.249%
15	8.549	2229	2242	2257	rBV	336690	576216	100.00%	14.912%
16	8.629	2257	2267	2299	rVB	167688	315683	54.79%	8.170%
17	9.414	2498	2511	2542	rBV	215103	358715	62.25%	9.283%
18	10.751	2916	2927	2945	rVB	64385	107414	18.64%	2.780%
19	10.886	2961	2969	2982	rVB4	7419	12000	2.08%	0.311%
20	11.809	3244	3256	3277	rBV	214116	351283	60.96%	9.091%
21	12.188	3362	3374	3392	rBV	163301	268602	46.61%	6.951%




Sum of corrected areas: 3864021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053882.D
Acq On : 25 Apr 2023 14:25
Operator : JC/MD
Sample : 02433-20 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

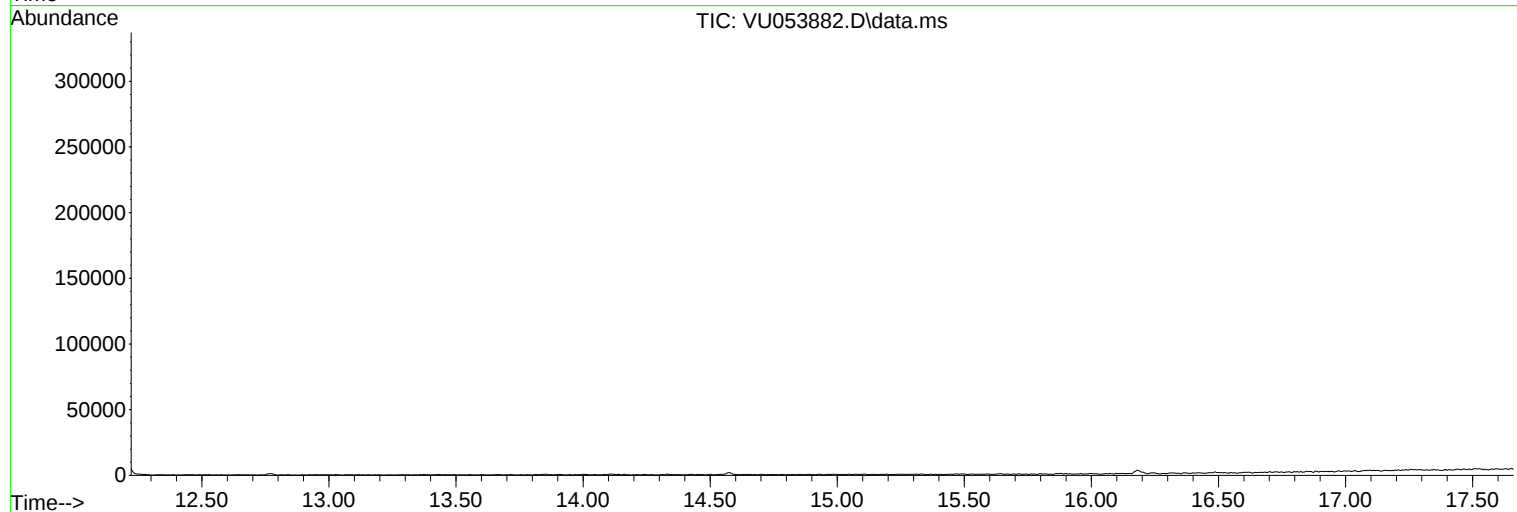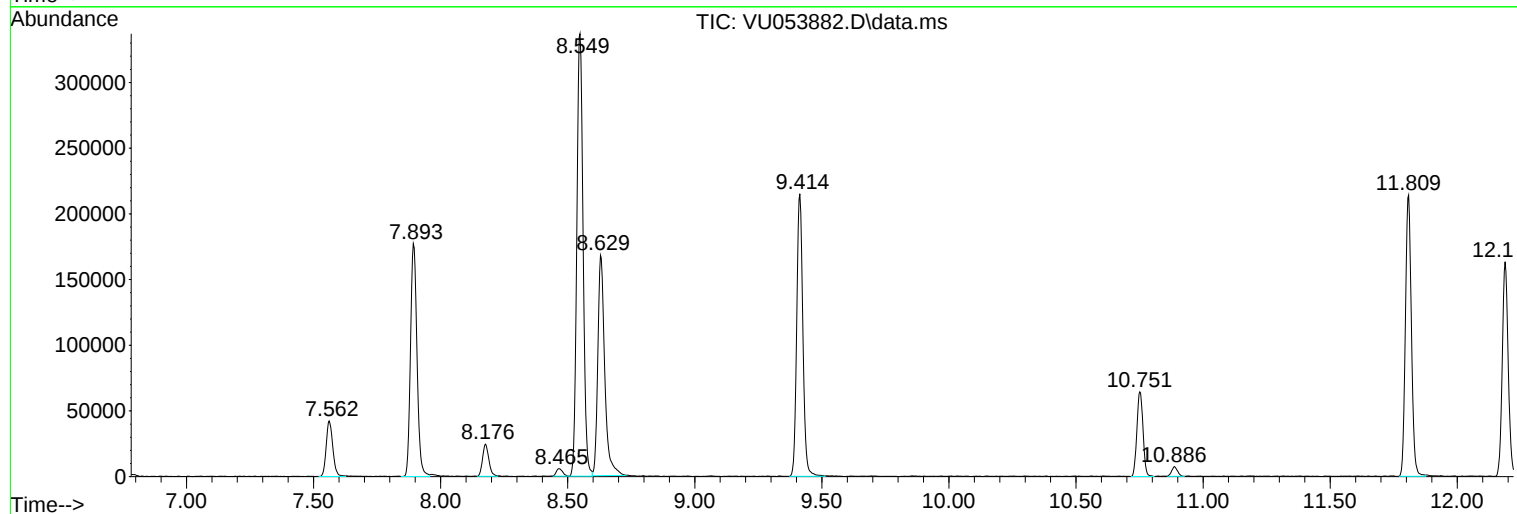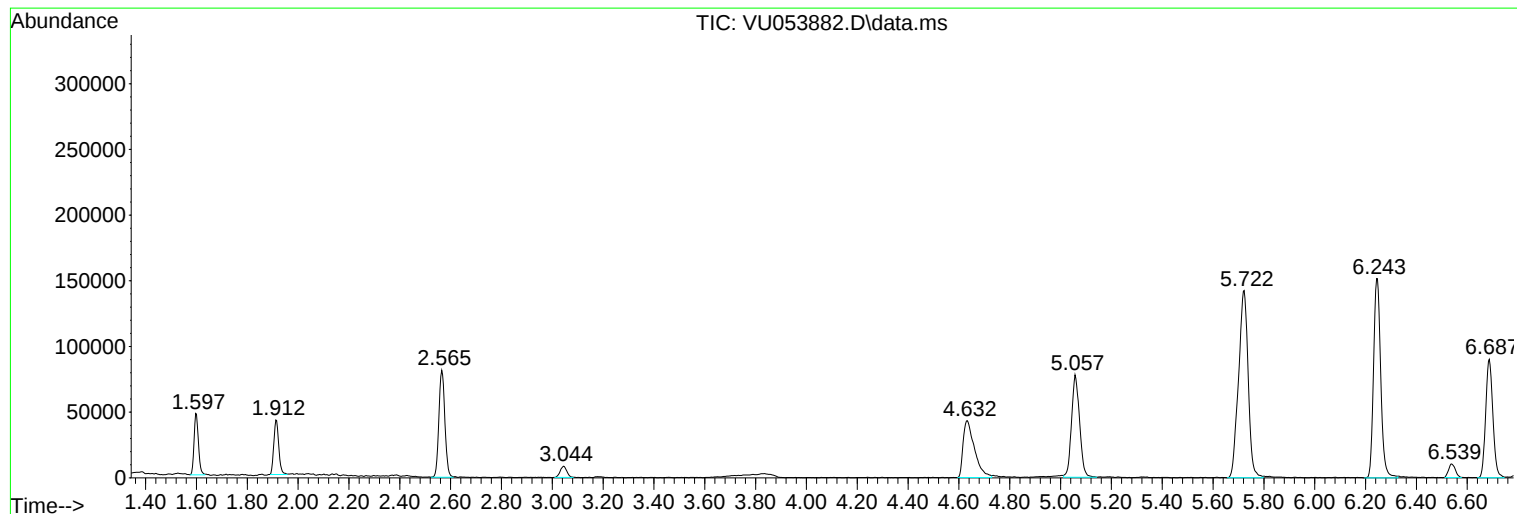

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053882.D
Acq On : 25 Apr 2023 14:25
Operator : JC/MD
Sample : 02433-20 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053882.D
Acq On : 25 Apr 2023 14:25
Operator : JC/MD
Sample : 02433-20 20X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE55

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc