

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
 Data File : VU053884.D
 Acq On : 25 Apr 2023 15:13
 Operator : JC/MD
 Sample : 02392-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE31

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053884.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	101	rVB	50549	61891	16.03%	1.840%
2	1.913	170	178	193	rBV	44131	59823	15.49%	1.779%
3	2.565	369	381	396	rBV	83171	135922	35.21%	4.042%
4	4.629	1012	1023	1052	rBV2	43357	125629	32.54%	3.736%
5	5.060	1142	1157	1176	rVB2	75891	172598	44.70%	5.132%
6	5.723	1342	1363	1384	rBV3	143503	366974	95.05%	10.912%
7	6.244	1513	1525	1553	rBV	169590	323875	83.89%	9.631%
8	6.687	1650	1663	1680	rBV	89108	174363	45.16%	5.185%
9	7.562	1922	1935	1955	rBV	42638	76508	19.82%	2.275%
10	7.893	2025	2038	2056	rBV	176771	308902	80.01%	9.185%
11	7.964	2056	2060	2077	rVB3	4404	8226	2.13%	0.245%
12	8.176	2112	2126	2144	rBV2	25311	43264	11.21%	1.286%
13	8.472	2201	2218	2228	rBV2	7093	13547	3.51%	0.403%
14	8.629	2254	2267	2301	rBV	167533	319932	82.87%	9.513%
15	9.414	2493	2511	2534	rBV	229209	385505	99.85%	11.463%
16	10.751	2916	2927	2943	rBV	66352	107328	27.80%	3.191%
17	10.890	2958	2970	2980	rBV3	11139	18691	4.84%	0.556%
18	11.809	3243	3256	3276	rBV	240303	386083	100.00%	11.480%
19	12.189	3360	3374	3392	rBV	165689	269975	69.93%	8.028%
20	16.179	4609	4615	4625	rVB5	2637	3925	1.02%	0.117%




Sum of corrected areas: 3362961

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053884.D
Acq On : 25 Apr 2023 15:13
Operator : JC/MD
Sample : 02392-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

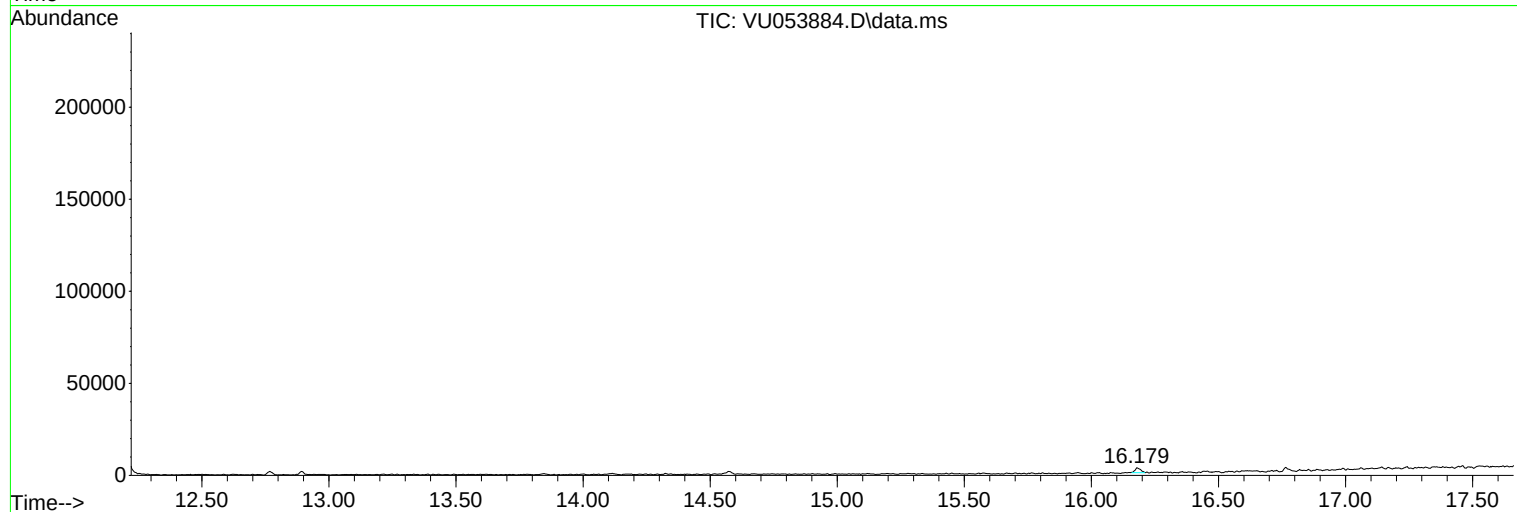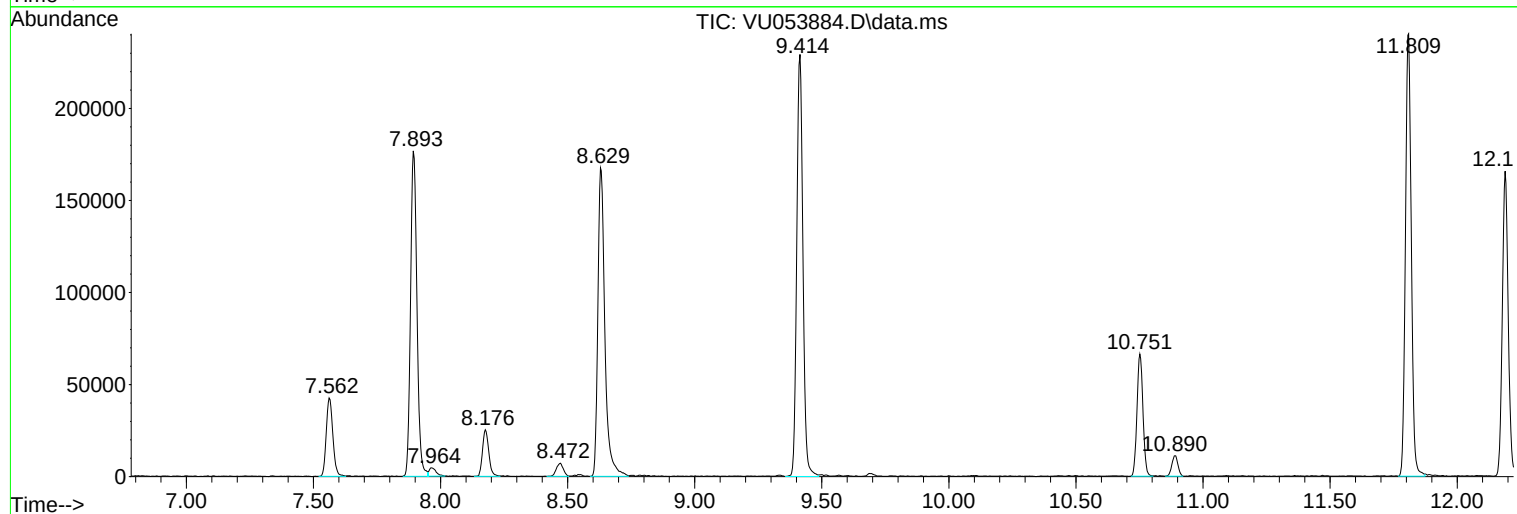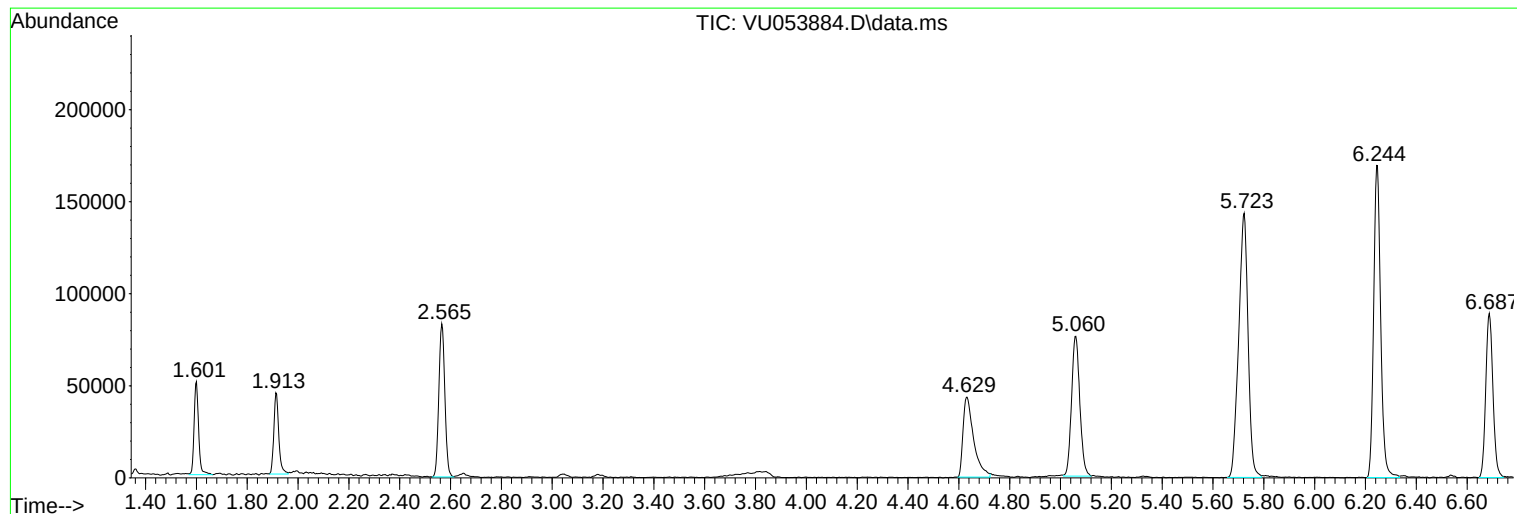

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053884.D
Acq On : 25 Apr 2023 15:13
Operator : JC/MD
Sample : 02392-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053884.D
Acq On : 25 Apr 2023 15:13
Operator : JC/MD
Sample : 02392-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc