

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
 Data File : VU053893.D
 Acq On : 25 Apr 2023 18:51
 Operator : JC/MD
 Sample : 02433-07DL 500X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE43DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053893.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	90	rBV	42595	51444	10.38%	1.388%
2	1.915	170	179	191	rBV	38649	53585	10.81%	1.446%
3	2.565	370	381	399	rVB	75107	124233	25.05%	3.352%
4	3.044	519	530	542	rVB3	8859	16964	3.42%	0.458%
5	4.636	1013	1025	1061	rBV	38797	125209	25.25%	3.378%
6	5.057	1141	1156	1177	rVB	75346	166127	33.50%	4.482%
7	5.722	1343	1363	1389	rBV2	139438	359525	72.51%	9.700%
8	6.243	1511	1525	1546	rBV	154982	300484	60.60%	8.107%
9	6.536	1605	1616	1631	rBV5	10572	19494	3.93%	0.526%
10	6.687	1650	1663	1681	rBV	86728	167674	33.82%	4.524%
11	7.562	1923	1935	1954	rBV2	41447	72593	14.64%	1.959%
12	7.893	2026	2038	2063	rBV	171968	303177	61.14%	8.180%
13	8.176	2116	2126	2142	rBV2	23938	41732	8.42%	1.126%
14	8.468	2206	2217	2227	rBV4	3882	6543	1.32%	0.177%
15	8.549	2227	2242	2257	rVV	297104	495843	100.00%	13.378%
16	8.629	2257	2267	2304	rVB	163667	313572	63.24%	8.461%
17	9.414	2494	2511	2532	rBV	218787	364625	73.54%	9.838%
18	10.751	2915	2927	2942	rBV2	64364	103253	20.82%	2.786%
19	10.889	2962	2970	2978	rVB3	5045	7090	1.43%	0.191%
20	11.806	3244	3255	3279	rBV	216137	353206	71.23%	9.530%
21	12.188	3362	3374	3393	rBV	158413	259910	52.42%	7.013%




Sum of corrected areas: 3706283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053893.D
Acq On : 25 Apr 2023 18:51
Operator : JC/MD
Sample : 02433-07DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

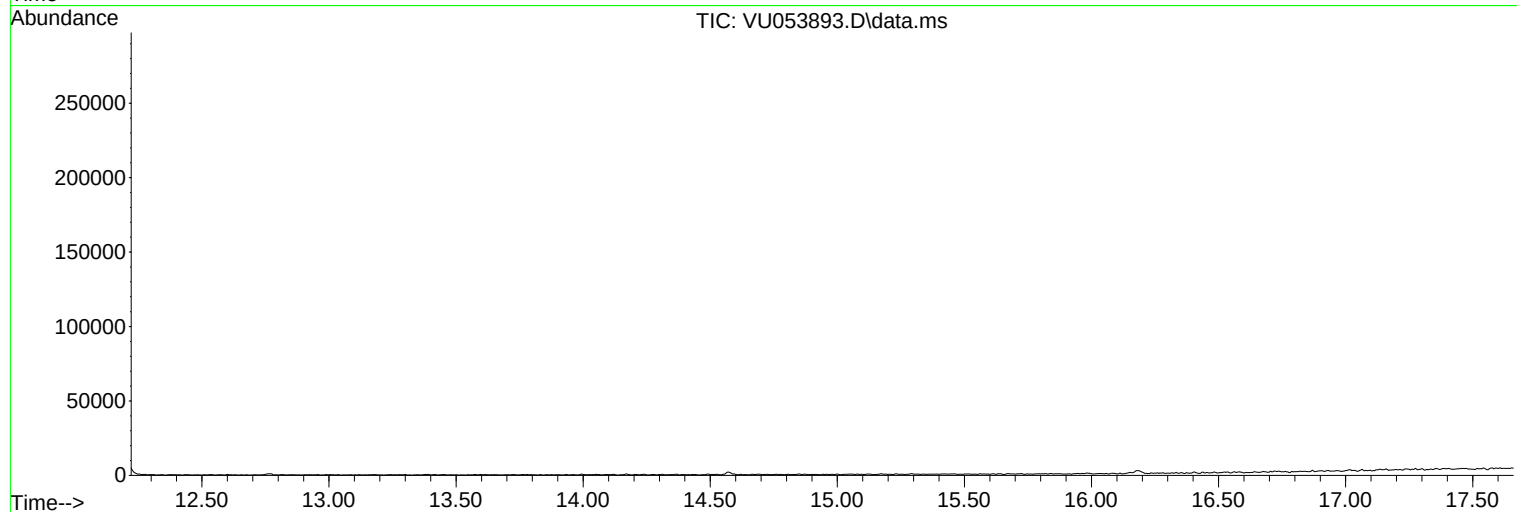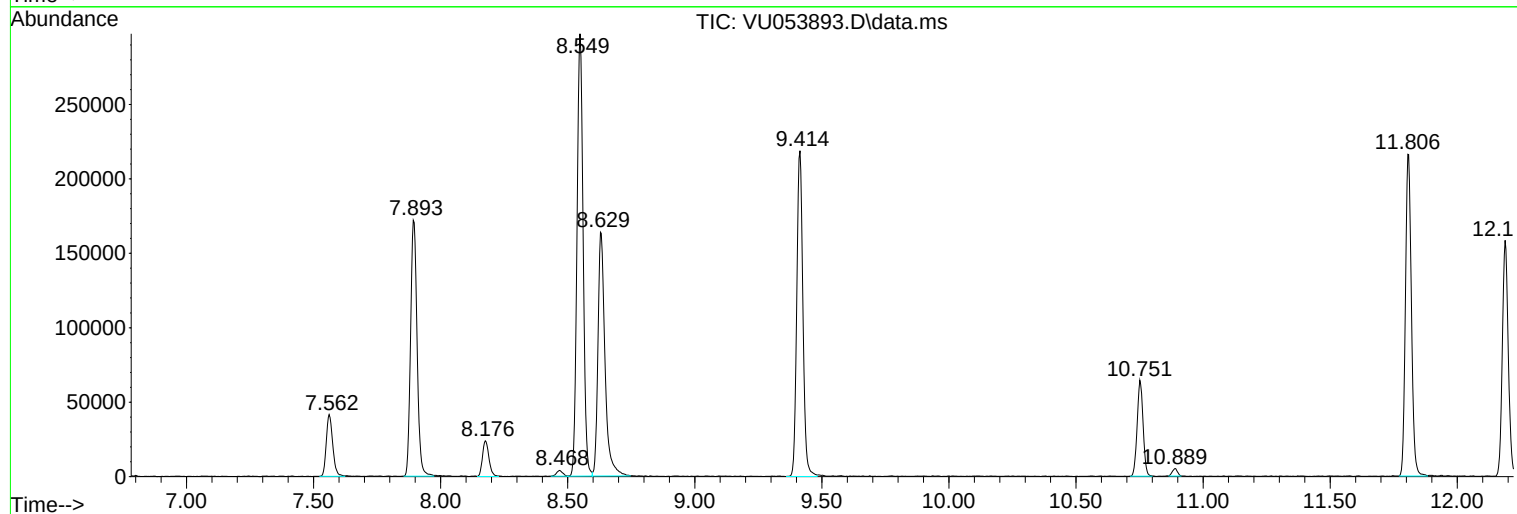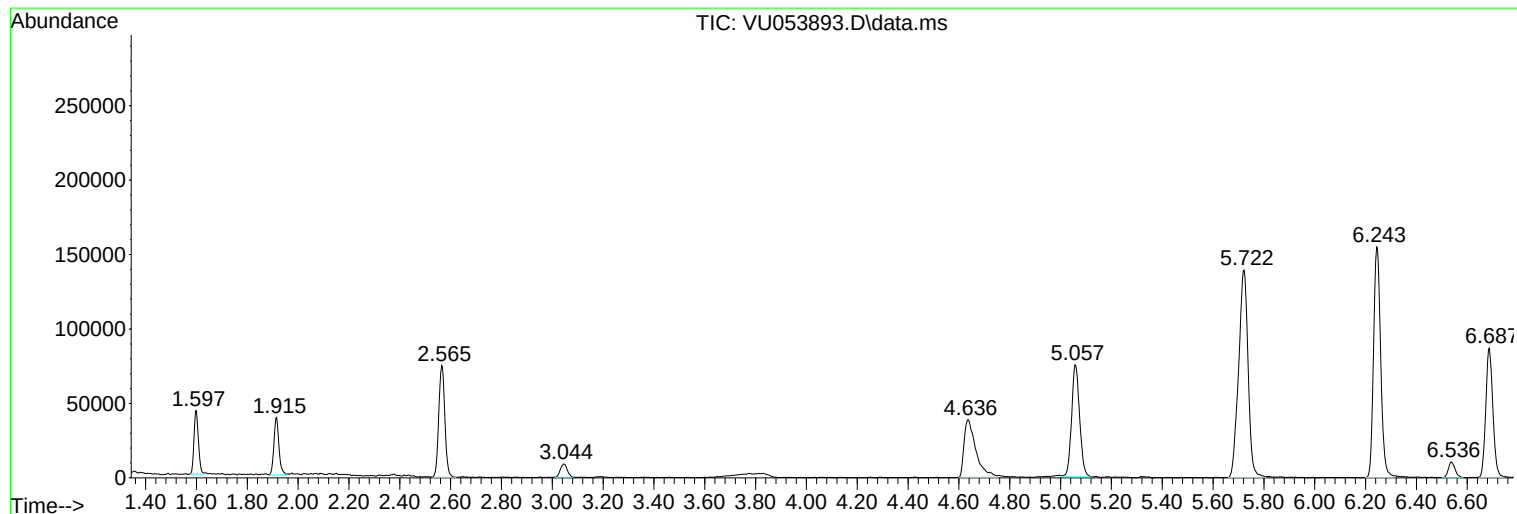

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053893.D
Acq On : 25 Apr 2023 18:51
Operator : JC/MD
Sample : 02433-07DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
Data File : VU053893.D
Acq On : 25 Apr 2023 18:51
Operator : JC/MD
Sample : 02433-07DL 500X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE43DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------