
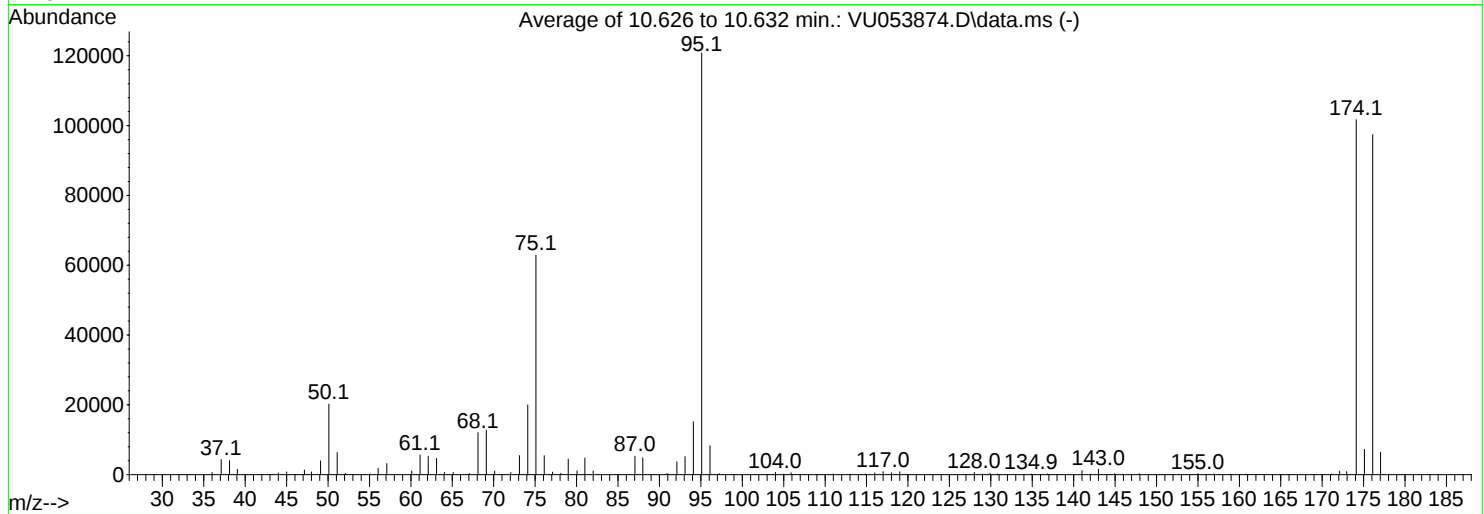


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042523\
 Data File : VU053874.D
 Acq On : 25 Apr 2023 10:04
 Operator : JC/MD
 Sample : BFB008
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB008

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Apr 27 05:52:18 2023

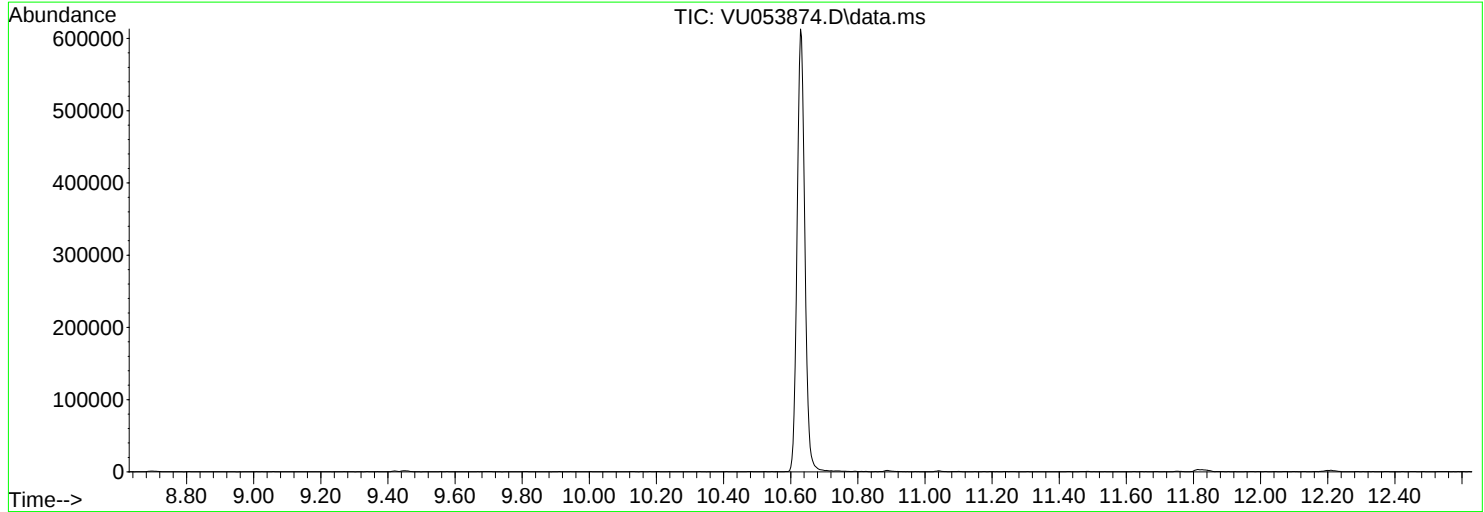

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	20205	PASS
75	95	30	80	52.0	62851	PASS
95	95	100	100	100.0	120843	PASS
96	95	5	9	6.9	8311	PASS
173	174	0.00	2	0.9	875	PASS
174	95	50	120	84.2	101712	PASS
175	174	5	9	7.1	7227	PASS
176	174	95	101	95.8	97435	PASS
177	176	5	9	6.6	6407	PASS

m/z	Abundance
39.90	128.0
44.00	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
36.00	721.0
37.10	4155.0
38.10	4038.0
39.00	1438.0
44.00	657.0
45.00	772.0
46.00	162.0
47.10	1257.0
48.00	778.0
49.10	4013.0
50.10	20120.0
51.10	6139.0
52.10	391.0
55.00	256.0
56.00	1788.0
57.10	3333.0
60.10	1050.0
61.10	5401.0
62.10	5201.0
63.10	4489.0
64.00	759.0
65.10	677.0
67.10	309.0
68.10	11494.0
69.10	12220.0
70.10	1071.0
72.20	541.0
73.10	5226.0
74.10	19480.0
75.10	60688.0
76.10	5086.0
77.10	801.0
78.10	392.0
79.00	4335.0
80.10	1069.0
81.00	4691.0
82.00	1059.0
83.00	103.0
87.00	5136.0
88.00	4308.0
90.90	458.0
92.10	3543.0
93.10	4849.0
94.10	14155.0
95.10	115096.0
96.10	8147.0
97.20	284.0
104.00	664.0
105.00	184.0
105.90	537.0
107.00	178.0
110.90	127.0
113.00	138.0
114.90	167.0
116.00	539.0
117.00	843.0
118.00	537.0
119.00	742.0
128.00	615.0
129.00	265.0
129.90	370.0
130.90	151.0
134.90	164.0
136.80	212.0
141.00	1122.0
142.00	205.0
143.00	1334.0
144.90	231.0
146.00	173.0
147.90	289.0
150.20	122.0
153.10	118.0
155.00	308.0
157.00	231.0
158.90	151.0
160.90	174.0
171.10	136.0
172.10	904.0
172.90	802.0
174.10	94032.0
175.10	7123.0
176.10	90128.0
177.00	5920.0
178.00	223.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
36.00	669.0
37.10	4534.0
38.10	4182.0
39.00	1620.0
40.20	113.0
44.00	731.0
45.00	778.0
46.10	113.0
47.20	1426.0
48.00	838.0
49.10	4039.0
50.10	21016.0
51.10	6600.0
52.10	397.0
55.00	270.0
56.10	1955.0
57.10	3222.0
60.10	1119.0
61.10	5849.0
62.10	5407.0
63.10	4731.0
64.10	705.0
65.10	661.0
66.00	114.0
67.00	309.0
68.10	12495.0
69.10	13317.0
70.10	1114.0
72.00	600.0
73.10	5623.0
74.10	20552.0
75.10	65176.0
76.10	5659.0
77.10	739.0
78.10	431.0
79.00	4597.0
80.00	1099.0
81.00	4908.0
82.00	1135.0
83.00	112.0
87.10	5537.0
88.00	4896.0
90.90	467.0
92.10	3743.0
93.10	5286.0
94.10	15851.0
95.10	124880.0
96.10	8673.0
97.20	342.0
104.00	670.0
105.00	205.0
105.90	562.0
107.00	157.0
110.90	191.0
113.00	125.0
114.90	180.0
116.00	599.0
117.00	923.0
118.00	582.0
119.00	890.0
128.00	688.0
129.00	245.0
129.90	423.0
130.90	162.0
134.90	169.0
136.80	238.0
141.00	1172.0
142.00	174.0
143.00	1579.0
145.00	302.0
145.90	187.0
147.90	273.0
149.90	153.0
153.00	138.0
154.10	107.0
155.00	338.0
156.90	212.0
158.90	165.0
160.90	202.0
171.10	186.0
172.10	1057.0
172.90	936.0
174.10	104896.0
175.10	7502.0
176.10	100984.0
177.10	6654.0
178.00	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
36.00	600.0
37.10	4362.0
38.10	3910.0
39.10	1552.0
40.20	127.0
44.10	888.0
45.00	814.0
47.20	1282.0
48.00	774.0
49.10	3769.0
50.10	19480.0
51.10	6377.0
52.10	323.0
55.10	237.0
56.10	1818.0
57.10	2977.0
58.10	119.0
60.10	1056.0
61.10	5769.0
62.10	5265.0
63.10	4642.0
64.10	532.0
65.10	599.0
66.00	112.0
67.00	308.0
68.10	12182.0
69.10	12698.0
70.10	1008.0
72.00	629.0
73.10	5474.0
74.10	19888.0
75.10	62688.0
76.10	5634.0
77.10	599.0
78.10	403.0
79.00	4368.0
80.00	1091.0
81.00	4744.0
82.00	996.0
82.90	113.0
86.10	148.0
87.10	5120.0
88.00	5218.0
91.10	470.0
92.10	3668.0
93.10	5356.0
94.10	15578.0
95.10	122552.0
96.10	8114.0
97.20	305.0
104.00	579.0
105.00	214.0
105.90	529.0
107.00	116.0
111.00	187.0
113.10	113.0
114.90	154.0
116.00	574.0
117.00	919.0
118.00	550.0
119.00	812.0
128.00	592.0
129.00	246.0
129.90	428.0
130.80	181.0
134.90	230.0
136.90	228.0
140.00	123.0
141.00	1265.0
142.00	128.0
143.00	1624.0
145.00	320.0
145.90	190.0
147.90	245.0
149.90	217.0
153.00	150.0
155.00	303.0
157.00	215.0
158.90	137.0
160.90	220.0
171.20	176.0
172.10	1043.0
173.00	886.0
174.10	106208.0
175.10	7056.0
176.10	101192.0
177.10	6648.0
178.10	146.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008