


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042524\
Data File : VU058796.D
Acq On : 25 Apr 2024 09:37
Operator : MD/SY
Sample : BFB149
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB149

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Apr 26 02:12:29 2024

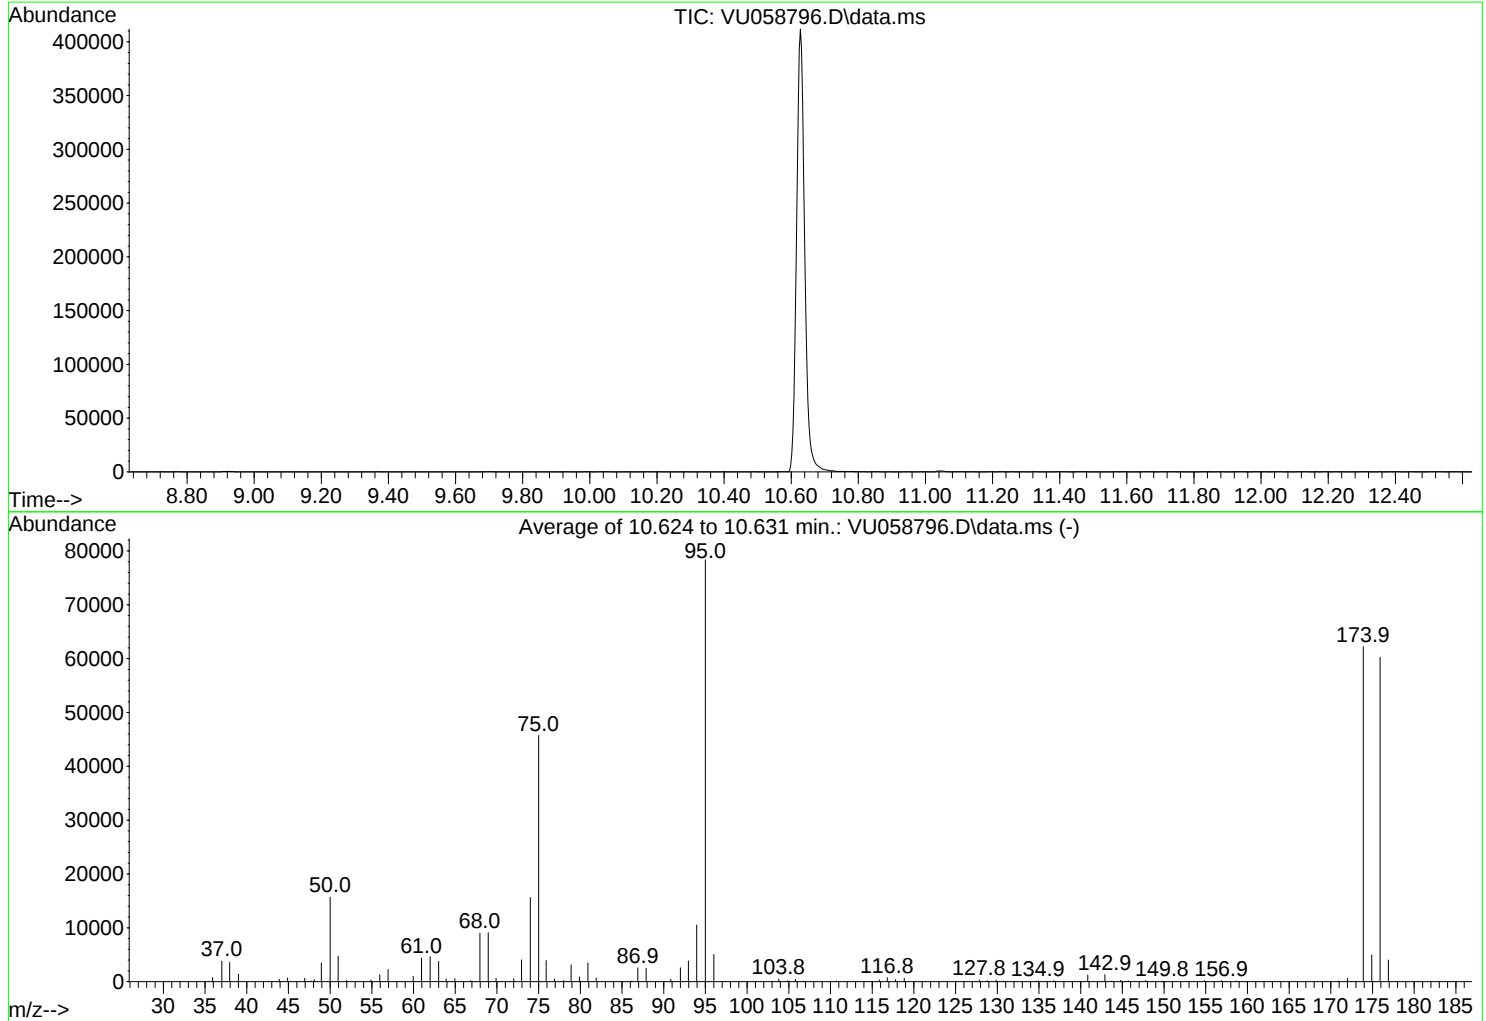

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.0	15708	PASS
75	95	30	80	58.3	45707	PASS
95	95	100	100	100.0	78357	PASS
96	95	5	9	6.4	5046	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.4	62224	PASS
175	174	5	9	8.0	4954	PASS
176	174	95	101	96.8	60240	PASS
177	176	5	9	6.6	4000	PASS

m/z	Abundance
43.90	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	769.0
37.00	3891.0
38.00	3558.0
39.00	1429.0
43.90	539.0
44.90	704.0
46.90	664.0
48.10	442.0
48.90	3579.0
50.00	15557.0
51.00	4836.0
52.00	234.0
54.90	294.0
55.90	1402.0
56.90	2249.0
57.90	100.0
60.00	883.0
60.90	4361.0
62.00	4538.0
63.00	3895.0
63.90	498.0
65.00	585.0
66.90	205.0
68.00	9147.0
68.90	8843.0
69.90	705.0
72.00	504.0
72.90	4103.0
74.00	15549.0
75.00	44880.0
75.90	3966.0
76.90	524.0
78.00	281.0
78.90	3079.0
79.90	767.0
80.90	3468.0
81.90	649.0
86.90	2443.0
87.90	2331.0
90.80	438.0
92.00	2609.0
93.00	3750.0
94.00	10571.0
95.00	77080.0
96.00	5090.0
97.00	113.0
103.80	451.0
104.90	144.0
105.80	404.0
106.80	108.0
110.70	139.0
115.80	306.0
116.80	710.0
117.80	354.0
118.90	571.0
127.90	340.0
128.80	160.0
129.90	280.0
130.80	119.0
134.70	173.0
136.80	177.0
140.80	1242.0
142.90	1268.0
143.70	101.0
144.90	217.0
145.80	163.0
147.80	231.0
154.80	202.0
156.90	252.0
158.70	124.0
160.90	132.0
170.90	120.0
172.00	624.0
173.90	60944.0
174.90	4727.0
175.90	58008.0
176.90	4019.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	769.0
37.00	3891.0
38.00	3558.0
39.00	1429.0
43.90	539.0
44.90	704.0
46.90	664.0
48.10	442.0
48.90	3579.0
50.00	15557.0
51.00	4836.0
52.00	234.0
54.90	294.0
55.90	1402.0
56.90	2249.0
57.90	100.0
60.00	883.0
60.90	4361.0
62.00	4538.0
63.00	3895.0
63.90	498.0
65.00	585.0
66.90	205.0
68.00	9147.0
68.90	8843.0
69.90	705.0
72.00	504.0
72.90	4103.0
74.00	15549.0
75.00	44880.0
75.90	3966.0
76.90	524.0
78.00	281.0
78.90	3079.0
79.90	767.0
80.90	3468.0
81.90	649.0
86.90	2443.0
87.90	2331.0
90.80	438.0
92.00	2609.0
93.00	3750.0
94.00	10571.0
95.00	77080.0
96.00	5090.0
97.00	113.0
103.80	451.0
104.90	144.0
105.80	404.0
106.80	108.0
110.70	139.0
115.80	306.0
116.80	710.0
117.80	354.0
118.90	571.0
127.90	340.0
128.80	160.0
129.90	280.0
130.80	119.0
134.70	173.0
136.80	177.0
140.80	1242.0
142.90	1268.0
143.70	101.0
144.90	217.0
145.80	163.0
147.80	231.0
154.80	202.0
156.90	252.0
158.70	124.0
160.90	132.0
170.90	120.0
172.00	624.0
173.90	60944.0
174.90	4727.0
175.90	58008.0
176.90	4019.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	785.0
37.00	3937.0
38.00	3642.0
39.00	1410.0
43.90	595.0
44.90	686.0
46.90	662.0
48.10	384.0
49.00	3560.0
50.00	16134.0
50.90	4922.0
52.00	226.0
54.90	295.0
55.90	1300.0
57.00	2316.0
58.00	101.0
59.90	1012.0
61.00	4475.0
62.00	4739.0
63.00	3833.0
63.90	523.0
65.00	578.0
66.80	195.0
68.00	9257.0
68.90	9422.0
69.90	639.0
72.00	550.0
73.00	4181.0
74.00	16130.0
75.00	47184.0
75.90	4001.0
76.90	483.0
78.00	308.0
78.90	3160.0
79.90	876.0
80.90	3607.0
81.90	708.0
86.10	191.0
86.90	2680.0
87.90	2546.0
90.90	440.0
92.00	2671.0
93.00	3911.0
94.00	10823.0
95.00	80984.0
96.00	5150.0
103.80	495.0
104.80	121.0
105.00	120.0
105.80	417.0
106.70	120.0
110.70	143.0
115.80	335.0
116.80	775.0
117.80	414.0
118.80	668.0
127.80	352.0
128.80	202.0
129.80	289.0
130.80	136.0
134.90	237.0
136.80	200.0
140.90	1294.0
142.90	1346.0
143.80	130.0
144.80	244.0
145.80	164.0
147.80	235.0
149.80	127.0
154.90	229.0
156.90	231.0
158.70	140.0
160.90	127.0
170.90	120.0
172.00	637.0
173.90	64096.0
174.90	5127.0
175.90	62264.0
176.90	4140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
35.90	745.0
37.00	3571.0
37.90	3525.0
39.00	1299.0
43.90	608.0
44.90	686.0
47.00	566.0
47.70	339.0
48.10	312.0
49.00	3316.0
50.00	15432.0
51.00	4478.0
51.90	223.0
54.90	302.0
56.00	1133.0
56.90	2252.0
59.90	1063.0
61.00	4278.0
62.00	4621.0
63.00	3468.0
63.90	507.0
64.90	541.0
66.80	184.0
67.90	8565.0
69.00	9059.0
69.90	528.0
72.00	518.0
73.00	3854.0
74.00	15262.0
75.00	45056.0
75.90	3798.0
76.90	385.0
78.90	3110.0
79.90	927.0
80.90	3408.0
81.90	740.0
86.10	178.0
86.90	2587.0
87.90	2513.0
90.90	416.0
92.00	2480.0
92.90	3838.0
93.90	10204.0
95.00	77008.0
96.00	4897.0
103.80	493.0
104.80	124.0
105.80	407.0
106.70	115.0
110.70	122.0
115.90	367.0
116.80	749.0
117.80	407.0
118.80	679.0
127.80	333.0
128.80	208.0
129.80	293.0
130.70	133.0
134.90	252.0
136.80	187.0
140.90	1168.0
142.90	1344.0
143.80	117.0
144.70	265.0
145.70	148.0
147.80	216.0
149.80	144.0
154.90	226.0
156.90	178.0
158.70	137.0
172.00	558.0
173.90	61632.0
174.90	5008.0
175.90	60448.0
176.90	3840.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149