



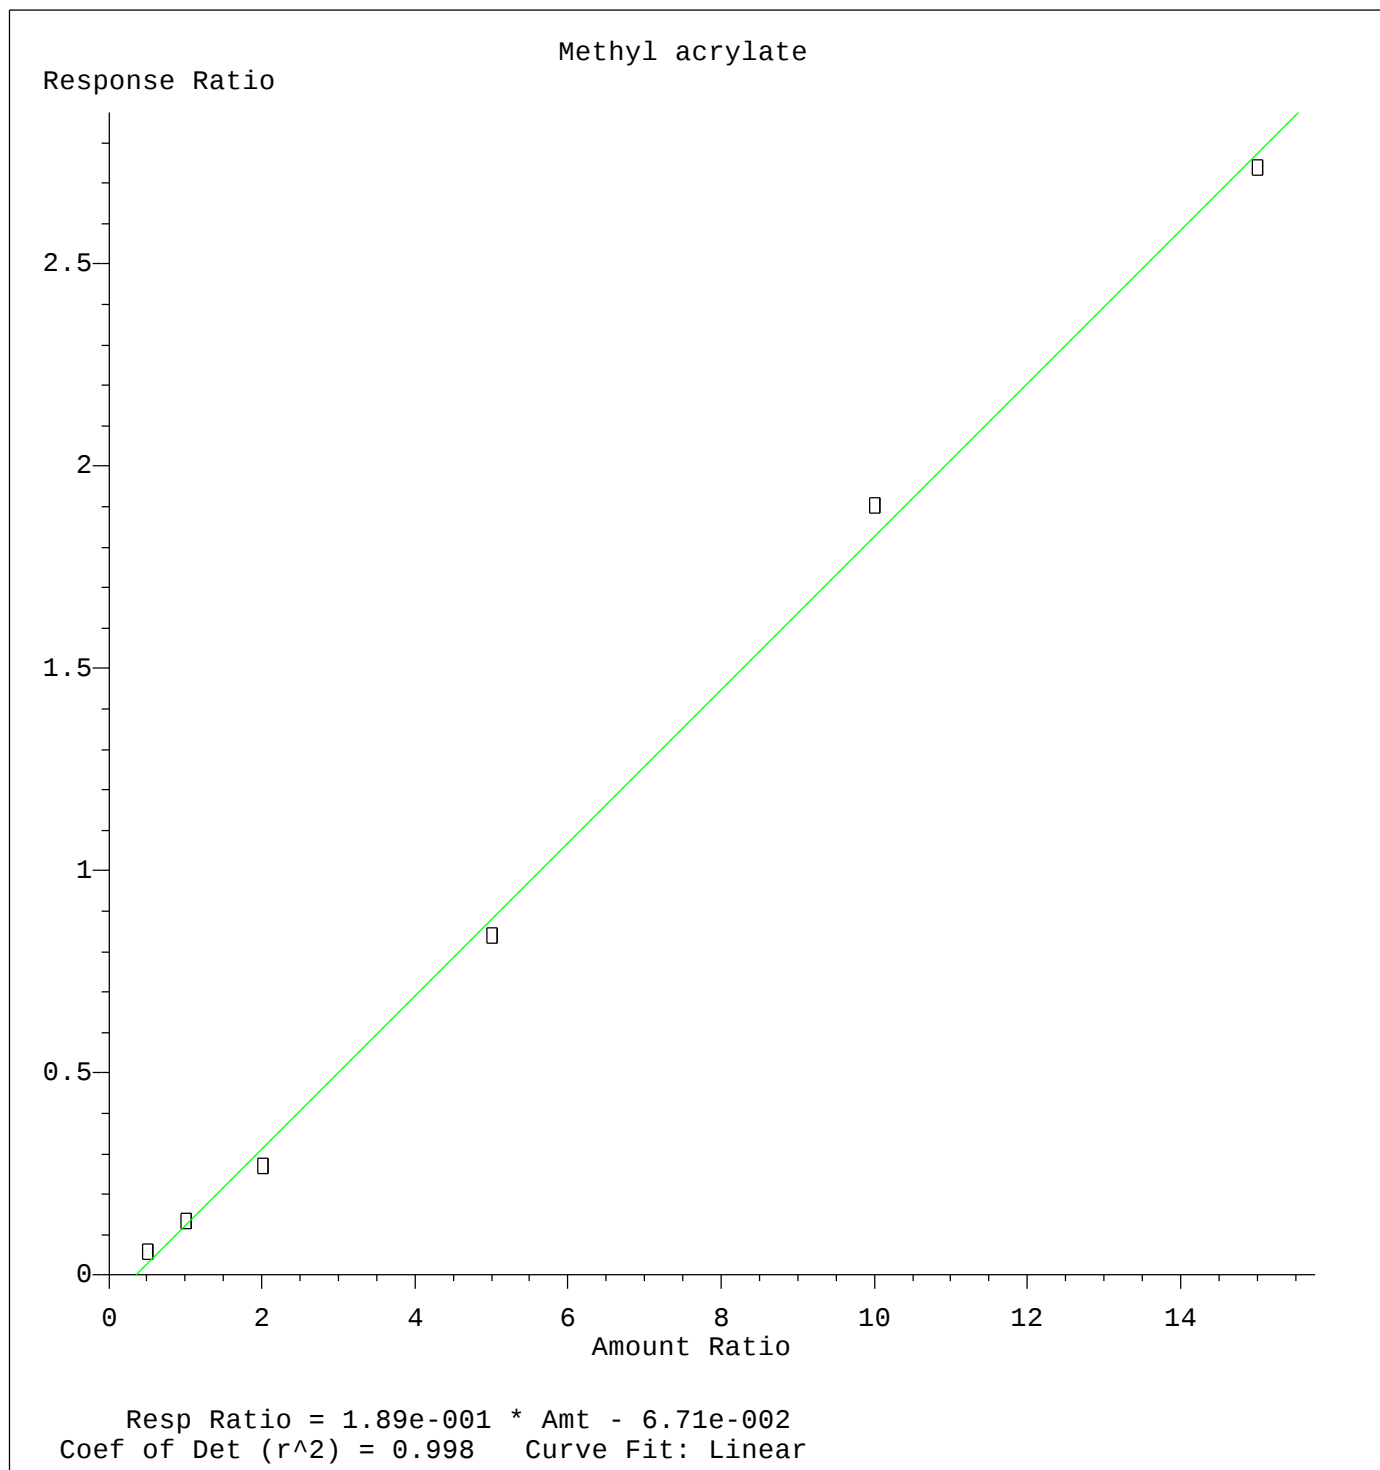

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019

Styrene

Response Ratio

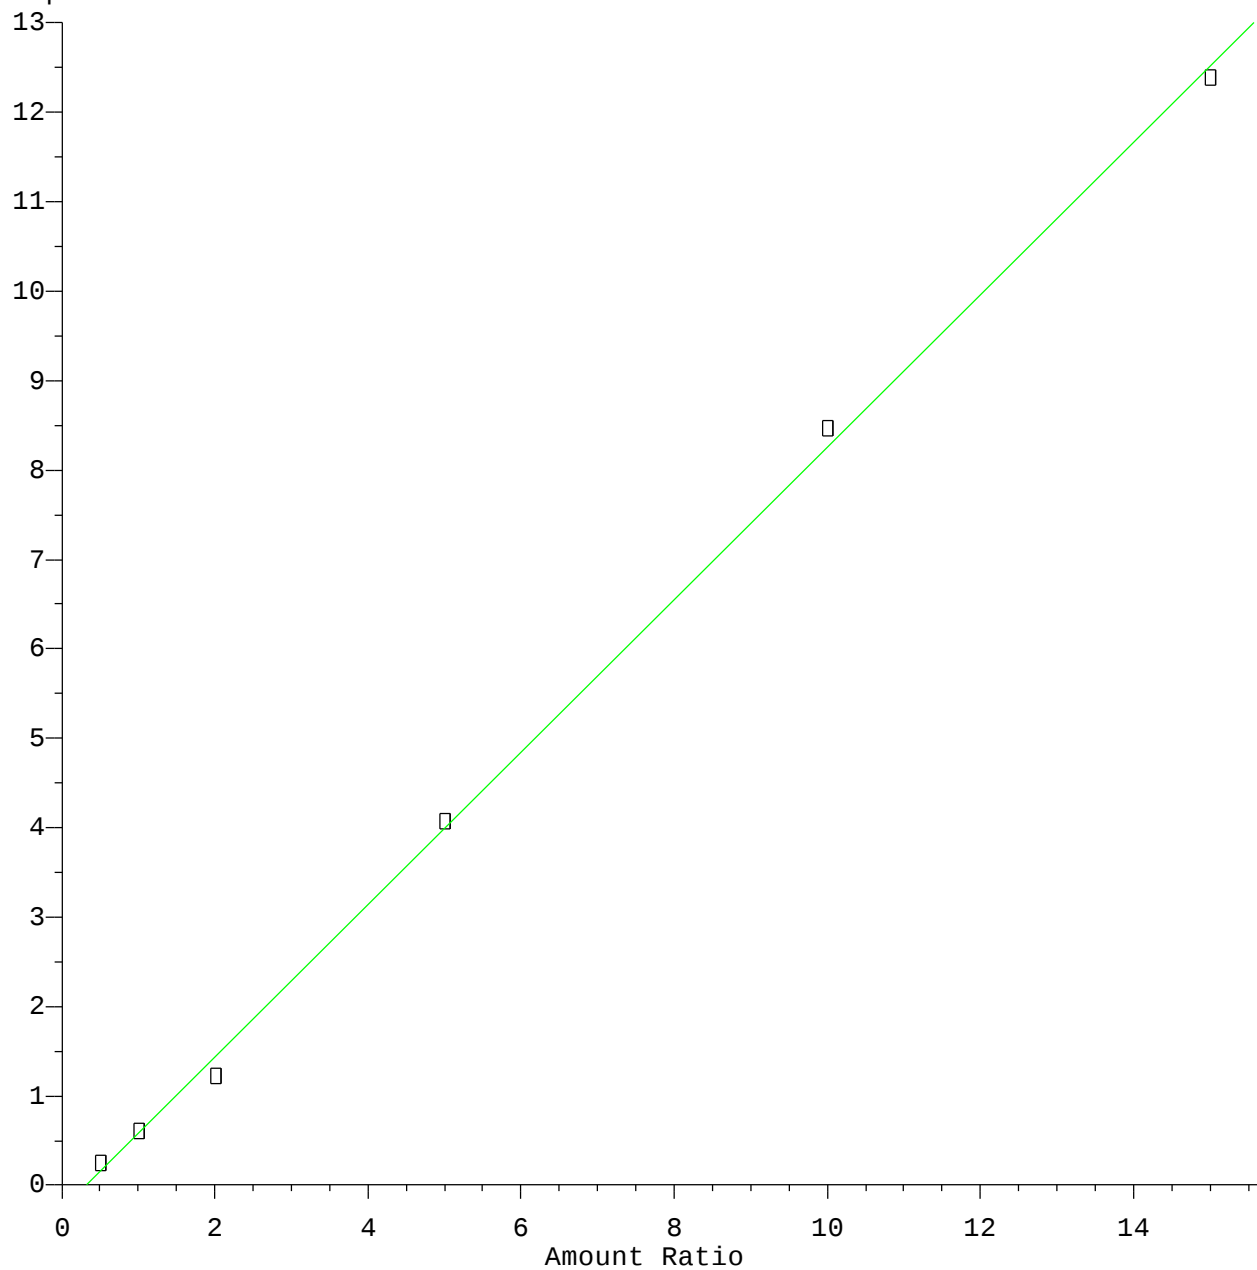


Resp Ratio = $8.52 \times 10^{-1} \times \text{Amt} - 2.61 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019


1,3,5-Trimethylbenzene

Response Ratio

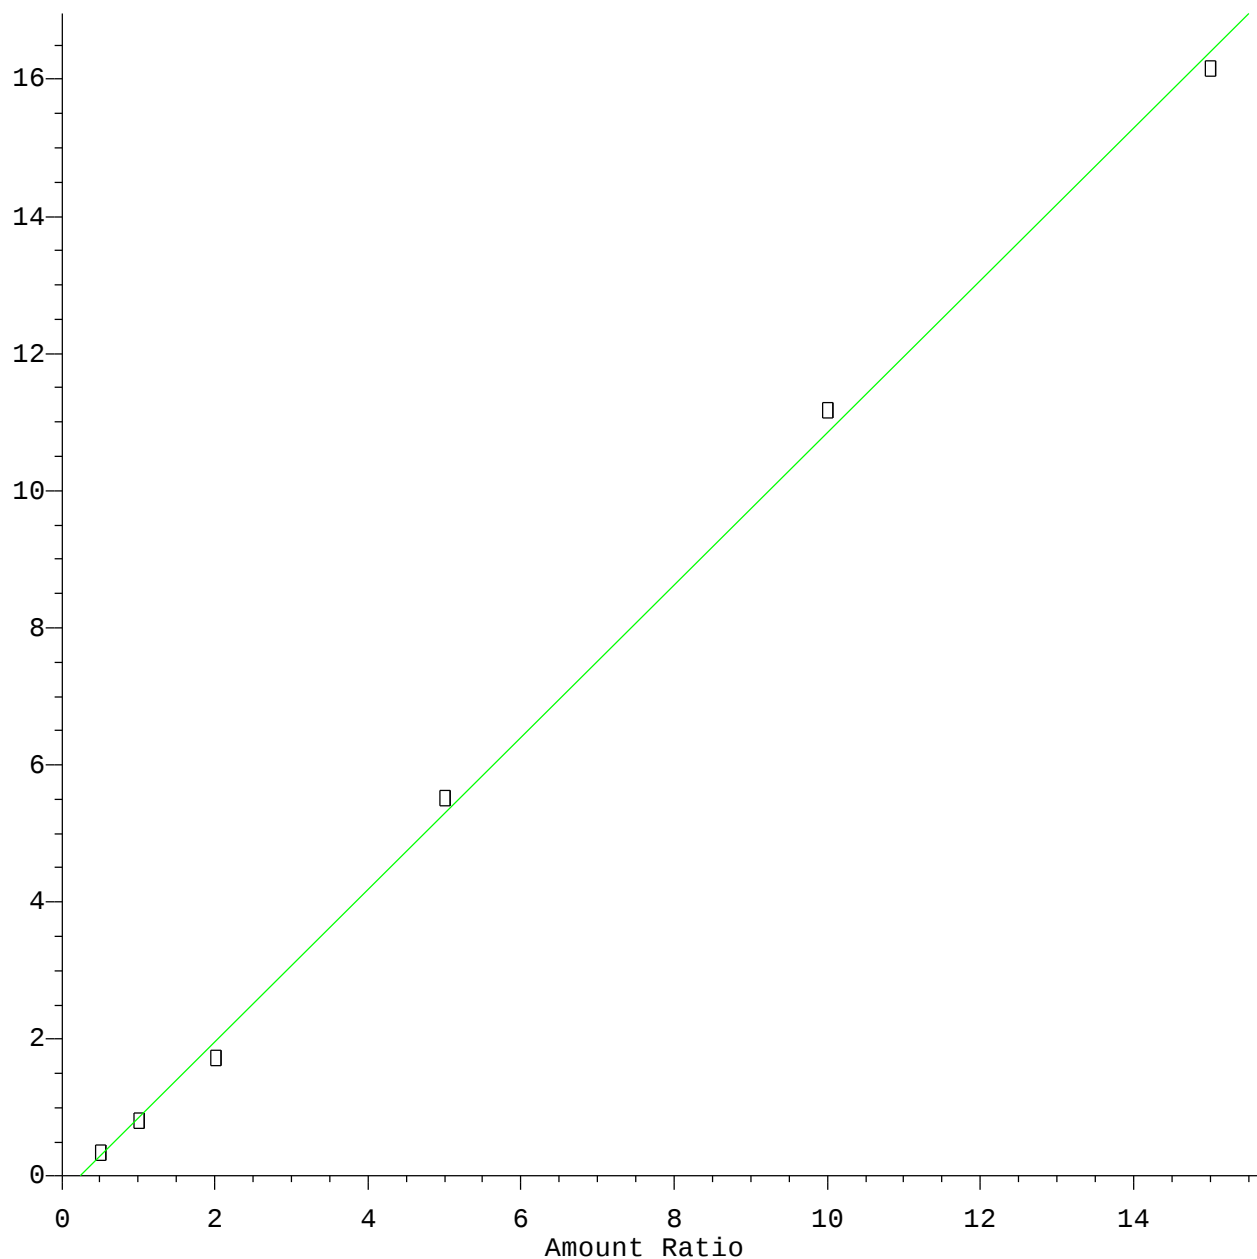

Resp Ratio = 1.11×10^0 * Amt - 2.50×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019

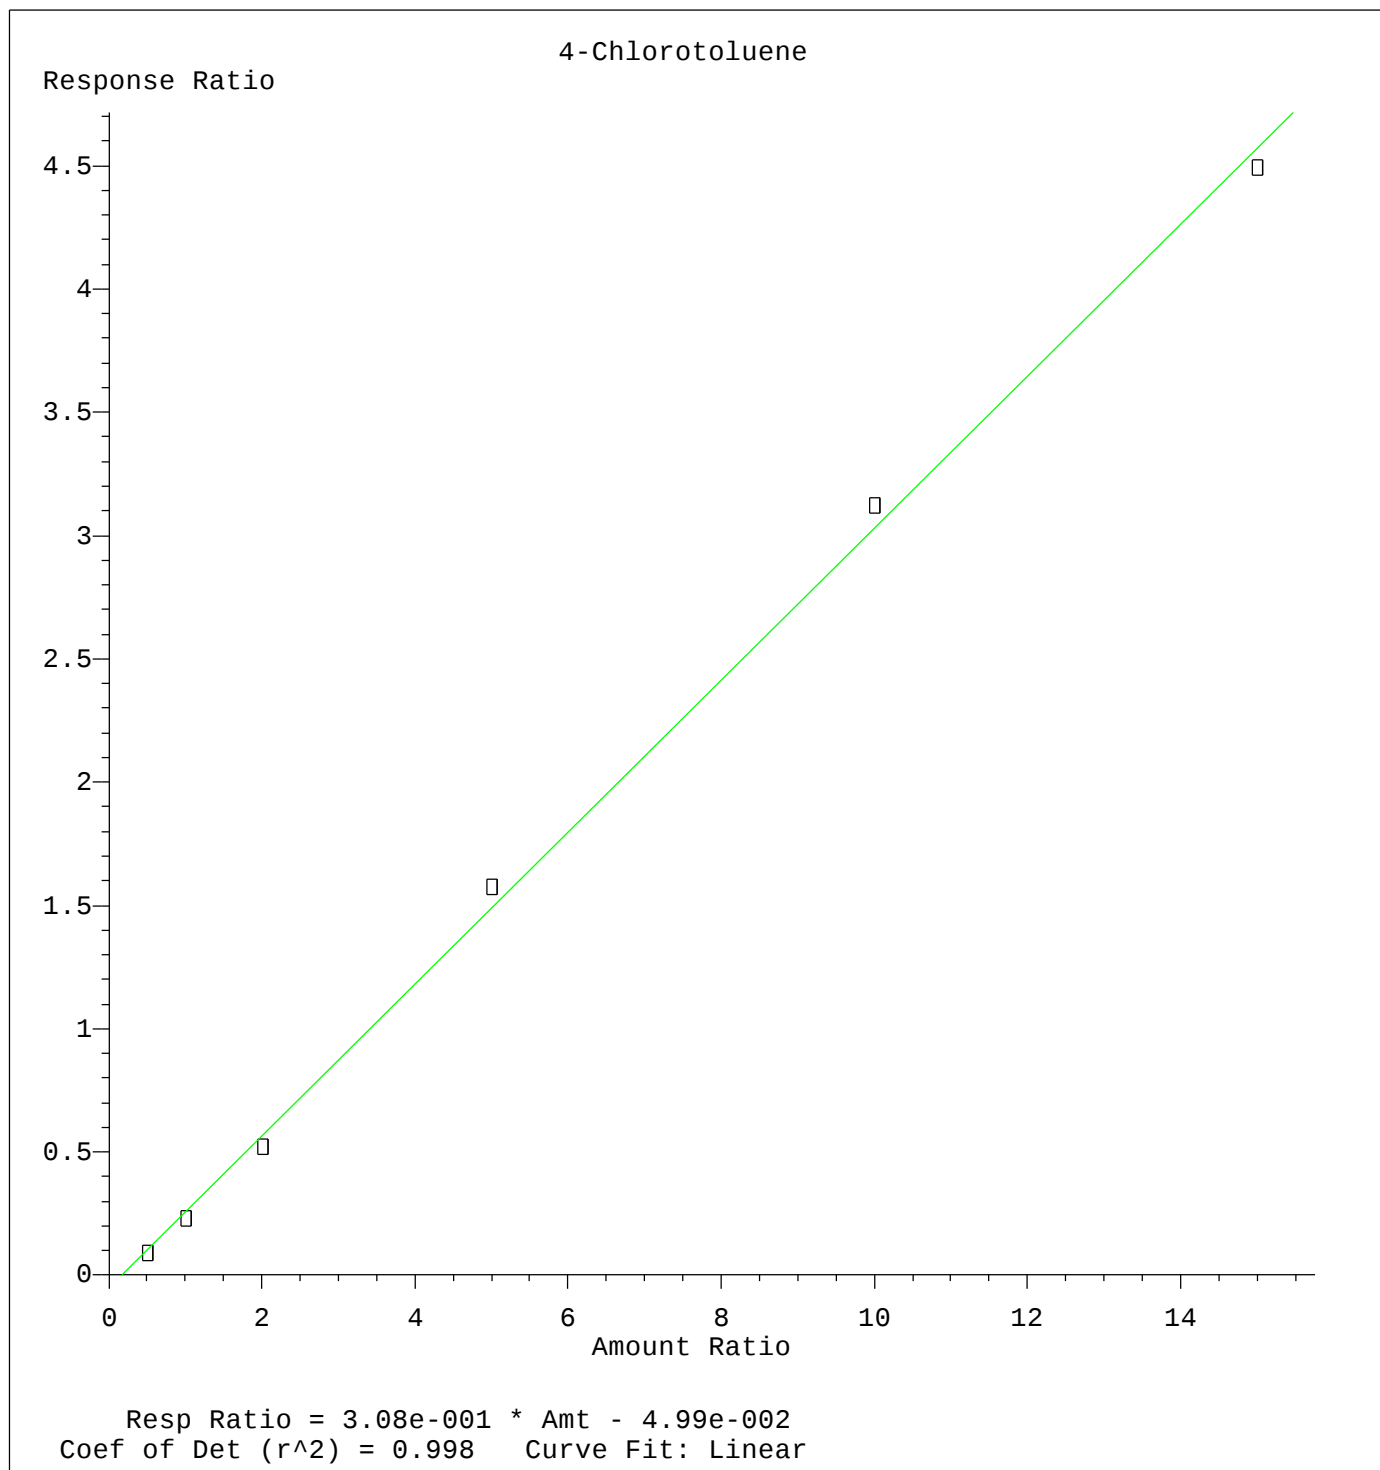

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019

1,2,4-Trimethylbenzene

Response Ratio

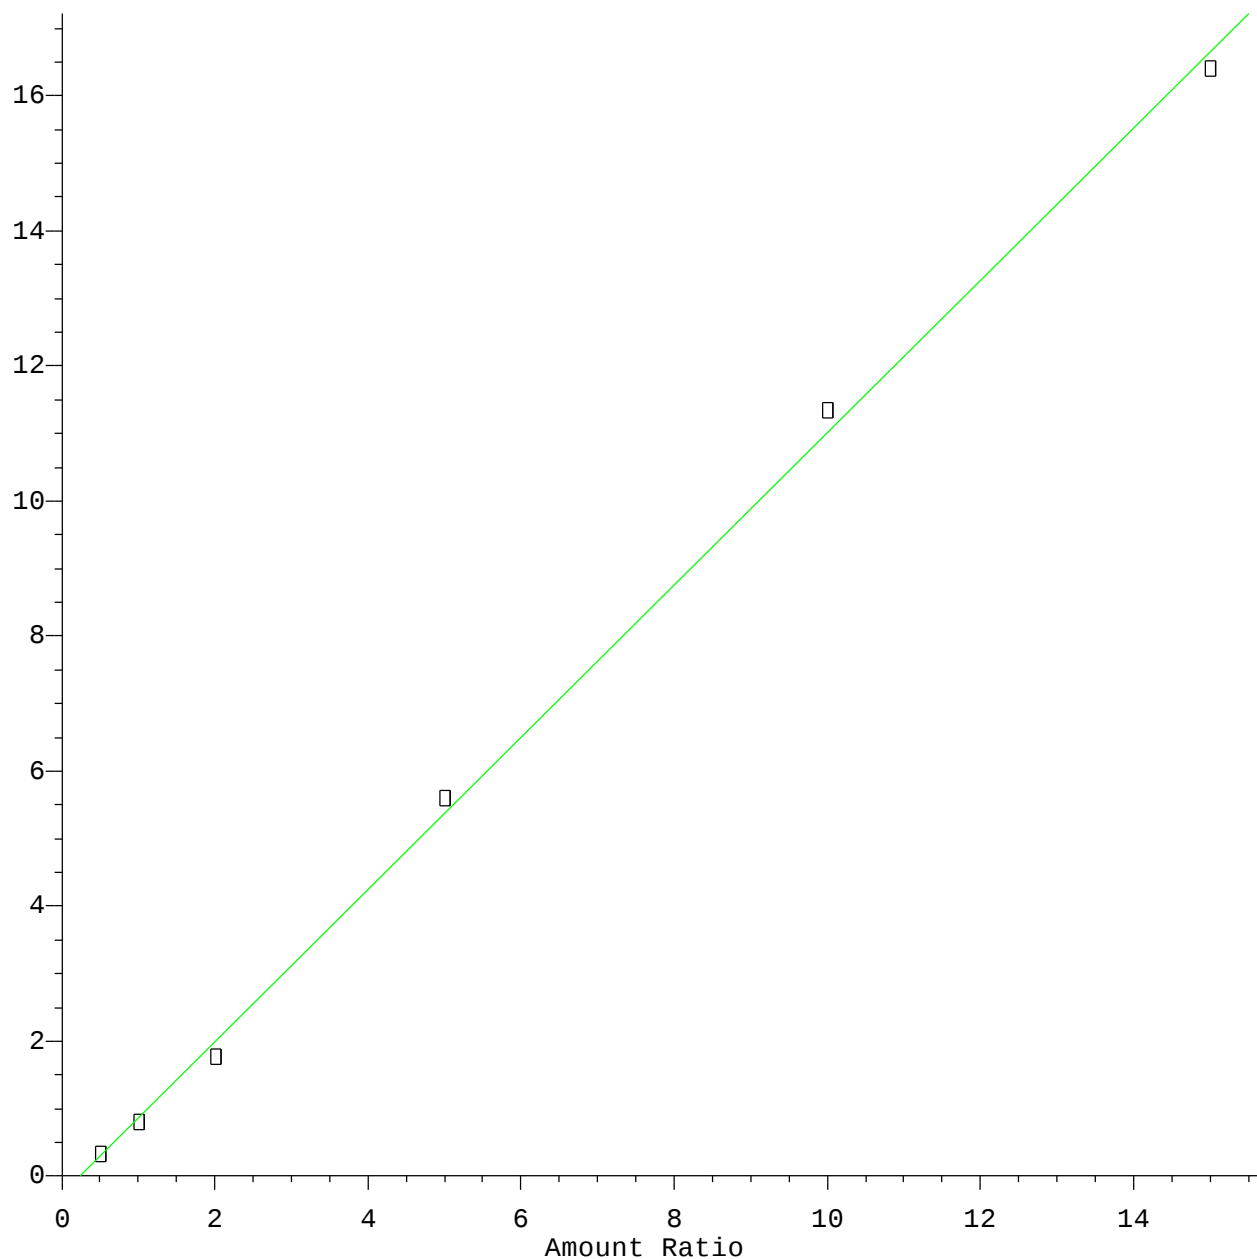


Resp Ratio = 1.13×10^0 * Amt - 2.58×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019

p-Isopropyltoluene

Response Ratio

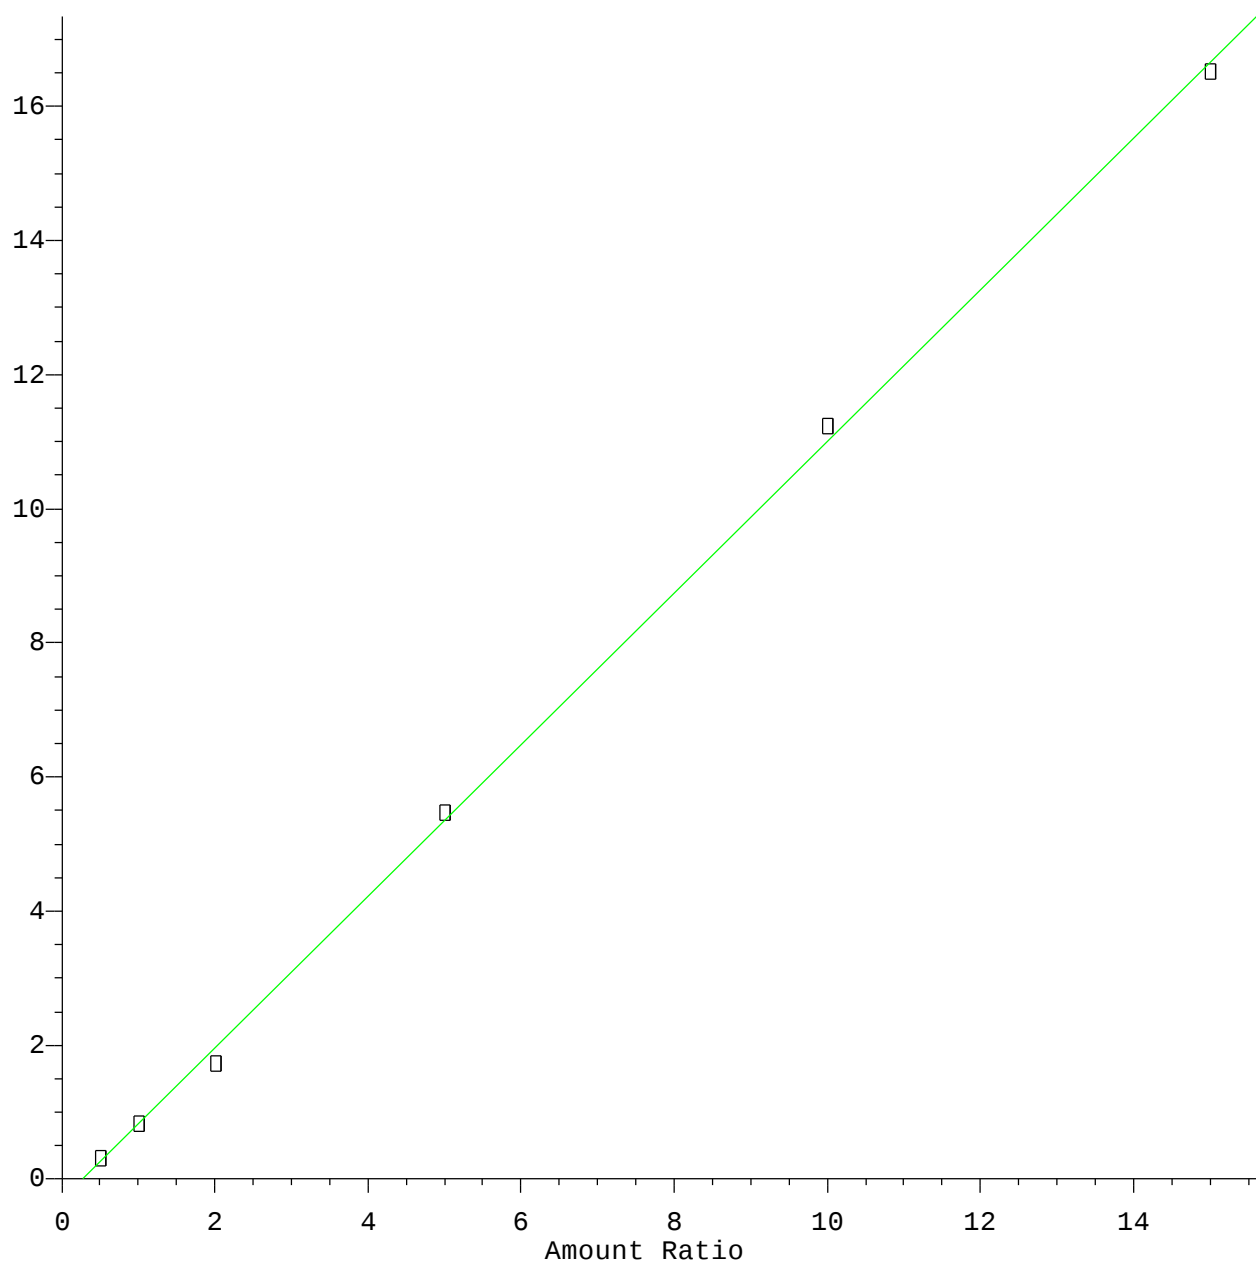


Resp Ratio = 1.13e+000 * Amt - 3.09e-001
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019

n-Butylbenzene

Response Ratio

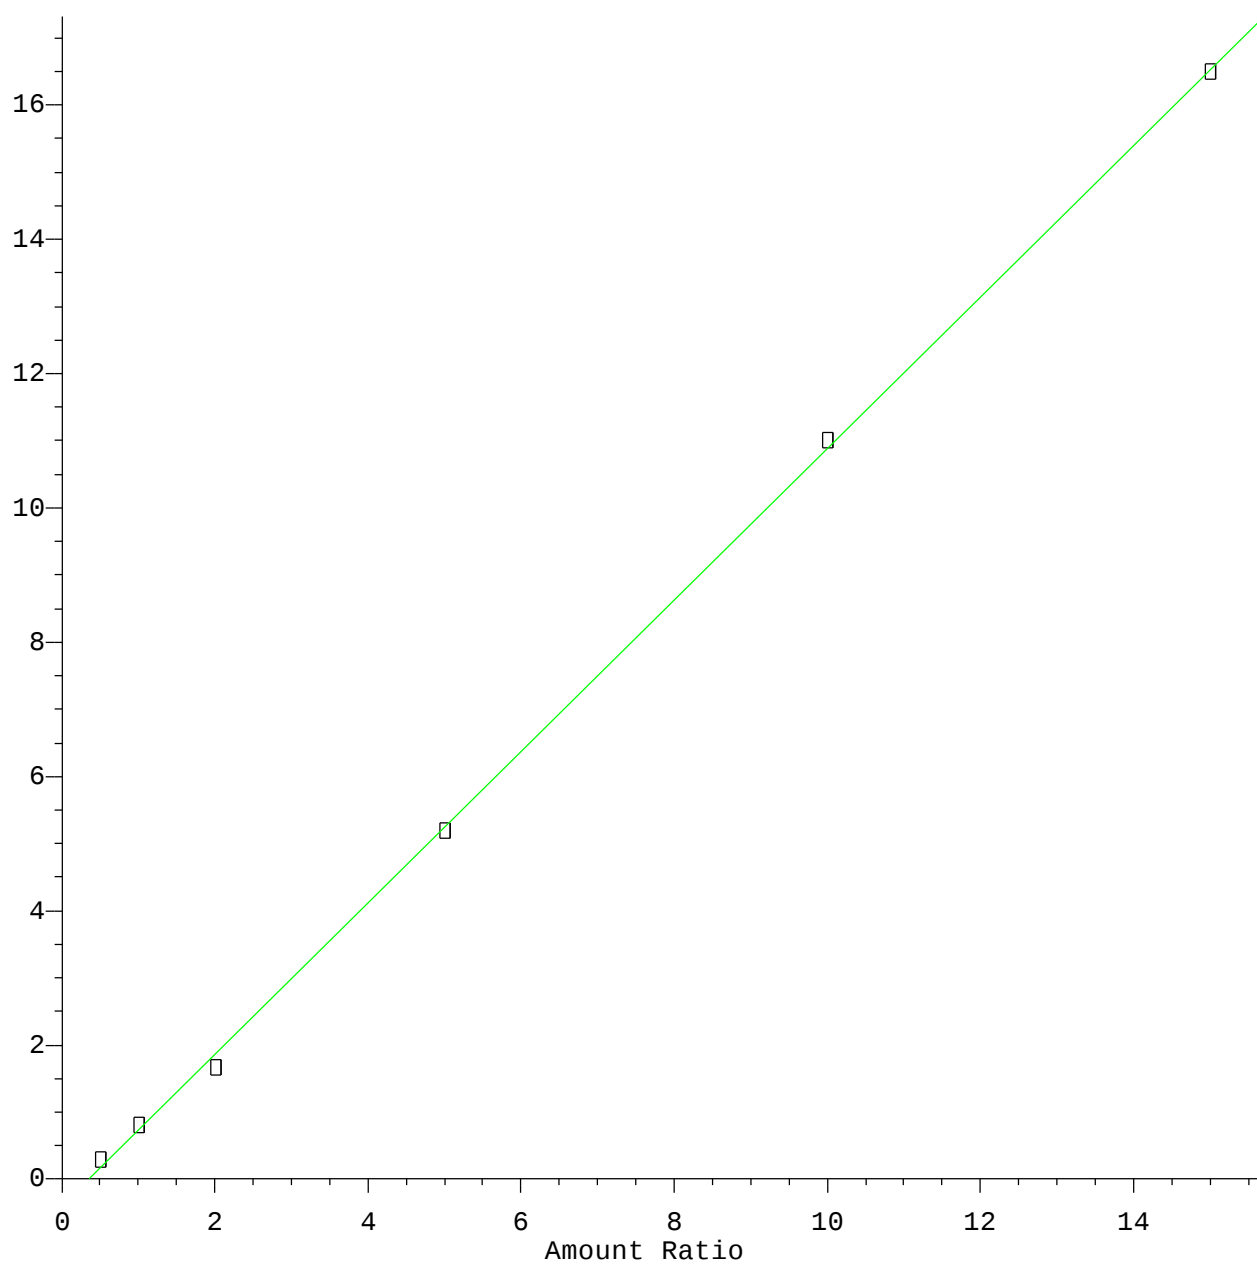


Resp Ratio = 1.13e+000 * Amt - 4.00e-001
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019


1,2,4-Trichlorobenzene

Response Ratio

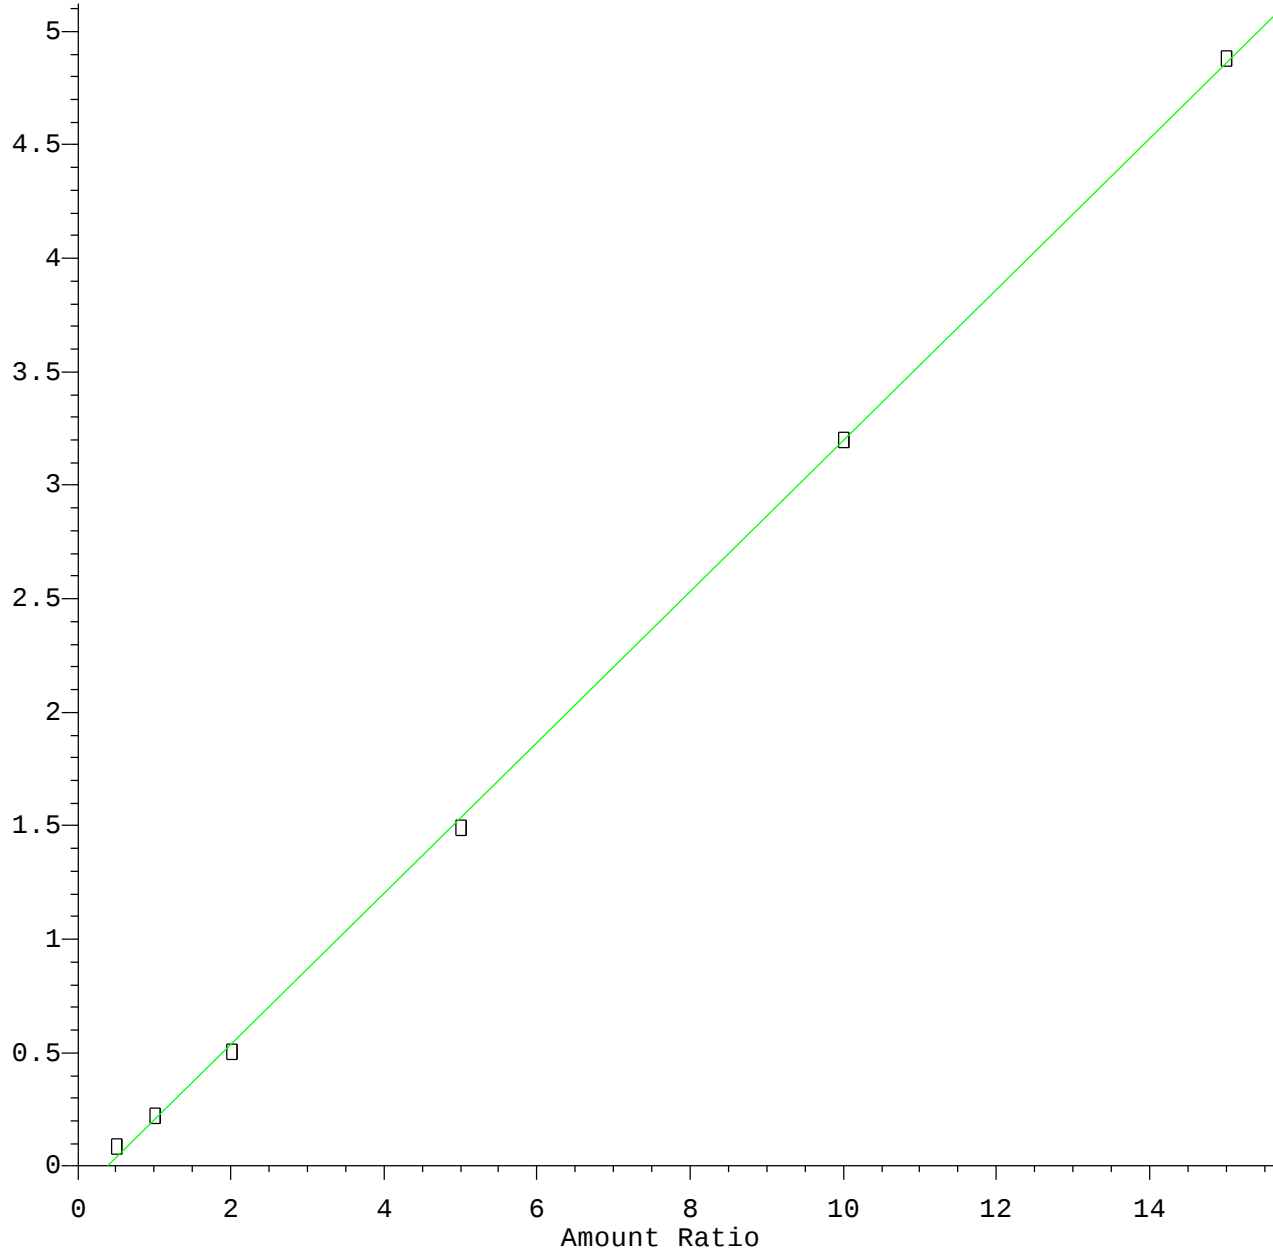

Resp Ratio = $3.32 \times 10^{-1} \times \text{Amt} - 1.28 \times 10^{-1}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019

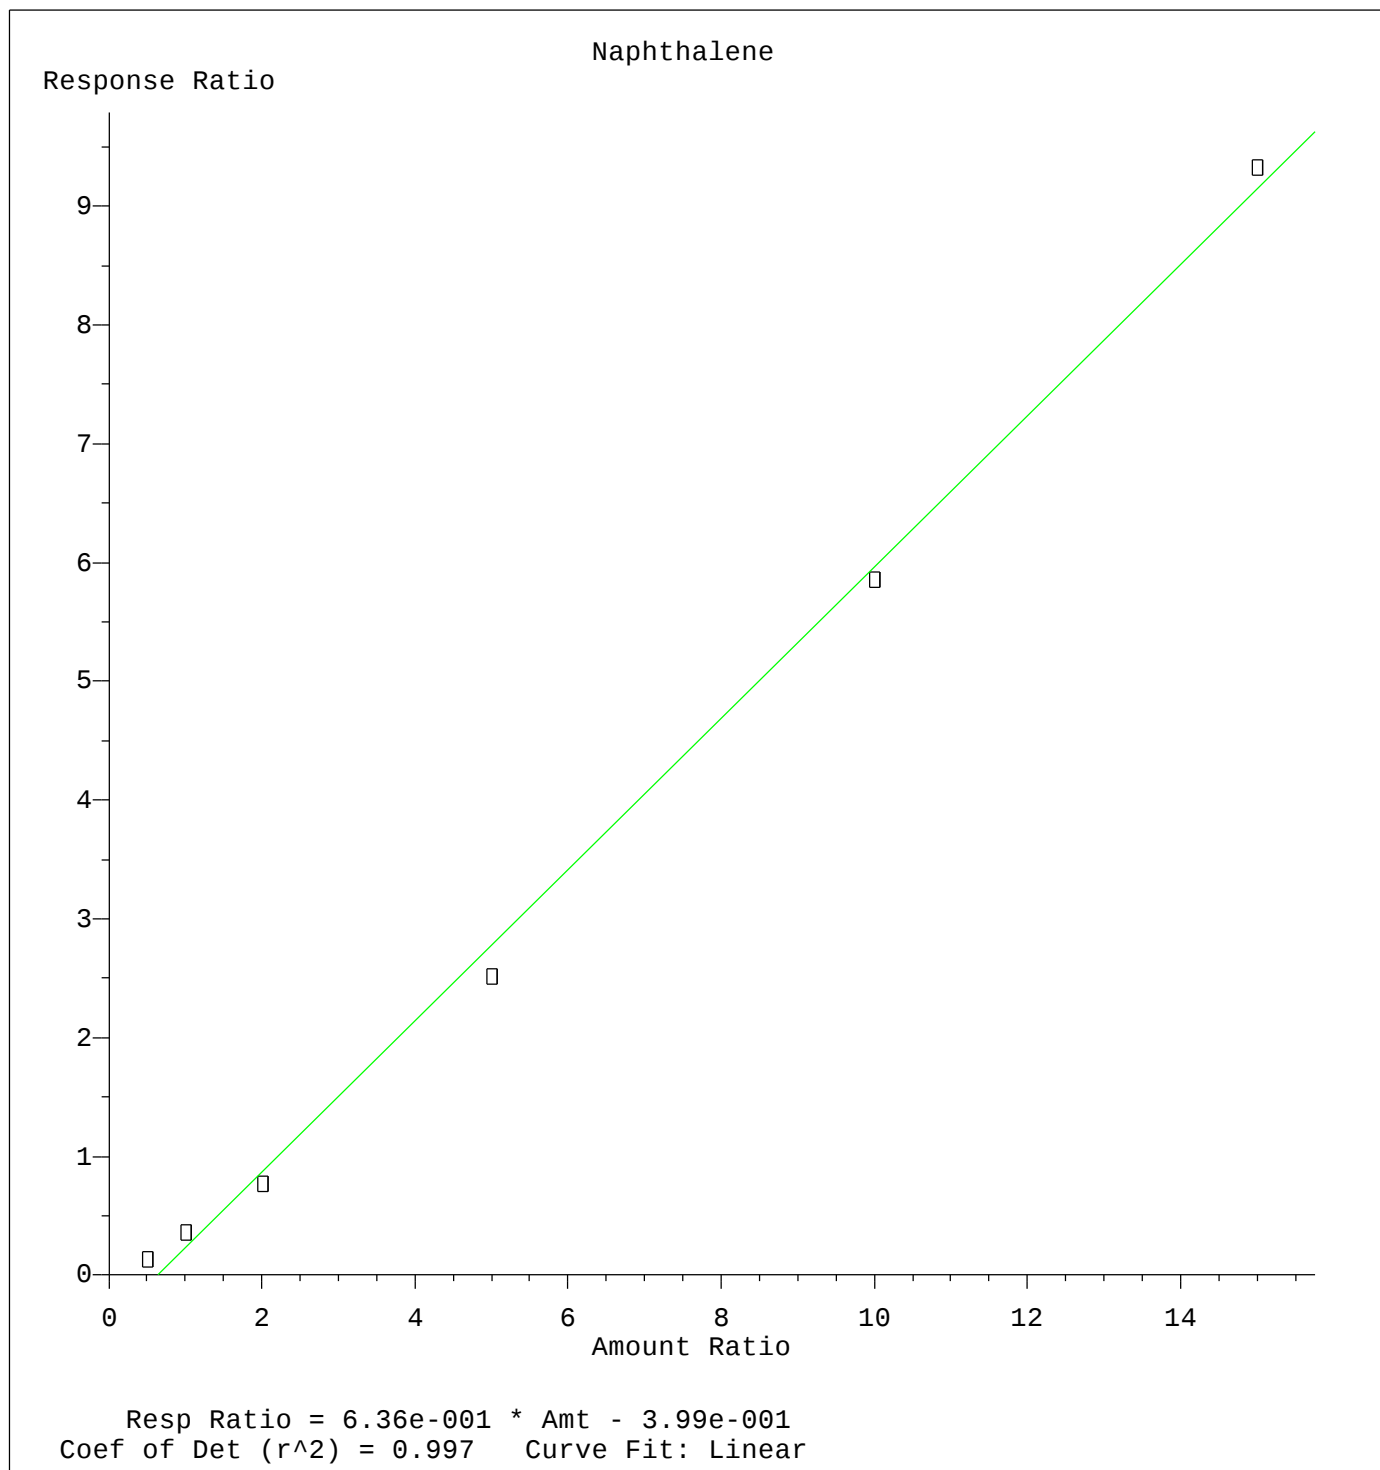

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U042619DW.M
Calibration Table Last Updated: Fri Apr 26 04:42:12 2019