


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
Data File : VU043324.D
Acq On : 26 Apr 2021 14:38
Operator : SY/MD
Sample : M2124-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4466

Quant Time: Apr 26 23:42:13 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Apr 26 23:40:31 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
4/27/2021 1:06:13 PM

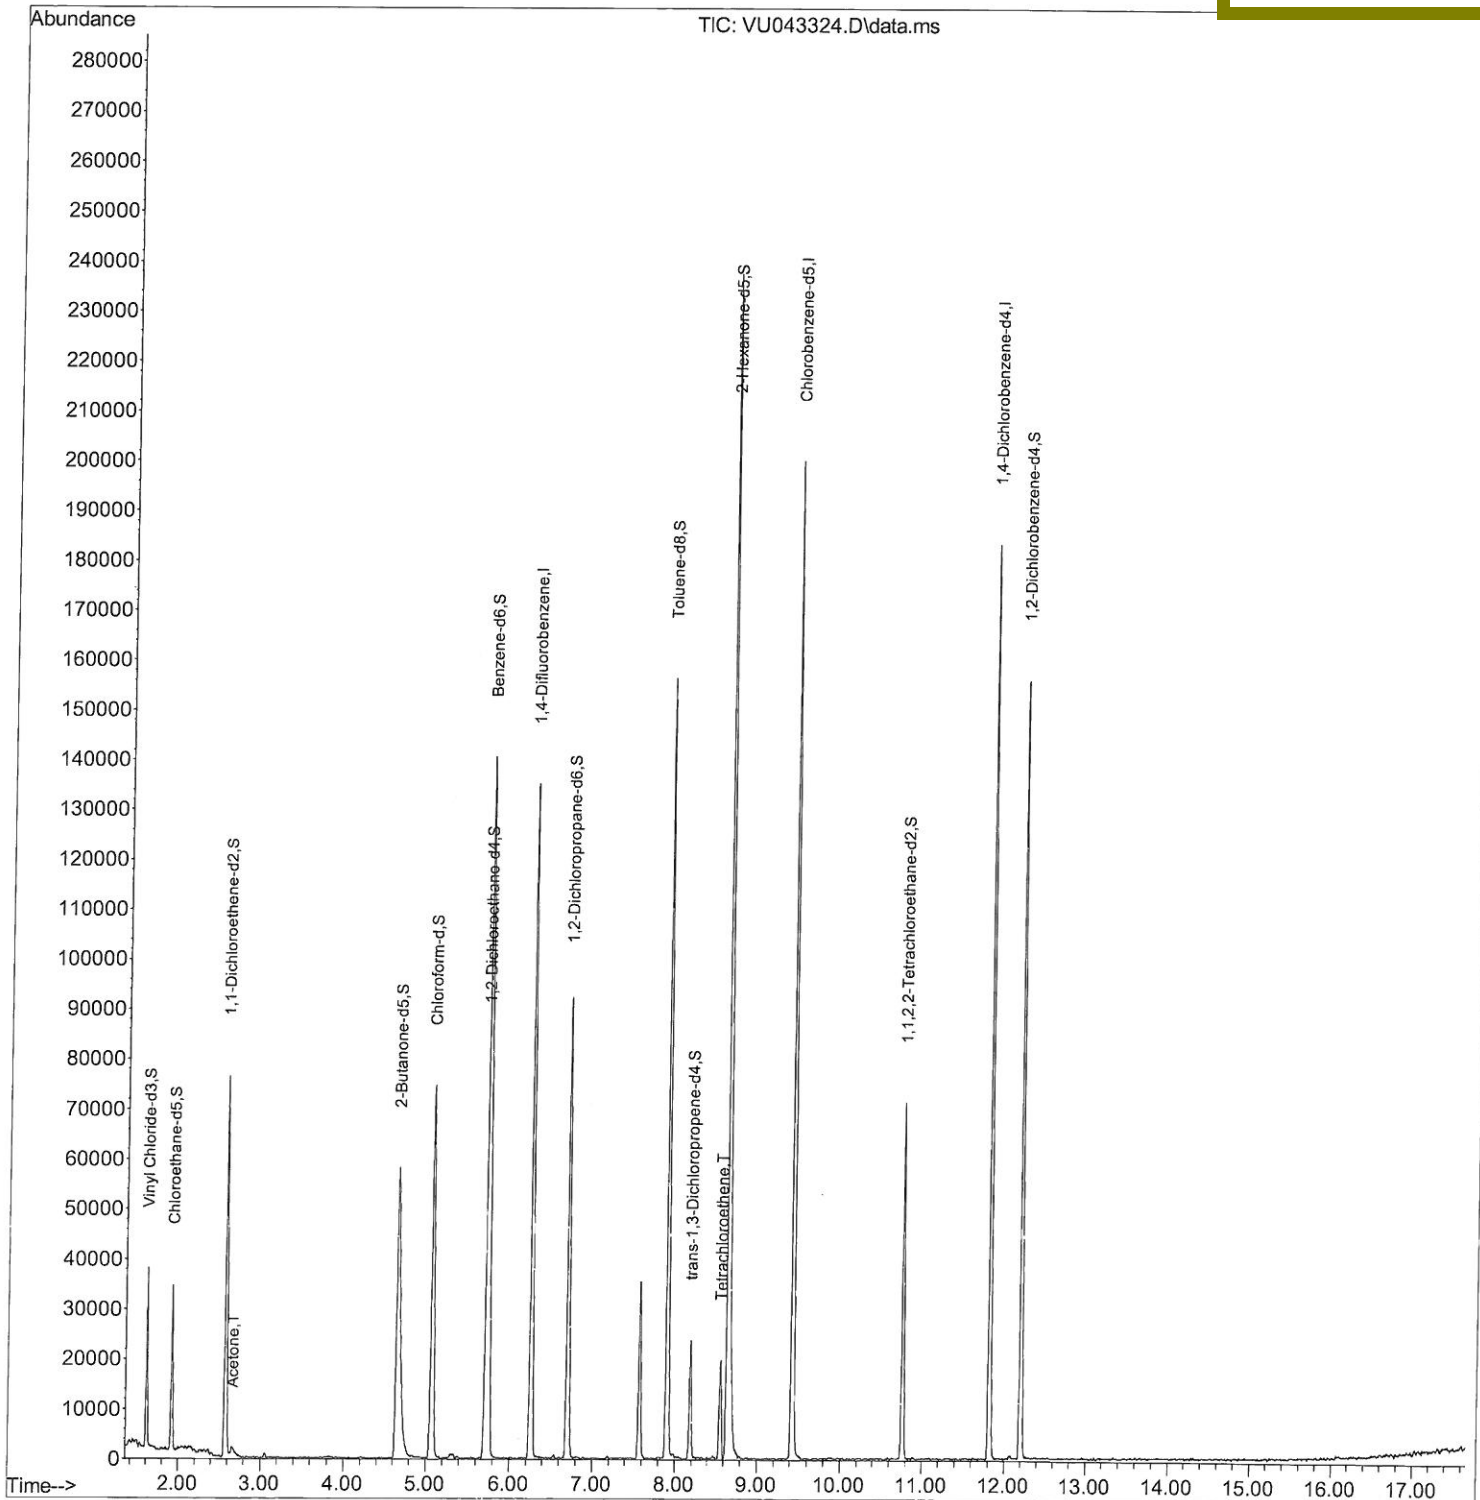

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
 Data File : VU043324.D
 Acq On : 26 Apr 2021 14:38
 Operator : SY/MD
 Sample : M2124-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4466

Quant Time: Apr 26 23:42:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 26 23:40:31 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 1:06:13 PM

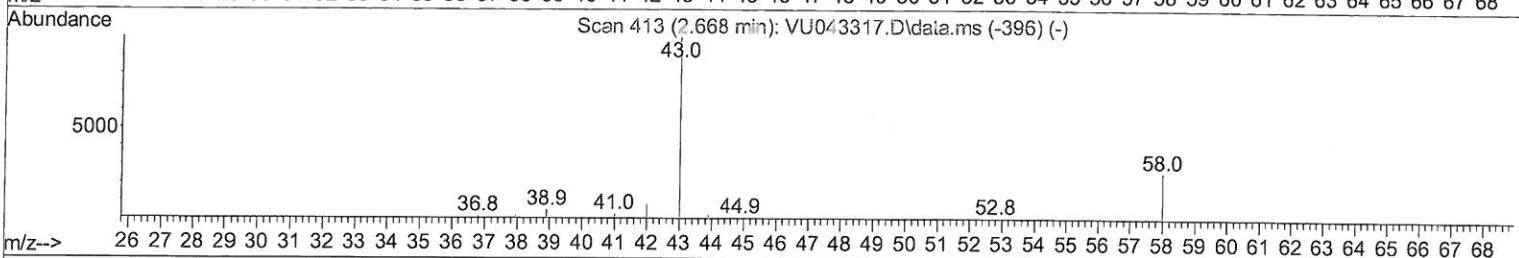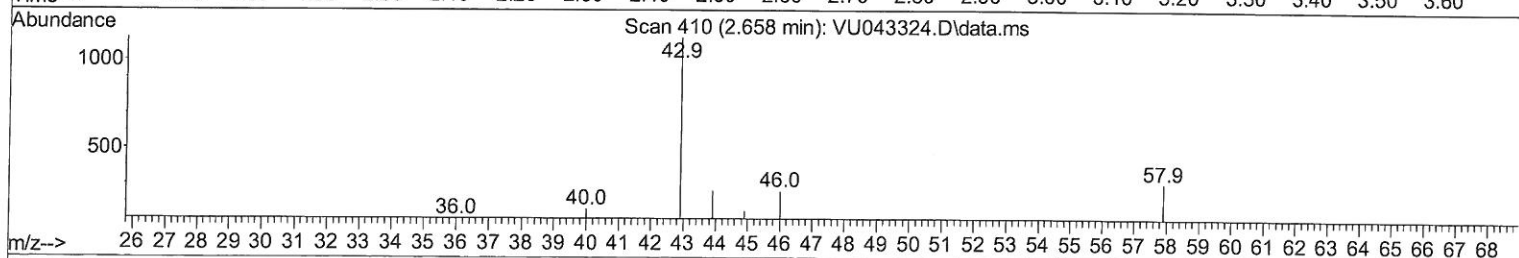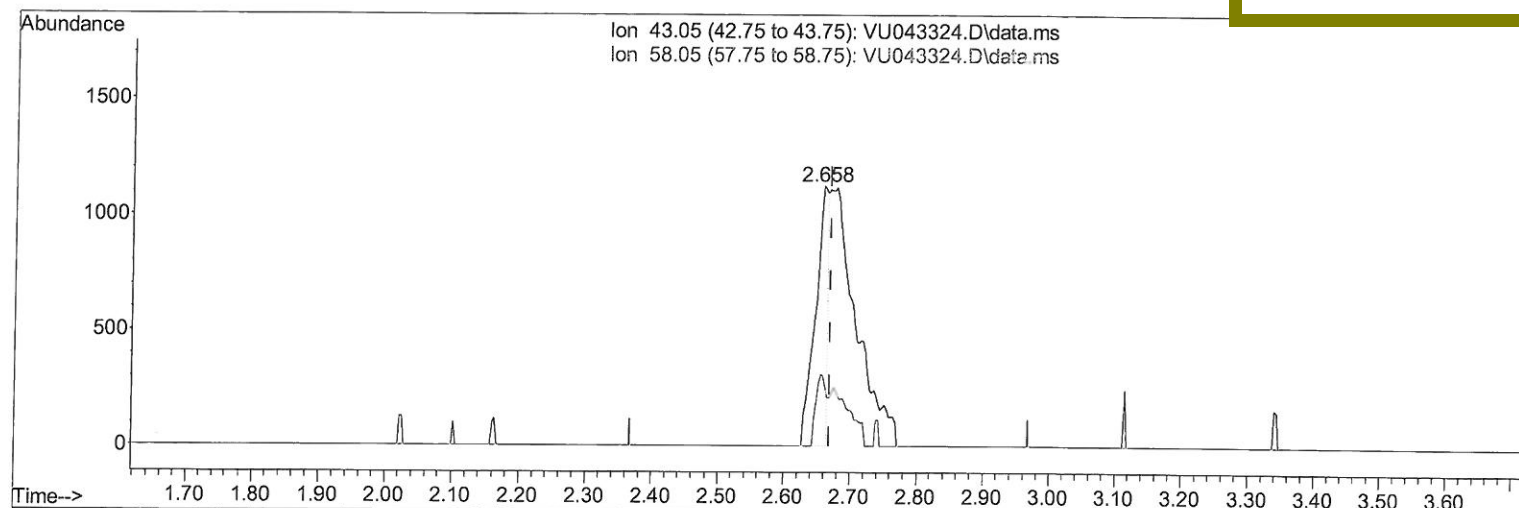

TIC: VU043324.D\data.ms

(13) Acetone (T)

2.658min (-0.010) 0.91 ug/L

response 1493

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.50	21.57
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
 Data File : VU043324.D
 Acq On : 26 Apr 2021 14:38
 Operator : SY/MD
 Sample : M2124-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4466

Quant Time: Apr 26 23:42:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 26 23:40:31 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 1:06:13 PM

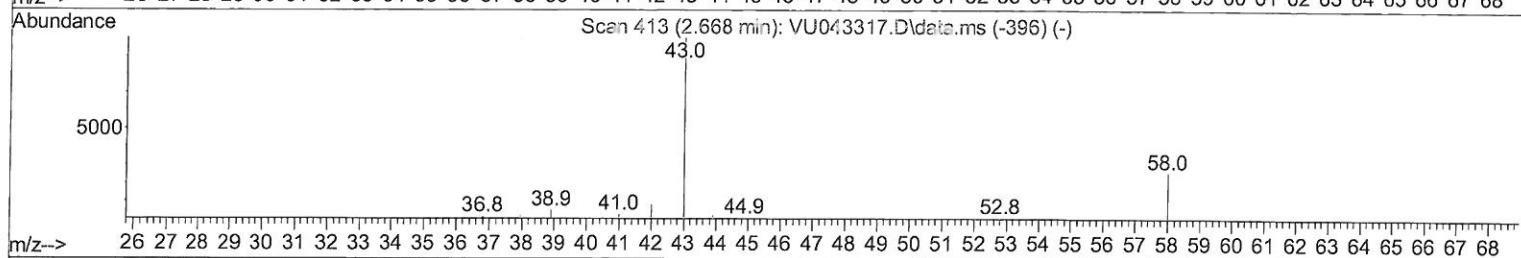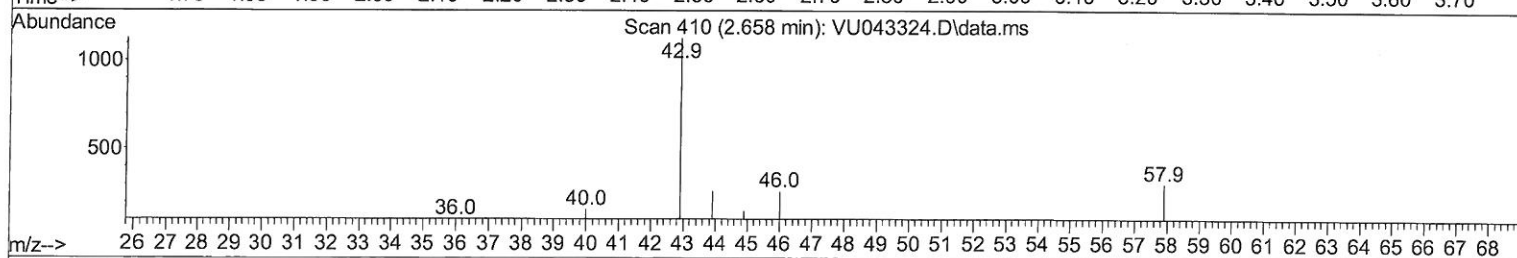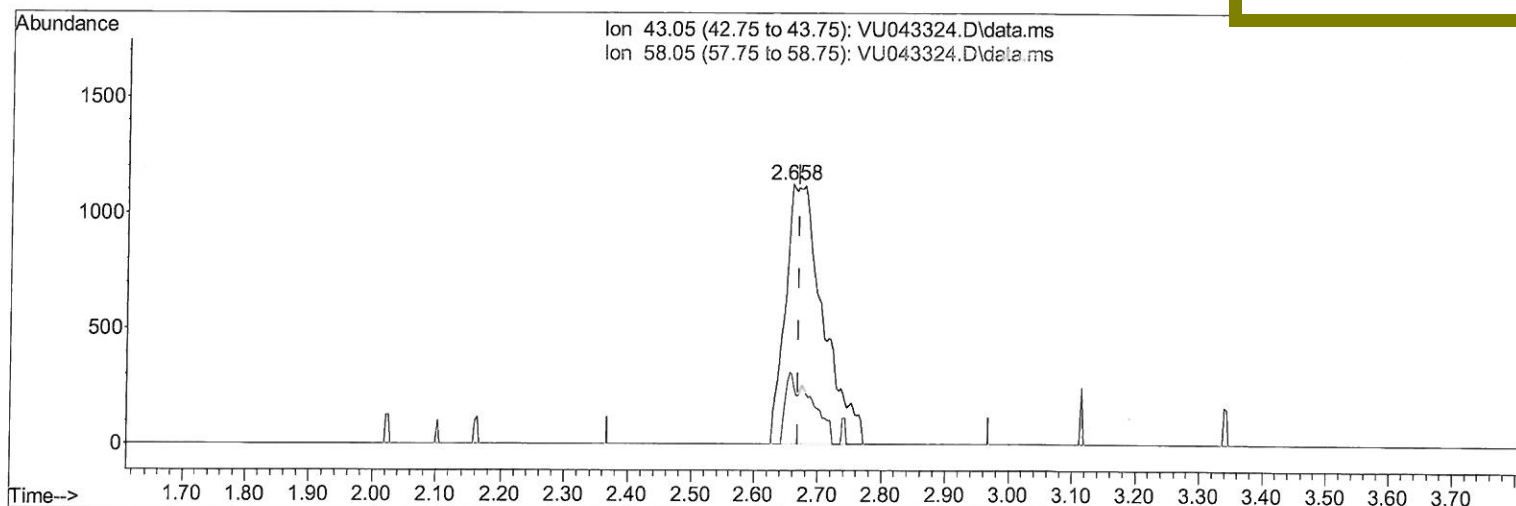

TIC: VU043324.D\data.ms

(13) Acetone (T)

2.658min (-0.010) 2.82 ug/L m

response 4599

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	12.50	7.00
0.00	0.00	0.00
0.00	0.00	0.00

MD
 4/28/21

Quantitation Report (QT Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
 Data File : VU043324.D
 Acq On : 26 Apr 2021 14:38
 Operator : SY/MD
 Sample : M2124-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sample ID :
 H4466

Quant Time: Apr 26 23:42:13 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 26 23:40:31 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/27/2021 1:06:13 PM

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	99644	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	99875	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	45958	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	24144	4.77	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	95.40%	
7) Chloroethane-d5	1.919	69	22335	4.68	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.60%	
11) 1,1-Dichloroethene-d2	2.575	65	14560	4.97	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	99.40%	
20) 2-Butanone-d5	4.652	46	124391	55.97	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	111.94%	
24) Chloroform-d	5.073	84	65662	5.10	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.00%	
26) 1,2-Dichloroethane-d4	5.713	65	42175	4.84	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.80%	
32) Benzene-d6	5.735	84	114782	4.94	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	98.80%	
36) 1,2-Dichloropropane-d6	6.697	67	38571	5.00	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	100.00%	
41) Toluene-d8	7.906	98	95906	3.97	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	79.40%	
43) trans-1,3-Dichloroprop...	8.185	79	12478	3.66	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	73.20%	
46) 2-Hexanone-d5	8.645	63	70689	41.62	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.24%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84	32821	4.84	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	96.80%	
66) 1,2-Dichlorobenzene-d4	12.201	152	38066	4.83	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	96.60%	
Target Compounds						
13) Acetone	2.658	43	4599m	2.82	ug/L	Qvalue
47) Tetrachloroethene	8.558	164	4174	0.72	ug/L	96

7 MD
 4/28/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed