

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
 Data File : VU043318.D
 Acq On : 26 Apr 2021 12:11
 Operator : SY/MD
 Sample : VU0426WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK138

Quant Time: Apr 26 23:41:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 26 23:40:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	108217	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	107134	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	48539	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	25940	4.71	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	94.20%
7) Chloroethane-d5	1.919	69	21974	4.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.80%
11) 1,1-Dichloroethene-d2	2.571	65	16748	5.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	105.20%
20) 2-Butanone-d5	4.655	46	111997	46.40	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.80%
24) Chloroform-d	5.073	84	68526	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.713	65	44911	4.75	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.00%
32) Benzene-d6	5.739	84	124129	4.98	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.60%
36) 1,2-Dichloropropane-d6	6.700	67	41020	4.96	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.20%
41) Toluene-d8	7.906	98	103614	4.00	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.00%
43) trans-1,3-Dichloroprop...	8.185	79	15904	4.35	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	87.00%
46) 2-Hexanone-d5	8.645	63	85670	47.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	94.04%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	35968	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.80%
66) 1,2-Dichlorobenzene-d4	12.201	152	41549	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%
Target Compounds						
16) Methylene chloride	3.057	84	2074	0.27	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
Data File : VU043318.D
Acq On : 26 Apr 2021 12:11
Operator : SY/MD
Sample : VU0426WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK138

Quant Time: Apr 26 23:41:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Apr 26 23:40:31 2021
Response via : Initial Calibration

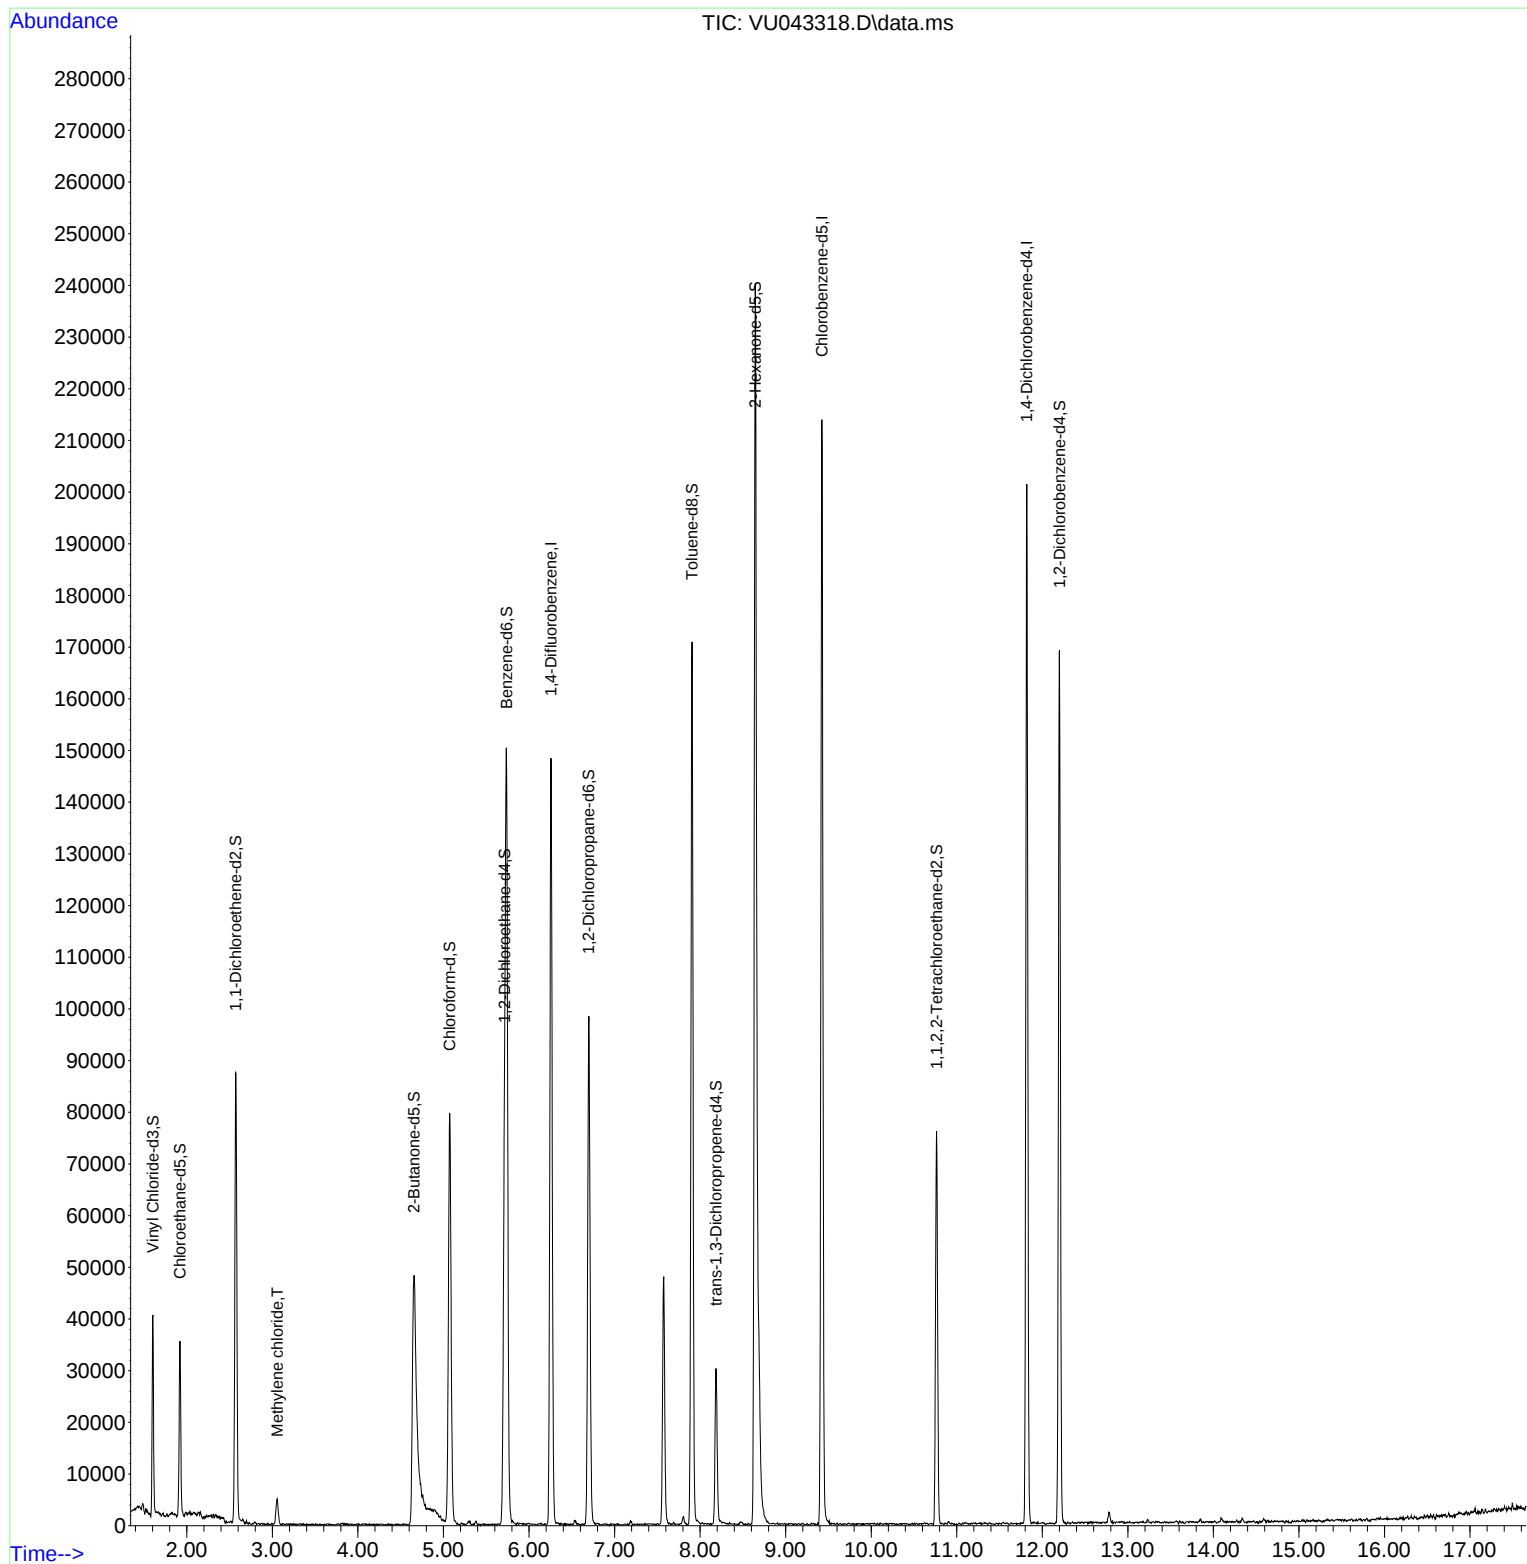

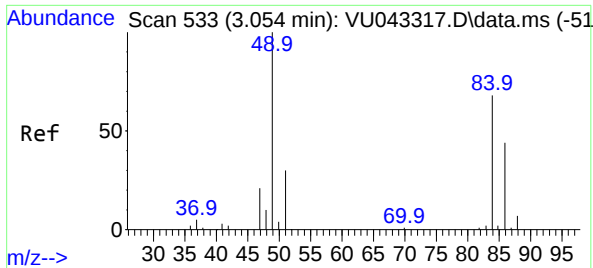

#16
Methylene chloride
Concen: 0.27 ug/L
RT: 3.057 min Scan# 534
Delta R.T. 0.003 min
Lab File: VU043318.D
Acq: 26 Apr 2021 12:11

Instrument :
MSVOA_U
ClientSampleId :
VBLK138

Tgt Ion: 84 Resp: 2074

Ion	Ratio	Lower	Upper
84	100		
86	68.7	44.9	83.5
49	149.4	79.0	146.8#

