

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
 Data File : VU043335.D
 Acq On : 26 Apr 2021 19:01
 Operator : SY/MD
 Sample : M2127-22
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AA3

Quant Time: Apr 26 23:44:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 26 23:40:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	107079	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	107825	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	49773	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	24620	4.52	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.40%
7) Chloroethane-d5	1.919	69	23539	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.575	65	16083	5.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	102.00%
20) 2-Butanone-d5	4.649	46	138190	57.86	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.72%
24) Chloroform-d	5.073	84	68421	4.94	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.80%
26) 1,2-Dichloroethane-d4	5.713	65	44005	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.00%
32) Benzene-d6	5.735	84	117320	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.700	67	41954	5.04	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.80%
41) Toluene-d8	7.906	98	101220	3.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.60%
43) trans-1,3-Dichloroprop...	8.185	79	14811	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.642	63	81548	44.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.94%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	35462	4.84	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.80%
66) 1,2-Dichlorobenzene-d4	12.198	152	40301	4.72	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.40%
Target Compounds						
13) Acetone	2.674	43	2737	1.56	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
Data File : VU043335.D
Acq On : 26 Apr 2021 19:01
Operator : SY/MD
Sample : M2127-22
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AA3

Quant Time: Apr 26 23:44:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Apr 26 23:40:31 2021
Response via : Initial Calibration

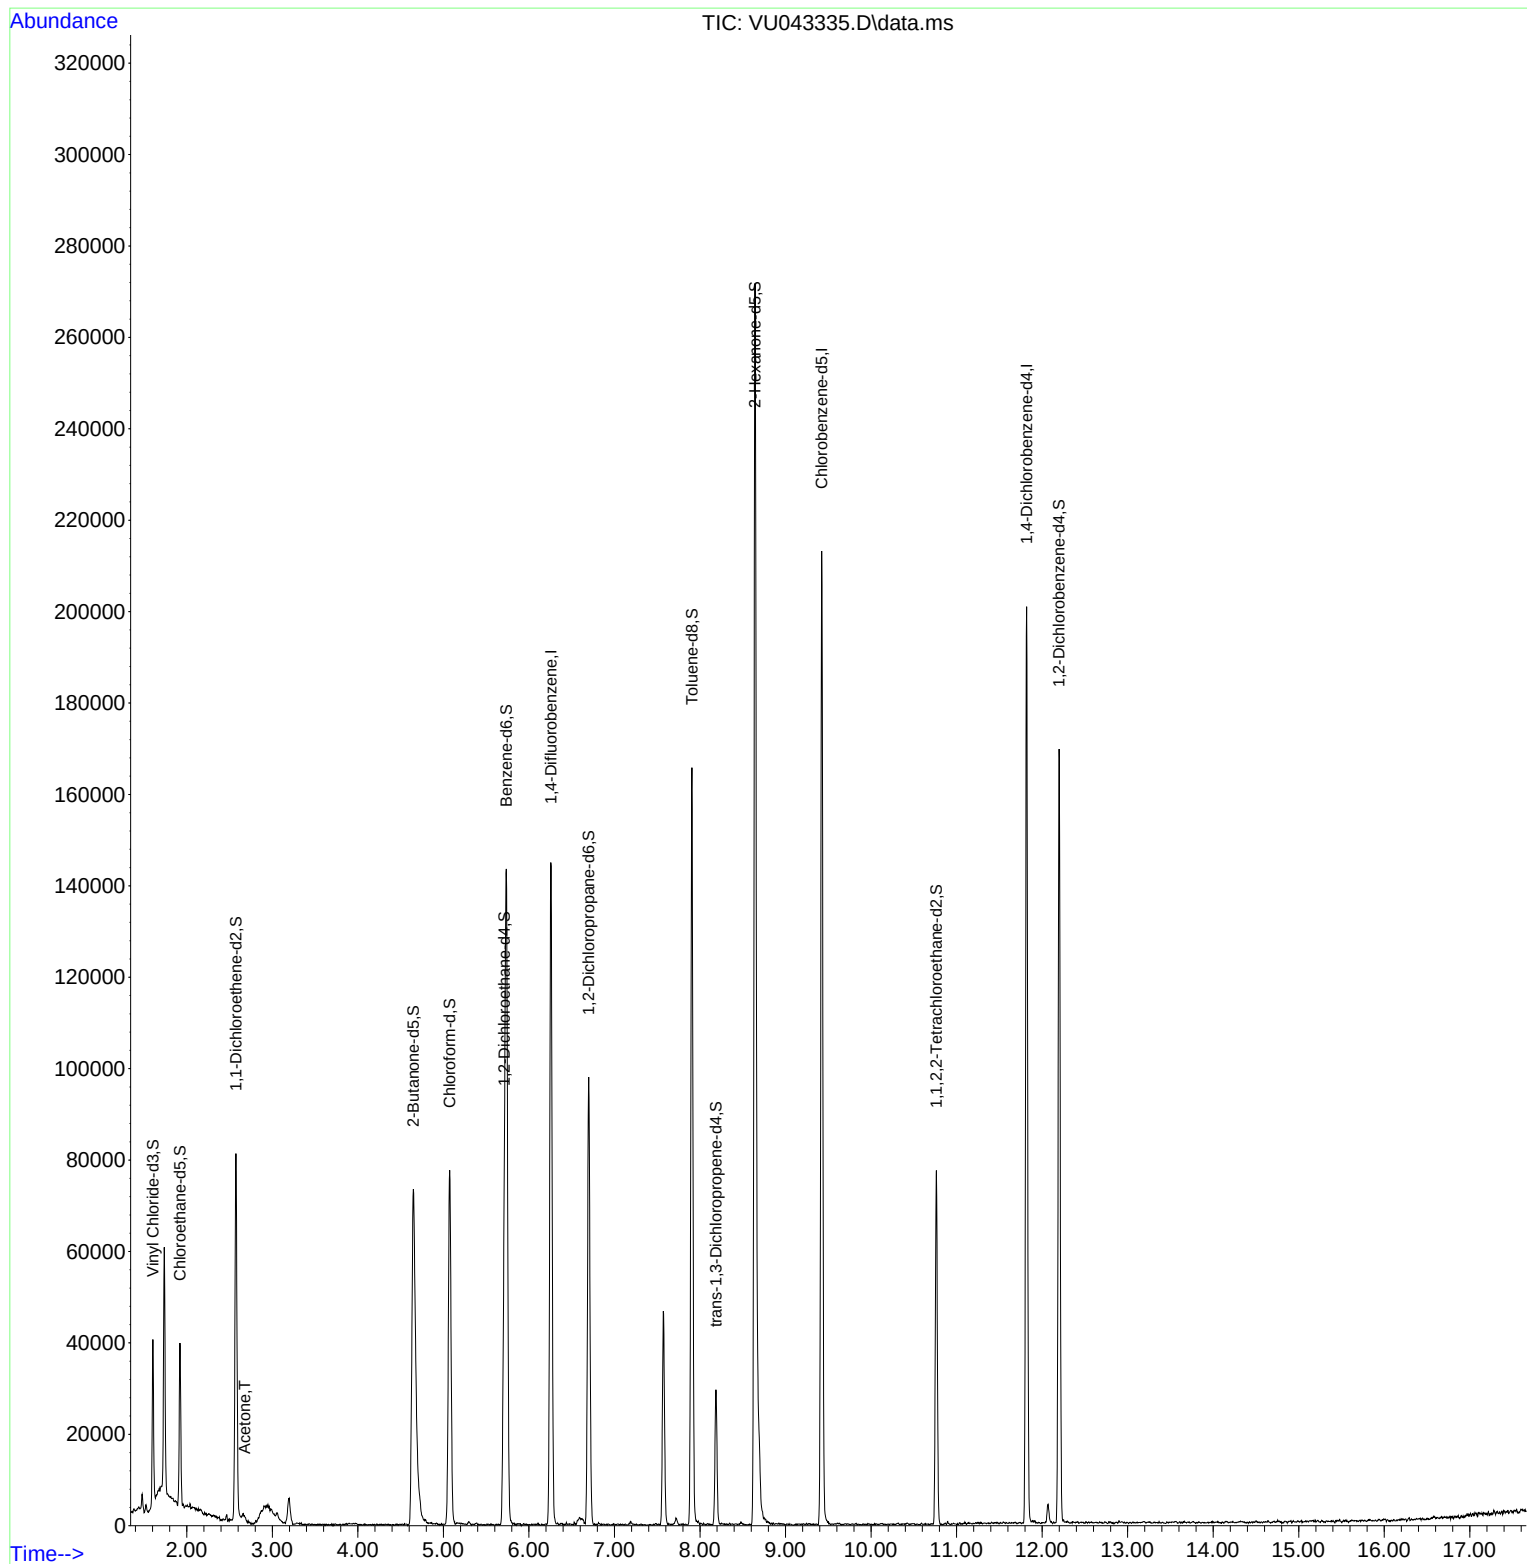

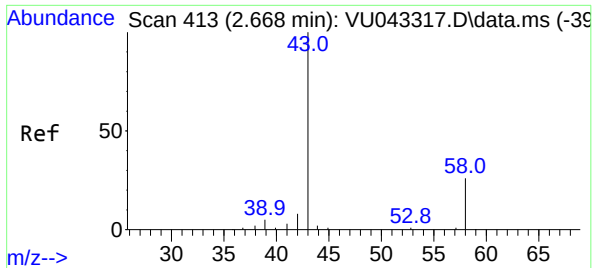

#13
 Acetone
 Concen: 1.56 ug/L
 RT: 2.674 min Scan# 415
 Delta R.T. 0.006 min
 Lab File: VU043335.D
 Acq: 26 Apr 2021 19:01

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AA3

Tgt Ion: 43 Resp: 2737
 Ion Ratio Lower Upper
 43 100
 58 17.2 0.0 25.0

