

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
 Data File : VU043336.D
 Acq On : 26 Apr 2021 19:25
 Operator : SY/MD
 Sample : M2127-23
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AA4

Quant Time: Apr 26 23:44:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 26 23:40:31 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.260	114	105942	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	106251	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	48048	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	24538	4.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.20%
7) Chloroethane-d5	1.919	69	22526	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.575	65	15328	4.92	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.40%
20) 2-Butanone-d5	4.652	46	136006	57.56	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.12%
24) Chloroform-d	5.073	84	66453	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	5.710	65	43127	4.66	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.20%
32) Benzene-d6	5.735	84	116151	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.700	67	40532	4.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.80%
41) Toluene-d8	7.906	98	96947	3.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.40%
43) trans-1,3-Dichloroprop...	8.185	79	14881	4.11	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.20%
46) 2-Hexanone-d5	8.642	63	80035	44.29	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.58%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	36242	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.40%
66) 1,2-Dichlorobenzene-d4	12.198	152	38925	4.73	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	94.60%
Target Compounds						
13) Acetone	2.668	43	3278	1.89	ug/L	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
Data File : VU043336.D
Acq On : 26 Apr 2021 19:25
Operator : SY/MD
Sample : M2127-23
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AA4

Quant Time: Apr 26 23:44:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Apr 26 23:40:31 2021
Response via : Initial Calibration

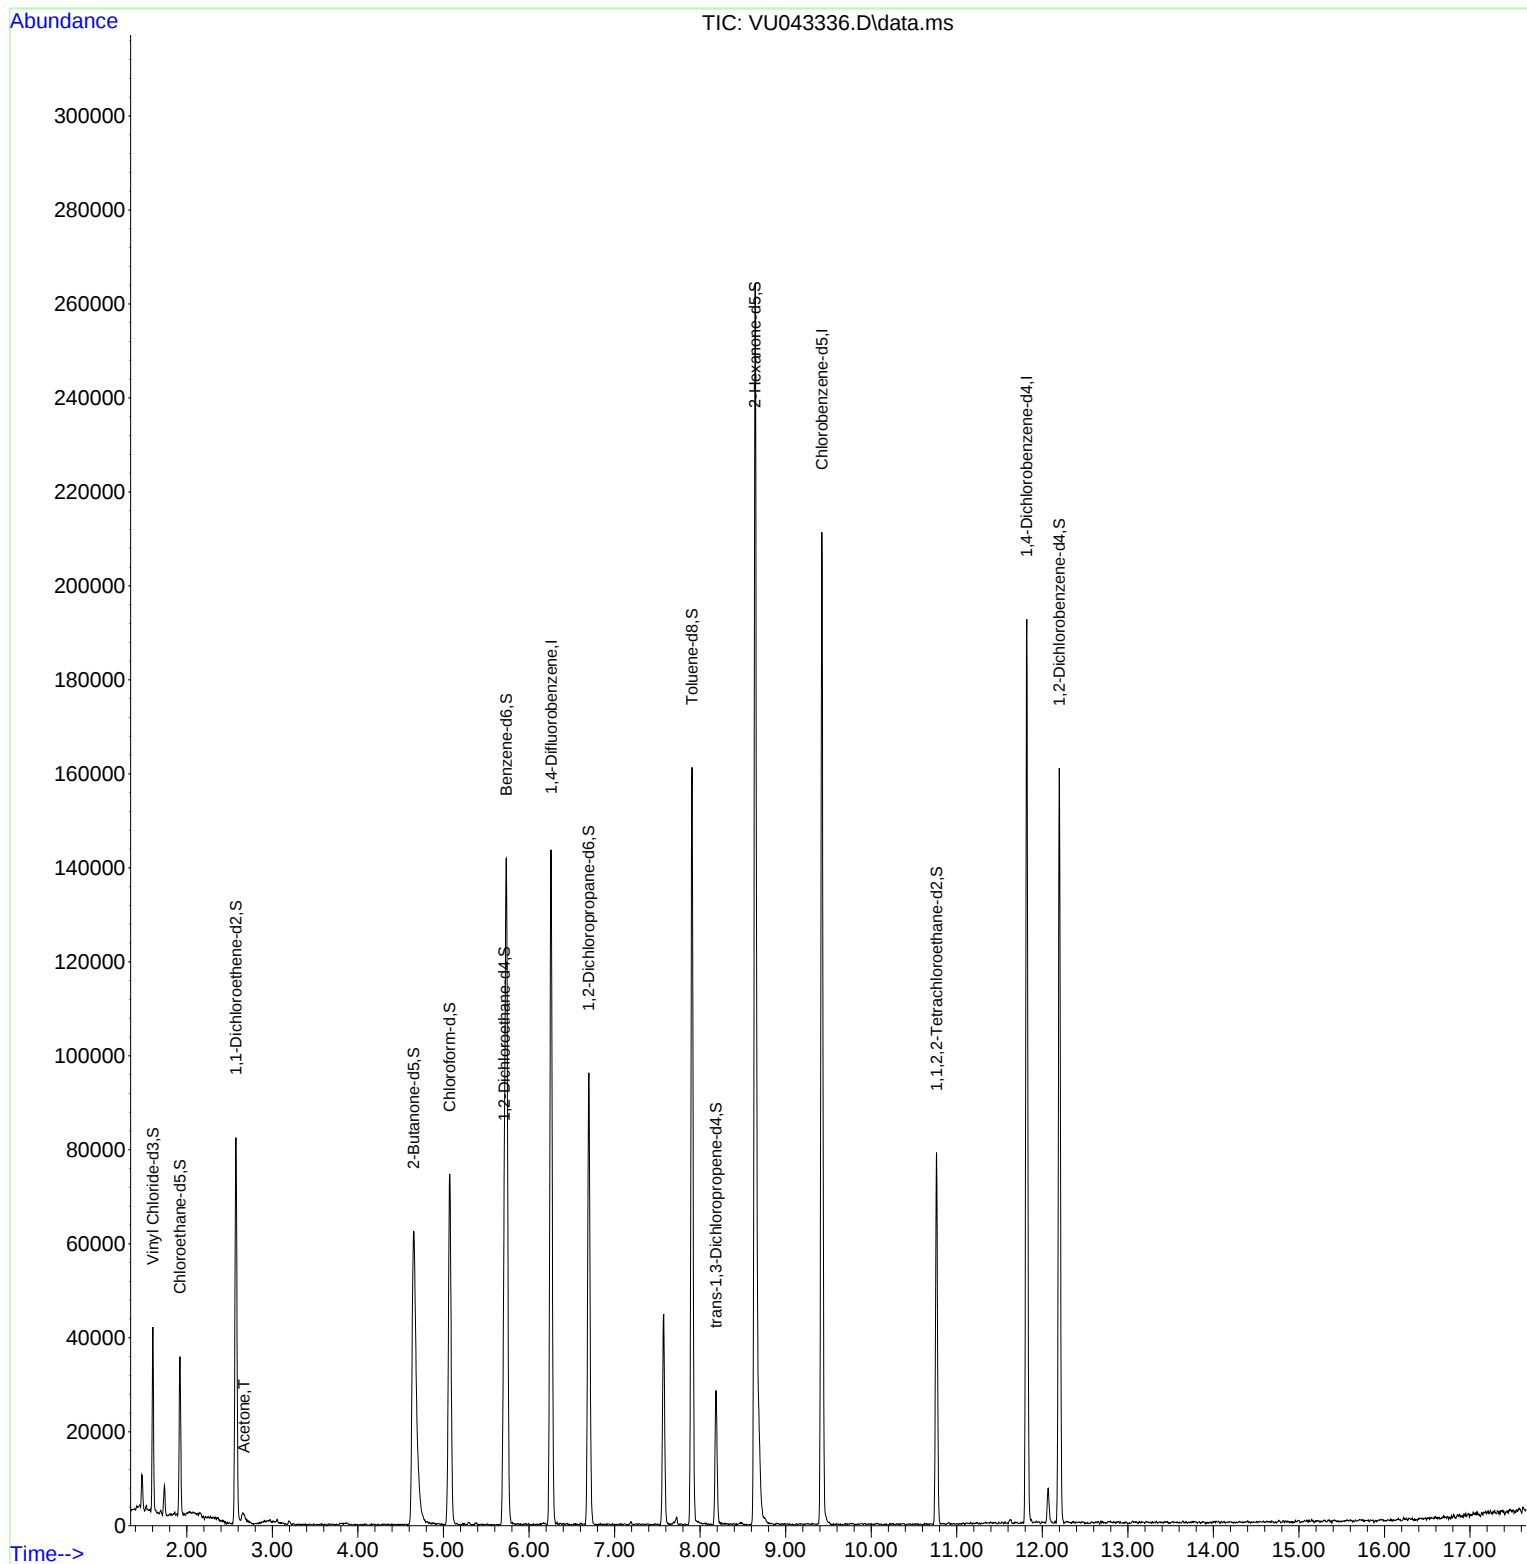

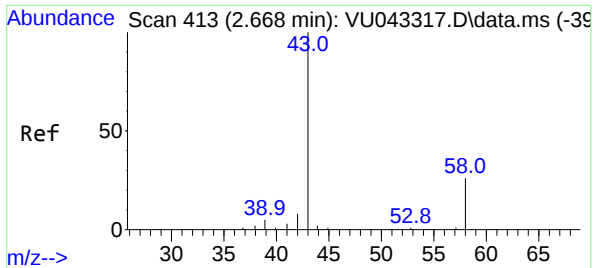

#13
Acetone
Concen: 1.89 ug/L
RT: 2.668 min Scan# 413
Delta R.T. -0.000 min
Lab File: VU043336.D
Acq: 26 Apr 2021 19:25

Instrument :
MSVOA_U
ClientSampleId :
E0AA4

Tgt Ion: 43 Resp: 3278
Ion Ratio Lower Upper
43 100
58 15.4 0.0 25.0

