


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042621\
Data File : VU043316.D
Acq On : 26 Apr 2021 09:45
Operator : SY/MD
Sample : BFB36
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB136

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Apr 26 23:40:31 2021

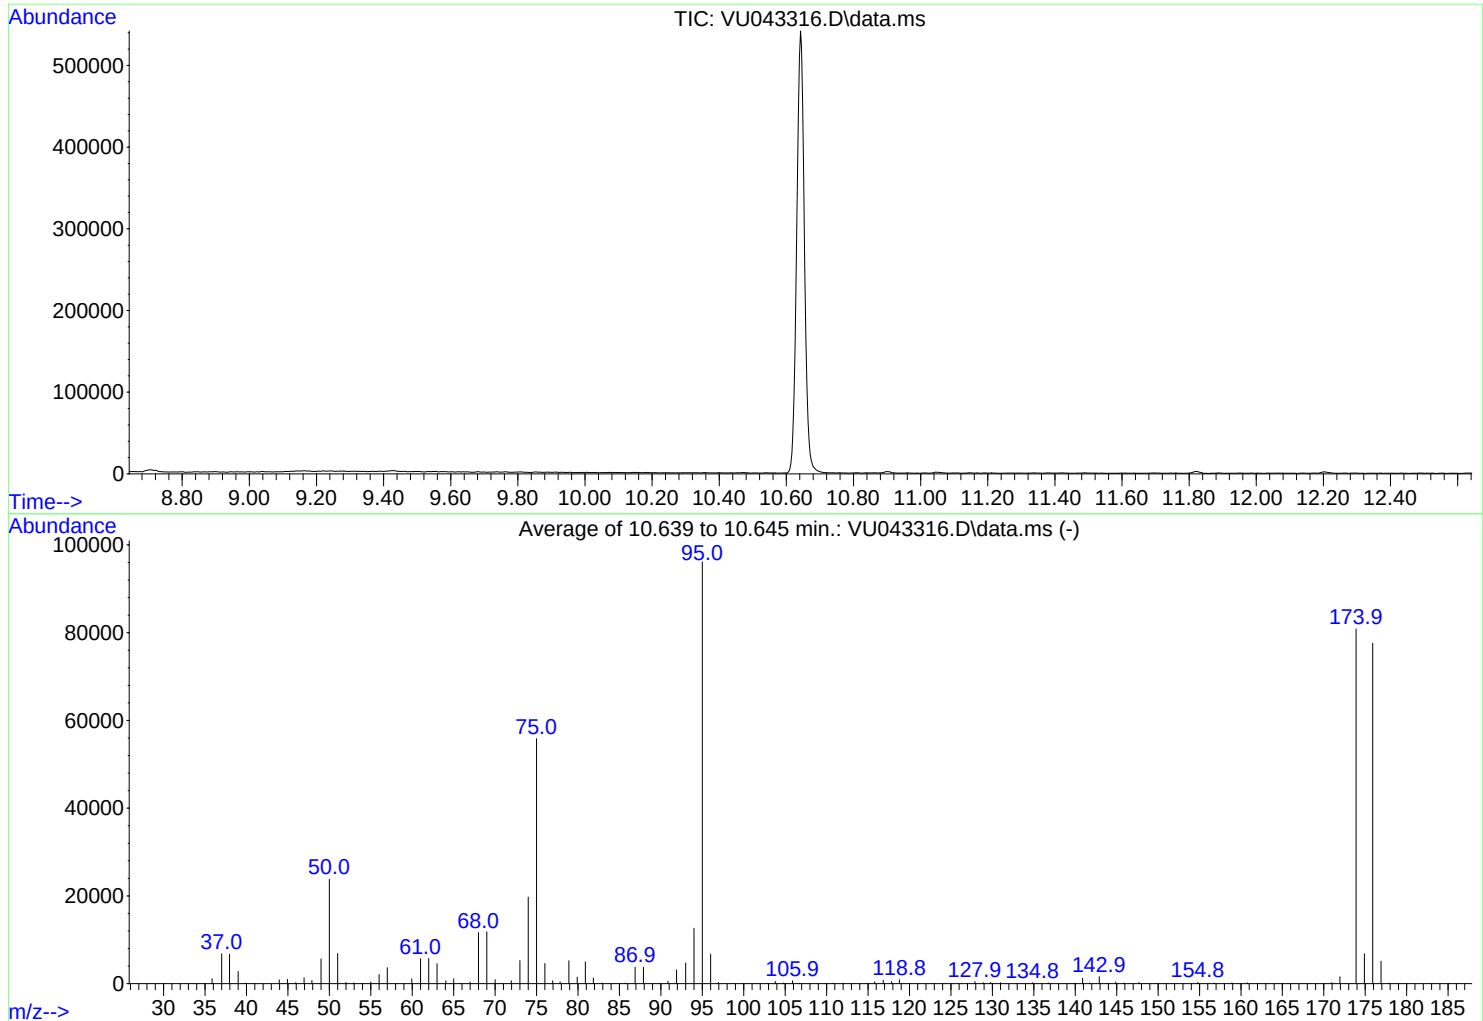

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.8	23827	PASS
75	95	30	80	58.1	55832	PASS
95	95	100	100	100.0	96157	PASS
96	95	5	9	7.0	6708	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.1	80859	PASS
175	174	5	9	8.4	6771	PASS
176	174	95	101	96.0	77632	PASS
177	176	5	9	6.6	5116	PASS

m/z	Abundance
35.90	1887.0
37.00	6781.0
38.00	6931.0
39.00	2844.0
39.90	261.0
43.90	953.0
45.00	1012.0
46.00	236.0
46.90	1318.0
47.90	772.0
49.00	5820.0
50.00	23464.0
51.00	6950.0
51.90	324.0
53.00	154.0
54.00	103.0
55.00	355.0
56.00	2030.0
57.00	3570.0
60.00	1131.0
61.00	5648.0
62.00	5666.0
63.00	4511.0
64.10	658.0
65.00	1098.0
66.90	346.0
68.00	11623.0
69.00	11592.0
70.00	933.0
71.90	640.0
73.00	5120.0
74.00	19064.0
75.00	54728.0
76.00	4386.0
76.90	673.0
77.90	340.0
78.90	5115.0
79.90	1525.0
80.90	5041.0
81.90	1255.0
82.90	158.0
85.70	156.0
86.90	3739.0
87.90	3774.0
90.90	568.0
91.90	3020.0
93.00	4789.0
94.00	12593.0
95.00	93088.0
96.00	6559.0
97.00	250.0
103.80	557.0
104.80	148.0
105.90	579.0
106.80	137.0
110.70	112.0
112.00	103.0
115.80	441.0
116.90	722.0
117.80	499.0
118.80	912.0
127.90	472.0
128.90	216.0
129.80	254.0
131.00	216.0
134.80	205.0
136.80	208.0
139.80	114.0
140.90	1190.0
141.80	194.0
142.90	1518.0
144.10	106.0
144.90	347.0
145.90	133.0
147.60	214.0
149.70	145.0
154.80	273.0
156.80	109.0
158.90	157.0
160.80	173.0
171.00	232.0
171.90	1578.0
173.90	76688.0
174.90	6764.0
175.90	73560.0
176.90	5120.0
177.90	127.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	681.0
37.80	218.0
39.80	168.0
44.00	159.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	1739.0
37.00	6655.0
38.00	6667.0
39.00	2580.0
39.90	304.0
44.00	1130.0
45.00	949.0
45.90	184.0
47.00	1333.0
47.90	694.0
49.00	5291.0
50.00	23480.0
51.00	6592.0
52.10	254.0
52.90	209.0
55.00	328.0
56.00	2106.0
57.00	3609.0
59.90	1025.0
61.00	5655.0
62.00	5749.0
63.00	4471.0
64.00	631.0
65.00	1089.0
65.80	105.0
67.10	382.0
68.00	11273.0
69.00	11560.0
70.00	900.0
71.90	679.0
73.00	5199.0
74.00	19640.0
75.00	55024.0
76.00	4606.0
77.00	618.0
77.80	447.0
78.90	5138.0
79.90	1379.0
80.90	4800.0
81.90	1271.0
82.90	133.0
85.70	132.0
86.90	3677.0
87.90	3513.0
90.90	539.0
91.90	3133.0
93.00	4525.0
94.00	12204.0
95.00	95808.0
96.00	6592.0
96.90	244.0
102.90	118.0
103.80	461.0
104.80	159.0
105.90	675.0
110.70	148.0
112.00	111.0
114.80	133.0
115.80	450.0
116.80	853.0
117.90	431.0
118.80	791.0
127.90	469.0
128.90	192.0
129.80	355.0
131.00	188.0
134.90	234.0
136.80	186.0
140.90	1299.0
141.70	187.0
142.90	1587.0
143.80	131.0
144.90	335.0
145.90	170.0
147.80	265.0
154.80	290.0
156.70	151.0
158.90	223.0
160.80	159.0
170.90	178.0
172.00	1519.0
173.90	82496.0
174.90	6573.0
175.90	79232.0
176.90	5006.0
177.80	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136

m/z	Abundance
35.90	1865.0
37.00	7003.0
38.00	7152.0
39.00	2873.0
39.90	305.0
44.00	1031.0
44.90	1016.0
45.90	251.0
46.90	1413.0
47.90	741.0
49.00	5733.0
50.00	24536.0
51.00	6990.0
52.00	317.0
52.90	184.0
55.00	365.0
56.00	2137.0
57.00	3767.0
59.90	1148.0
61.00	5810.0
62.00	5869.0
63.00	4735.0
64.00	689.0
65.00	1158.0
67.00	357.0
68.00	12026.0
69.00	12319.0
70.00	943.0
72.00	658.0
73.00	5399.0
74.00	20528.0
75.00	57744.0
76.00	4781.0
77.00	670.0
77.90	430.0
78.90	5417.0
79.90	1542.0
80.90	5078.0
81.80	1356.0
82.90	161.0
85.70	153.0
86.90	3808.0
87.90	3884.0
90.80	589.0
91.90	3241.0
93.00	4817.0
94.00	13023.0
95.00	99576.0
96.00	6973.0
96.90	274.0
102.90	111.0
103.80	537.0
104.80	155.0
105.90	671.0
106.70	120.0
109.90	100.0
110.70	127.0
112.00	130.0
114.80	122.0
115.80	451.0
116.80	770.0
117.90	476.0
118.80	925.0
127.90	530.0
128.90	210.0
129.80	300.0
131.00	236.0
134.90	229.0
136.70	212.0
140.00	110.0
140.90	1289.0
141.80	213.0
142.90	1673.0
143.80	117.0
144.90	388.0
145.90	168.0
147.70	259.0
149.80	117.0
154.80	316.0
156.80	139.0
158.90	210.0
160.80	191.0
171.00	224.0
171.90	1651.0
173.90	83392.0
174.90	6975.0
175.90	80104.0
176.90	5223.0
177.90	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB136