

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048294.D
 Acq On : 26 Apr 2022 12:20
 Operator : SY/MD
 Sample : VU0426MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.481	40	44	50	rBV2	3396	4216	0.25%	0.033%
2	1.600	73	81	101	rBV	208238	268102	15.89%	2.082%
3	1.887	162	170	189	rVB	140311	218285	12.94%	1.695%
4	2.562	367	380	400	rBV	353731	580493	34.40%	4.508%
5	2.710	422	426	429	rBV2	342	324	0.02%	0.003%
6	2.768	441	444	445	rBV2	404	230	0.01%	0.002%
7	2.787	446	450	455	rVB4	927	990	0.06%	0.008%
8	2.896	480	484	488	rVB4	357	297	0.02%	0.002%
9	2.948	496	500	504	rBV4	398	373	0.02%	0.003%
10	3.047	523	531	537	rVV4	1796	2873	0.17%	0.022%
11	3.099	543	547	549	rVB	307	208	0.01%	0.002%
12	3.121	549	554	558	rBV2	589	545	0.03%	0.004%
13	3.182	562	573	575	rBV4	1585	2496	0.15%	0.019%
14	3.288	603	606	610	rVB2	243	214	0.01%	0.002%
15	3.346	623	624	626	rBV2	385	206	0.01%	0.002%
16	3.462	656	660	665	rVB3	244	294	0.02%	0.002%
17	3.491	665	669	673	rBV2	227	215	0.01%	0.002%
18	3.649	714	718	721	rBV	360	261	0.02%	0.002%
19	3.729	735	743	745	rBV2	385	377	0.02%	0.003%
20	3.764	750	754	757	rVB	297	284	0.02%	0.002%
21	3.787	757	761	765	rBV2	480	452	0.03%	0.004%
22	3.854	778	782	789	rVB2	352	429	0.03%	0.003%
23	3.912	797	800	804	rBV2	240	194	0.01%	0.002%
24	4.012	826	831	833	rBV2	237	241	0.01%	0.002%
25	4.140	864	871	875	rBV	395	448	0.03%	0.003%
26	4.620	1005	1020	1064	rBV	175268	442547	26.23%	3.437%
27	4.964	1124	1127	1128	rBV	329	220	0.01%	0.002%
28	5.063	1141	1158	1182	rBV	302739	654174	38.77%	5.081%
29	5.333	1237	1242	1244	rBV	595	609	0.04%	0.005%
30	5.722	1341	1363	1393	rBV2	625147	1687472	100.00%	13.105%
31	5.976	1434	1442	1451	rVB5	1085	1735	0.10%	0.013%
32	6.034	1456	1460	1463	rBV3	645	461	0.03%	0.004%
33	6.092	1474	1478	1480	rBV	375	221	0.01%	0.002%
34	6.131	1487	1490	1494	rVB3	325	223	0.01%	0.002%
35	6.250	1511	1527	1549	rBV	417034	793291	47.01%	6.161%
36	6.529	1606	1614	1627	rVB6	1799	3381	0.20%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048294.D
 Acq On : 26 Apr 2022 12:20
 Operator : SY/MD
 Sample : VU0426MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.594	1629	1634	1637	rBV3	370	369	0.02%	0.003%
38	6.690	1649	1664	1692	rBV	388431	753910	44.68%	5.855%
39	6.803	1694	1699	1701	rBV4	811	874	0.05%	0.007%
40	6.896	1724	1728	1734	rBV2	372	411	0.02%	0.003%
41	6.960	1745	1748	1752	rBV3	318	263	0.02%	0.002%
42	7.176	1801	1815	1831	rVV5	3162	7802	0.46%	0.061%
43	7.253	1836	1839	1844	rVV	324	300	0.02%	0.002%
44	7.385	1877	1880	1884	rVB2	255	199	0.01%	0.002%
45	7.565	1920	1936	1956	rBV	210367	368959	21.86%	2.865%
46	7.668	1963	1968	1969	rBV2	374	258	0.02%	0.002%
47	7.793	1998	2007	2016	rBV6	2016	3327	0.20%	0.026%
48	7.899	2024	2040	2056	rBV	772319	1338981	79.35%	10.399%
49	8.179	2115	2127	2147	rBV	146279	249166	14.77%	1.935%
50	8.391	2189	2193	2195	rBV3	378	342	0.02%	0.003%
51	8.558	2241	2245	2249	rBV4	1055	688	0.04%	0.005%
52	8.635	2256	2269	2300	rBV	569340	1063492	63.02%	8.259%
53	8.832	2328	2330	2334	rBV2	560	291	0.02%	0.002%
54	9.028	2389	2391	2395	rVB2	404	227	0.01%	0.002%
55	9.208	2444	2447	2450	rBV	280	249	0.01%	0.002%
56	9.314	2477	2480	2484	rVB3	358	307	0.02%	0.002%
57	9.417	2498	2512	2544	rBV	618878	1044991	61.93%	8.116%
58	9.568	2553	2559	2568	rVB3	1260	1757	0.10%	0.014%
59	9.606	2568	2571	2577	rBV2	306	248	0.01%	0.002%
60	9.645	2579	2583	2584	rBV	328	233	0.01%	0.002%
61	9.690	2589	2597	2598	rBV	1256	1032	0.06%	0.008%
62	9.867	2649	2652	2655	rBV3	253	223	0.01%	0.002%
63	9.886	2655	2658	2663	rVB3	252	206	0.01%	0.002%
64	9.960	2675	2681	2683	rBV2	302	279	0.02%	0.002%
65	10.118	2718	2730	2738	rVB8	1493	2931	0.17%	0.023%
66	10.253	2764	2772	2775	rBV2	357	314	0.02%	0.002%
67	10.275	2775	2779	2781	rBV	319	312	0.02%	0.002%
68	10.484	2837	2844	2855	rVB5	1129	1903	0.11%	0.015%
69	10.565	2861	2869	2871	rBV2	302	303	0.02%	0.002%
70	10.671	2895	2902	2912	rVB3	2620	3440	0.20%	0.027%
71	10.758	2916	2929	2947	rBV	649680	1052697	62.38%	8.176%
72	10.825	2947	2950	2956	rVB3	1613	1641	0.10%	0.013%
73	10.867	2960	2963	2967	rBV3	557	514	0.03%	0.004%
74	11.037	3013	3016	3020	rBV	187	222	0.01%	0.002%
75	11.089	3027	3032	3036	rBV4	909	1099	0.07%	0.009%
76	11.320	3101	3104	3108	rBV2	262	235	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048294.D
 Acq On : 26 Apr 2022 12:20
 Operator : SY/MD
 Sample : VU0426MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.404	3126	3130	3131	rBV2	284	190	0.01%	0.001%
78	11.468	3140	3150	3161	rVB7	2821	5157	0.31%	0.040%
79	11.581	3181	3185	3189	rVB2	595	511	0.03%	0.004%
80	11.622	3194	3198	3200	rBV2	313	235	0.01%	0.002%
81	11.690	3215	3219	3221	rBV3	809	582	0.03%	0.005%
82	11.748	3227	3237	3244	rBV2	2543	3925	0.23%	0.030%
83	11.812	3244	3257	3281	rVV	621201	983452	58.28%	7.638%
84	11.928	3291	3293	3295	rBV	554	282	0.02%	0.002%
85	11.970	3303	3306	3307	rBV2	631	391	0.02%	0.003%
86	12.098	3343	3346	3349	rBV2	336	229	0.01%	0.002%
87	12.195	3362	3376	3398	rBV	760029	1230770	72.94%	9.559%
88	12.629	3507	3511	3513	rBV2	634	430	0.03%	0.003%
89	12.690	3526	3530	3532	rBV2	418	296	0.02%	0.002%
90	12.774	3551	3556	3558	rBV4	611	645	0.04%	0.005%
91	12.912	3593	3599	3602	rBV2	410	513	0.03%	0.004%
92	13.005	3623	3628	3631	rBV2	640	619	0.04%	0.005%
93	13.224	3690	3696	3709	rVB4	4178	6669	0.40%	0.052%
94	13.323	3723	3727	3728	rBV2	520	358	0.02%	0.003%
95	13.372	3738	3742	3744	rBV	284	273	0.02%	0.002%
96	13.407	3750	3753	3755	rBV2	376	239	0.01%	0.002%
97	13.680	3836	3838	3843	rVB2	381	239	0.01%	0.002%
98	13.844	3881	3889	3902	rVB3	9452	13999	0.83%	0.109%
99	14.092	3956	3966	3982	rBV2	21382	34879	2.07%	0.271%
100	14.333	4032	4041	4055	rVB2	11981	18813	1.11%	0.146%




Sum of corrected areas: 12876072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048294.D
Acq On : 26 Apr 2022 12:20
Operator : SY/MD
Sample : VU0426MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

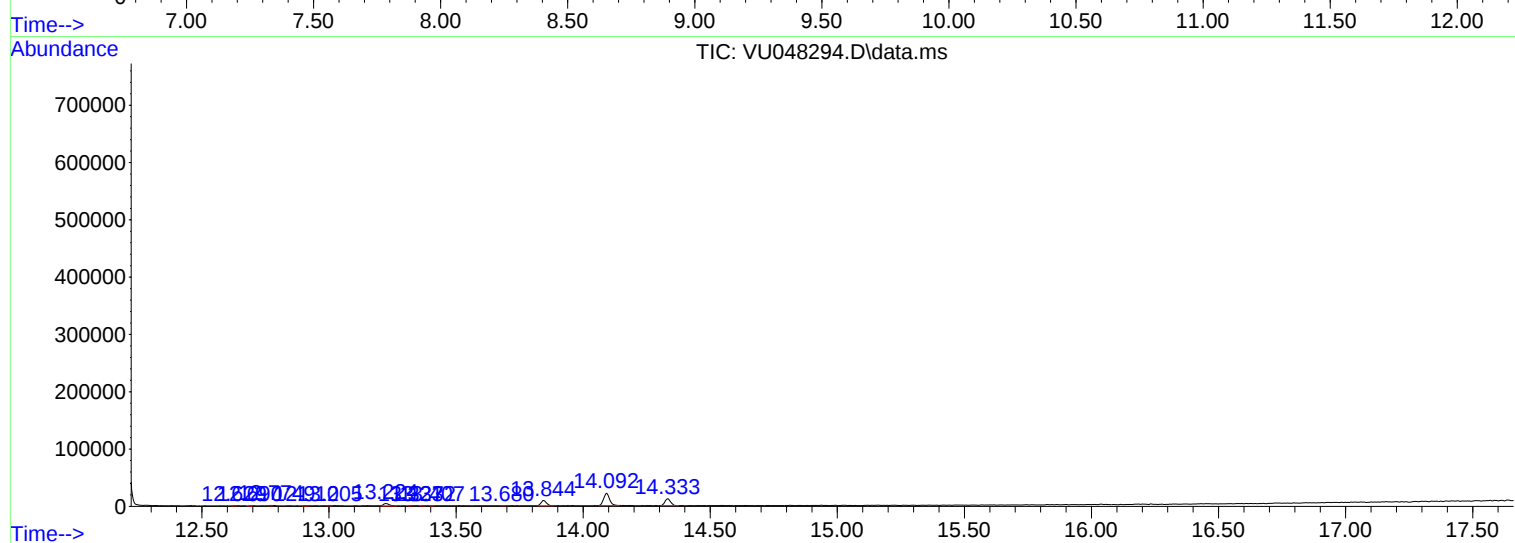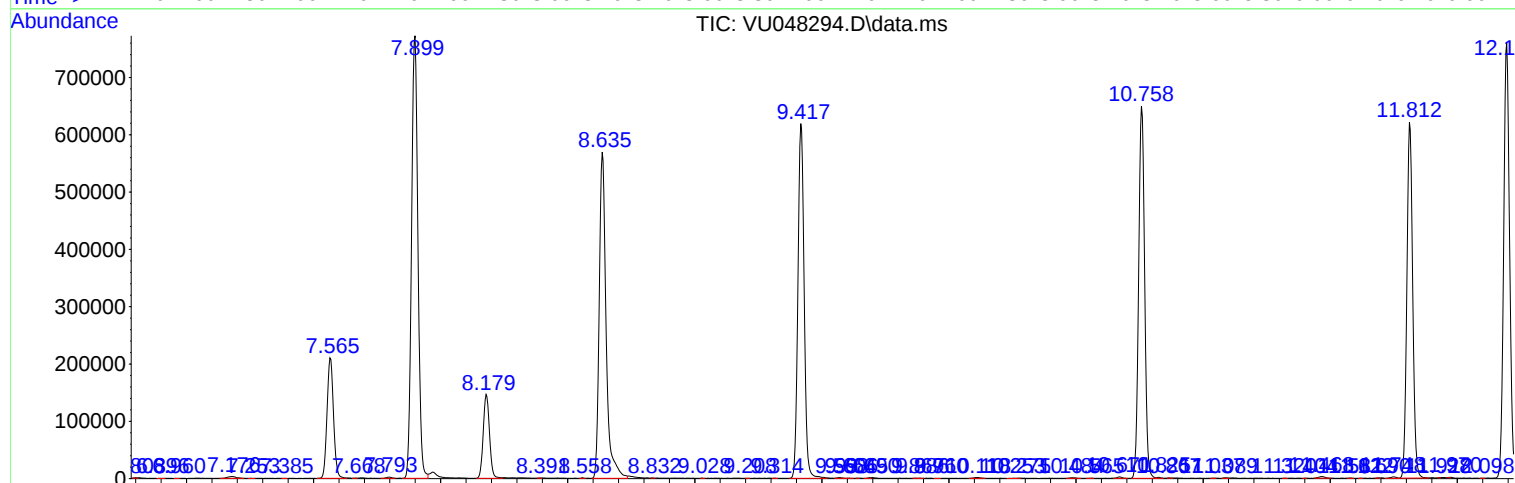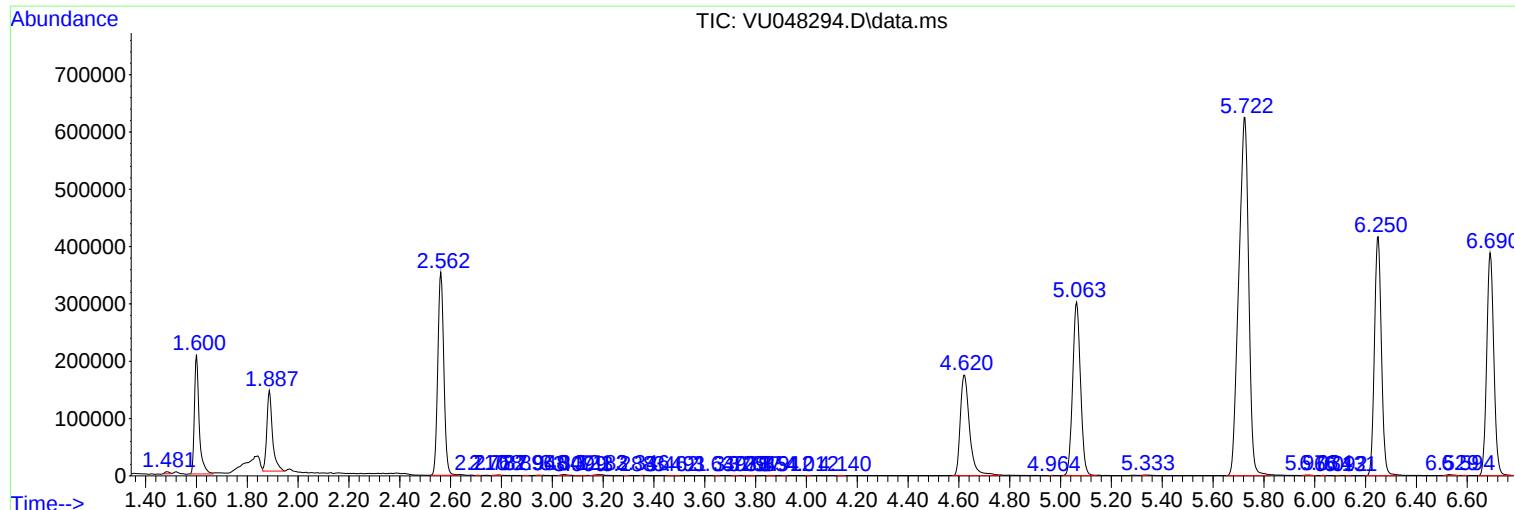

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048294.D
Acq On : 26 Apr 2022 12:20
Operator : SY/MD
Sample : VU0426MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048294.D
Acq On : 26 Apr 2022 12:20
Operator : SY/MD
Sample : VU0426MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK112

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc