

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048296.D
 Acq On : 26 Apr 2022 13:06
 Operator : SY/MD
 Sample : N2518-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	39	47	52	rBV2	21980	27369	1.70%	0.219%
2	1.600	73	81	100	rBV	159022	210792	13.10%	1.689%
3	1.877	161	167	194	rVB	139308	221848	13.78%	1.778%
4	2.559	366	379	393	rBV	314076	526047	32.68%	4.215%
5	2.629	394	401	416	rVB	16529	29740	1.85%	0.238%
6	2.784	445	449	450	rBV2	478	341	0.02%	0.003%
7	2.829	460	463	467	rBV2	468	338	0.02%	0.003%
8	2.903	477	486	491	rBV4	1254	1928	0.12%	0.015%
9	2.957	501	503	510	rVB4	746	788	0.05%	0.006%
10	3.038	523	528	529	rBV3	561	431	0.03%	0.003%
11	3.121	550	554	558	rBV2	346	269	0.02%	0.002%
12	3.182	560	573	586	rBV	5813	13518	0.84%	0.108%
13	3.362	626	629	630	rBV2	320	211	0.01%	0.002%
14	3.436	648	652	655	rBV2	189	193	0.01%	0.002%
15	3.578	691	696	701	rBV4	900	1294	0.08%	0.010%
16	3.668	719	724	725	rBV2	244	169	0.01%	0.001%
17	3.700	730	734	739	rVV2	250	233	0.01%	0.002%
18	3.832	772	775	778	rBV	292	221	0.01%	0.002%
19	3.922	801	803	809	rVV3	286	265	0.02%	0.002%
20	3.996	820	826	829	rBV2	289	345	0.02%	0.003%
21	4.215	892	894	897	rBV2	235	178	0.01%	0.001%
22	4.346	932	935	940	rBV2	273	314	0.02%	0.003%
23	4.388	945	948	952	rVB2	250	180	0.01%	0.001%
24	4.481	972	977	979	rVB3	353	313	0.02%	0.003%
25	4.555	984	1000	1006	rBV2	2516	6059	0.38%	0.049%
26	4.623	1007	1021	1043	rBV	176217	449111	27.90%	3.598%
27	5.060	1141	1157	1183	rVV	292638	642632	39.93%	5.149%
28	5.186	1194	1196	1202	rVB2	353	271	0.02%	0.002%
29	5.288	1215	1228	1234	rBV2	918	1634	0.10%	0.013%
30	5.430	1269	1272	1275	rVB2	258	171	0.01%	0.001%
31	5.504	1290	1295	1299	rBV2	316	324	0.02%	0.003%
32	5.722	1340	1363	1388	rBV2	596322	1609573	100.00%	12.896%
33	5.909	1419	1421	1425	rVB2	333	197	0.01%	0.002%
34	5.964	1432	1438	1439	rBV2	1295	1220	0.08%	0.010%
35	6.115	1480	1485	1488	rBV2	542	457	0.03%	0.004%
36	6.147	1492	1495	1496	rBV	442	200	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048296.D
 Acq On : 26 Apr 2022 13:06
 Operator : SY/MD
 Sample : N2518-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.189	1504	1508	1511	rBV	322	206	0.01%	0.002%
38	6.247	1511	1526	1556	rBV	416503	791597	49.18%	6.343%
39	6.430	1580	1583	1589	rVB4	387	337	0.02%	0.003%
40	6.472	1592	1596	1600	rVB3	333	196	0.01%	0.002%
41	6.491	1600	1602	1606	rBV2	299	225	0.01%	0.002%
42	6.530	1606	1614	1623	rBV5	1212	2298	0.14%	0.018%
43	6.690	1648	1664	1690	rBV	375694	735033	45.67%	5.889%
44	6.796	1693	1697	1700	rBV4	867	774	0.05%	0.006%
45	7.031	1767	1770	1772	rBV2	357	195	0.01%	0.002%
46	7.124	1797	1799	1802	rVB2	374	182	0.01%	0.001%
47	7.176	1803	1815	1828	rBV5	5486	12130	0.75%	0.097%
48	7.266	1840	1843	1846	rVB2	357	175	0.01%	0.001%
49	7.407	1883	1887	1890	rBV	216	172	0.01%	0.001%
50	7.423	1890	1892	1897	rVB2	318	201	0.01%	0.002%
51	7.449	1897	1900	1904	rBV2	343	350	0.02%	0.003%
52	7.565	1922	1936	1957	rBV	183294	322565	20.04%	2.585%
53	7.648	1959	1962	1964	rVV	501	383	0.02%	0.003%
54	7.690	1967	1975	1988	rVB3	2162	3801	0.24%	0.030%
55	7.787	2001	2005	2006	rBV2	391	253	0.02%	0.002%
56	7.800	2006	2009	2016	rVB3	616	599	0.04%	0.005%
57	7.896	2026	2039	2055	rBV	707866	1226138	76.18%	9.824%
58	8.124	2107	2110	2114	rVB3	223	178	0.01%	0.001%
59	8.179	2114	2127	2141	rBV2	130311	222007	13.79%	1.779%
60	8.475	2207	2219	2229	rBV2	2686	4901	0.30%	0.039%
61	8.555	2240	2244	2248	rBV2	384	300	0.02%	0.002%
62	8.578	2248	2251	2254	rVB2	415	241	0.01%	0.002%
63	8.639	2254	2270	2304	rBV	580481	1125477	69.92%	9.018%
64	9.111	2412	2417	2420	rBV2	320	260	0.02%	0.002%
65	9.163	2428	2433	2435	rBV2	326	284	0.02%	0.002%
66	9.214	2446	2449	2455	rBV2	195	180	0.01%	0.001%
67	9.298	2472	2475	2478	rBV2	386	251	0.02%	0.002%
68	9.336	2484	2487	2494	rBV	314	317	0.02%	0.003%
69	9.417	2498	2512	2533	rBV	617576	1032732	64.16%	8.275%
70	9.536	2547	2549	2554	rVB4	361	171	0.01%	0.001%
71	9.655	2583	2586	2590	rBV3	370	310	0.02%	0.002%
72	9.693	2592	2598	2607	rVB3	1391	2087	0.13%	0.017%
73	9.845	2643	2645	2651	rBV2	168	182	0.01%	0.001%
74	9.915	2660	2667	2671	rBV2	438	586	0.04%	0.005%
75	10.108	2724	2727	2730	rVV3	527	431	0.03%	0.003%
76	10.359	2803	2805	2810	rVB2	336	202	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048296.D
 Acq On : 26 Apr 2022 13:06
 Operator : SY/MD
 Sample : N2518-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.484	2837	2844	2845	rBV2	475	527	0.03%	0.004%
78	10.674	2891	2903	2912	rBV6	1702	2703	0.17%	0.022%
79	10.758	2915	2929	2947	rBV	659971	1073427	66.69%	8.601%
80	10.893	2963	2971	2983	rVB3	4424	6869	0.43%	0.055%
81	11.121	3039	3042	3046	rBV2	425	293	0.02%	0.002%
82	11.237	3076	3078	3085	rBV	242	259	0.02%	0.002%
83	11.317	3100	3103	3105	rBV3	457	349	0.02%	0.003%
84	11.478	3140	3153	3163	rBV9	2378	6198	0.39%	0.050%
85	11.697	3216	3221	3229	rVB4	741	1000	0.06%	0.008%
86	11.748	3230	3237	3244	rBV5	1062	1247	0.08%	0.010%
87	11.812	3244	3257	3276	rBV	609070	958767	59.57%	7.682%
88	11.938	3292	3296	3301	rBV4	705	665	0.04%	0.005%
89	12.066	3329	3336	3340	rBV6	1154	1518	0.09%	0.012%
90	12.195	3362	3376	3394	rBV	712002	1171950	72.81%	9.390%
91	12.420	3444	3446	3449	rVB	414	179	0.01%	0.001%
92	12.446	3449	3454	3456	rBV2	318	343	0.02%	0.003%
93	12.516	3472	3476	3477	rBV2	340	242	0.02%	0.002%
94	12.770	3548	3555	3564	rBV4	1627	2463	0.15%	0.020%
95	13.012	3627	3630	3632	rBV2	288	205	0.01%	0.002%
96	13.298	3717	3719	3723	rBV2	270	183	0.01%	0.001%
97	13.844	3885	3889	3890	rBV3	1961	1340	0.08%	0.011%
98	14.095	3960	3967	3979	rVB2	4313	6322	0.39%	0.051%
99	14.333	4035	4041	4052	rVB7	2914	4521	0.28%	0.036%
100	14.995	4241	4247	4252	rBV4	699	1058	0.07%	0.008%




Sum of corrected areas: 12480709

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048296.D
Acq On : 26 Apr 2022 13:06
Operator : SY/MD
Sample : N2518-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

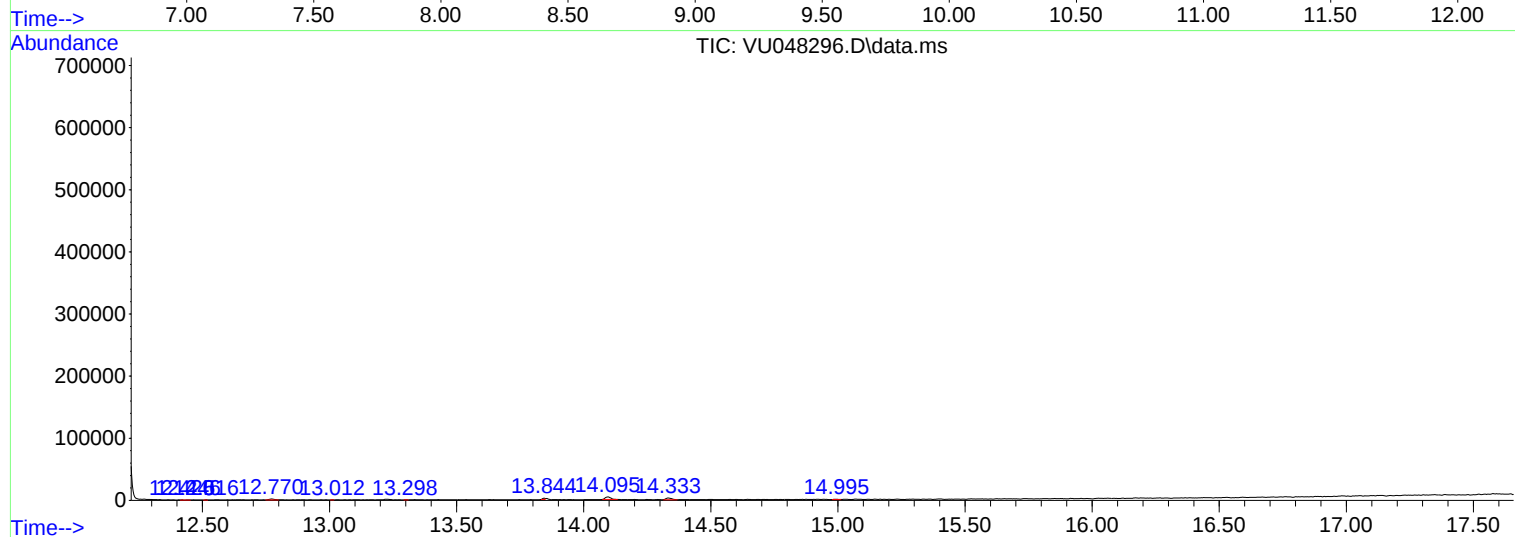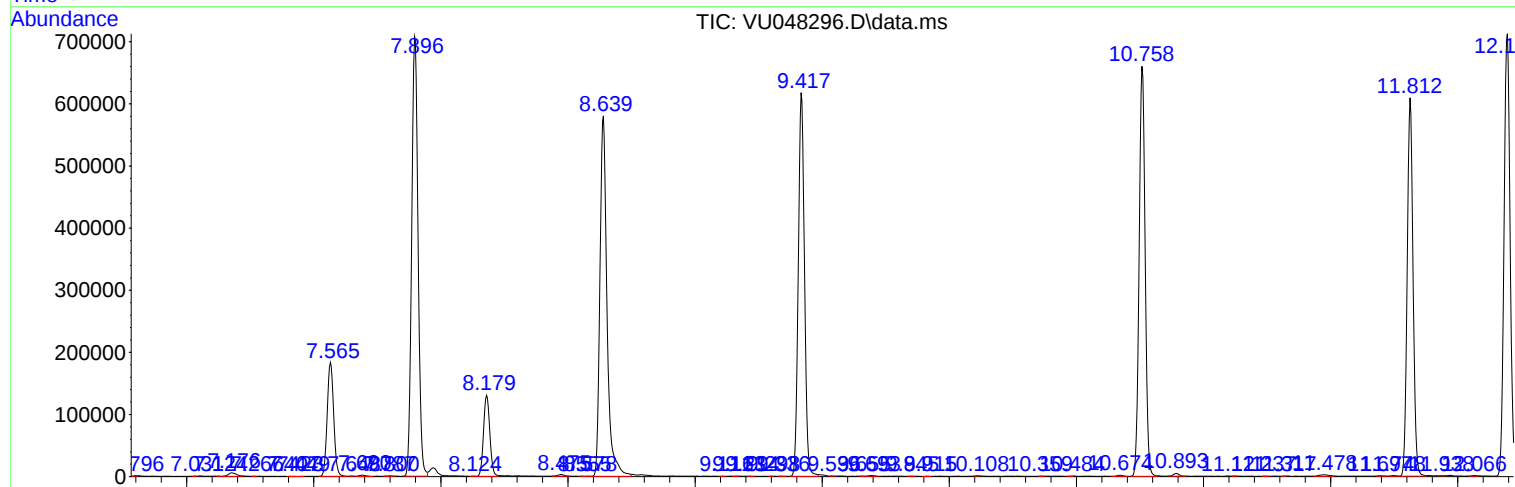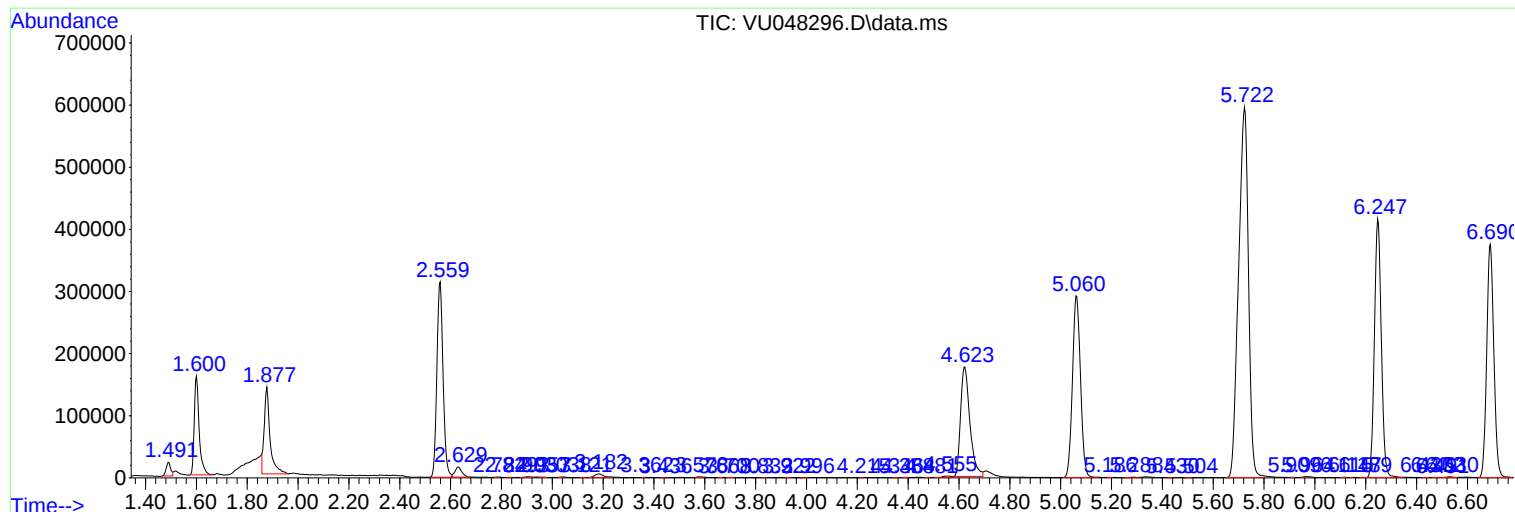

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048296.D
Acq On : 26 Apr 2022 13:06
Operator : SY/MD
Sample : N2518-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048296.D
Acq On : 26 Apr 2022 13:06
Operator : SY/MD
Sample : N2518-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------