

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048299.D
 Acq On : 26 Apr 2022 14:18
 Operator : SY/MD
 Sample : N2518-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048299.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	39	47	54	rBV2	25582	31570	1.90%	0.255%
2	1.600	72	81	102	rBV	200670	257330	15.45%	2.080%
3	1.893	163	172	189	rVB	133569	199838	12.00%	1.615%
4	2.562	368	380	393	rBV	347100	567927	34.11%	4.590%
5	2.626	394	400	415	rVB	17174	29368	1.76%	0.237%
6	2.764	441	443	445	rBV2	359	217	0.01%	0.002%
7	2.861	469	473	476	rVB3	291	234	0.01%	0.002%
8	2.909	476	488	494	rBV5	1259	2642	0.16%	0.021%
9	2.967	504	506	513	rVB3	472	416	0.02%	0.003%
10	3.031	523	526	527	rBV2	405	229	0.01%	0.002%
11	3.047	527	531	537	rVB2	1190	1271	0.08%	0.010%
12	3.089	537	544	545	rBV2	274	359	0.02%	0.003%
13	3.189	563	575	590	rBV5	2290	5940	0.36%	0.048%
14	3.314	610	614	619	rBV2	188	214	0.01%	0.002%
15	3.501	669	672	674	rBV2	335	223	0.01%	0.002%
16	3.571	683	694	696	rBV4	942	1259	0.08%	0.010%
17	3.771	752	756	761	rVB2	231	196	0.01%	0.002%
18	3.861	778	784	785	rBV	204	190	0.01%	0.002%
19	4.436	954	963	964	rBV2	460	521	0.03%	0.004%
20	4.555	989	1000	1006	rBV3	2539	5524	0.33%	0.045%
21	4.620	1007	1020	1041	rBV	170174	411511	24.71%	3.326%
22	4.903	1106	1108	1113	rVB3	215	188	0.01%	0.002%
23	4.944	1118	1121	1127	rVB2	234	229	0.01%	0.002%
24	5.063	1140	1158	1180	rBV	295444	648078	38.92%	5.238%
25	5.169	1189	1191	1196	rBV3	360	289	0.02%	0.002%
26	5.276	1221	1224	1226	rBV3	331	235	0.01%	0.002%
27	5.340	1234	1244	1253	rBV5	1087	2194	0.13%	0.018%
28	5.526	1299	1302	1306	rVV2	277	204	0.01%	0.002%
29	5.726	1339	1364	1400	rBV2	620099	1665060	100.00%	13.458%
30	5.977	1433	1442	1447	rVB4	945	1498	0.09%	0.012%
31	6.038	1456	1461	1465	rBV4	455	491	0.03%	0.004%
32	6.112	1481	1484	1491	rBV	365	416	0.02%	0.003%
33	6.250	1512	1527	1557	rBV	400910	759475	45.61%	6.139%
34	6.530	1607	1614	1621	rBV4	1235	1889	0.11%	0.015%
35	6.562	1621	1624	1629	rVB3	286	226	0.01%	0.002%
36	6.690	1649	1664	1691	rVV	383807	742246	44.58%	5.999%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048299.D
 Acq On : 26 Apr 2022 14:18
 Operator : SY/MD
 Sample : N2518-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.806	1697	1700	1704	rVV3	661	586	0.04%	0.005%
38	7.079	1783	1785	1790	rVB2	299	200	0.01%	0.002%
39	7.112	1790	1795	1800	rBV4	463	583	0.04%	0.005%
40	7.179	1804	1816	1828	rVV5	2723	5612	0.34%	0.045%
41	7.565	1923	1936	1951	rBV	203235	354355	21.28%	2.864%
42	7.687	1968	1974	1982	rVB5	950	1519	0.09%	0.012%
43	7.777	1999	2002	2004	rBV2	285	191	0.01%	0.002%
44	7.812	2010	2013	2018	rVB3	477	358	0.02%	0.003%
45	7.899	2025	2040	2056	rBV	753752	1308285	78.57%	10.575%
46	8.179	2107	2127	2146	rBV	144325	241796	14.52%	1.954%
47	8.292	2159	2162	2165	rVB2	490	317	0.02%	0.003%
48	8.343	2175	2178	2184	rVB3	455	401	0.02%	0.003%
49	8.388	2190	2192	2197	rVB2	392	236	0.01%	0.002%
50	8.468	2213	2217	2226	rVB3	967	1419	0.09%	0.011%
51	8.529	2235	2236	2241	rVB	388	191	0.01%	0.002%
52	8.552	2241	2243	2245	rBV	374	195	0.01%	0.002%
53	8.565	2245	2247	2253	rVB	359	193	0.01%	0.002%
54	8.636	2257	2269	2297	rBV	532895	1012679	60.82%	8.185%
55	8.935	2358	2362	2365	rBV3	317	315	0.02%	0.003%
56	9.066	2398	2403	2405	rVV2	240	246	0.01%	0.002%
57	9.079	2405	2407	2413	rVV2	330	249	0.01%	0.002%
58	9.108	2414	2416	2425	rVB3	319	336	0.02%	0.003%
59	9.156	2429	2431	2437	rBV2	376	406	0.02%	0.003%
60	9.185	2438	2440	2444	rVB2	392	198	0.01%	0.002%
61	9.234	2452	2455	2460	rVB	345	308	0.02%	0.002%
62	9.288	2466	2472	2478	rVB3	294	365	0.02%	0.003%
63	9.417	2499	2512	2533	rBV	592757	986010	59.22%	7.970%
64	9.568	2552	2559	2566	rBV3	714	996	0.06%	0.008%
65	9.645	2579	2583	2589	rBV2	523	667	0.04%	0.005%
66	9.693	2592	2598	2607	rVV3	1097	1489	0.09%	0.012%
67	10.108	2720	2727	2729	rBV2	558	616	0.04%	0.005%
68	10.362	2802	2806	2809	rVB	406	282	0.02%	0.002%
69	10.594	2875	2878	2882	rBV	245	197	0.01%	0.002%
70	10.671	2893	2902	2910	rVB5	2174	2712	0.16%	0.022%
71	10.758	2916	2929	2953	rBV	628622	1014806	60.95%	8.203%
72	10.844	2953	2956	2959	rBV2	281	194	0.01%	0.002%
73	10.896	2963	2972	2978	rVB4	1900	3186	0.19%	0.026%
74	11.047	3016	3019	3022	rBV	413	317	0.02%	0.003%
75	11.086	3029	3031	3035	rBV2	268	253	0.02%	0.002%
76	11.111	3036	3039	3046	rVB3	542	661	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048299.D
 Acq On : 26 Apr 2022 14:18
 Operator : SY/MD
 Sample : N2518-10
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.327	3100	3106	3110	rBV3	495	635	0.04%	0.005%
78	11.414	3130	3133	3137	rBV4	266	193	0.01%	0.002%
79	11.455	3141	3146	3148	rBV3	1099	1146	0.07%	0.009%
80	11.571	3179	3182	3184	rBV	309	226	0.01%	0.002%
81	11.700	3216	3222	3231	rBV5	1140	1575	0.09%	0.013%
82	11.745	3233	3236	3243	rBV4	596	775	0.05%	0.006%
83	11.812	3243	3257	3278	rBV	562026	902216	54.19%	7.292%
84	11.941	3295	3297	3300	rBV3	488	329	0.02%	0.003%
85	11.967	3302	3305	3317	rVB7	1980	2827	0.17%	0.023%
86	12.070	3328	3337	3346	rVV5	2575	4813	0.29%	0.039%
87	12.195	3360	3376	3397	rBV	718399	1168240	70.16%	9.443%
88	12.324	3413	3416	3421	rVB5	819	610	0.04%	0.005%
89	12.516	3473	3476	3480	rVB3	425	323	0.02%	0.003%
90	12.549	3481	3486	3487	rBV3	297	224	0.01%	0.002%
91	12.616	3503	3507	3510	rBV	462	495	0.03%	0.004%
92	12.635	3510	3513	3514	rBV2	535	288	0.02%	0.002%
93	12.777	3548	3557	3558	rBV3	692	934	0.06%	0.008%
94	12.812	3565	3568	3574	rVB2	269	235	0.01%	0.002%
95	12.848	3574	3579	3582	rVB3	383	317	0.02%	0.003%
96	12.886	3586	3591	3595	rBV2	277	356	0.02%	0.003%
97	13.092	3651	3655	3660	rBV2	492	546	0.03%	0.004%
98	13.848	3888	3890	3893	rBV3	654	339	0.02%	0.003%
99	14.918	4220	4223	4226	rBV3	550	362	0.02%	0.003%
100	15.249	4323	4326	4327	rBV	508	254	0.02%	0.002%




Sum of corrected areas: 12371880

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048299.D
Acq On : 26 Apr 2022 14:18
Operator : SY/MD
Sample : N2518-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

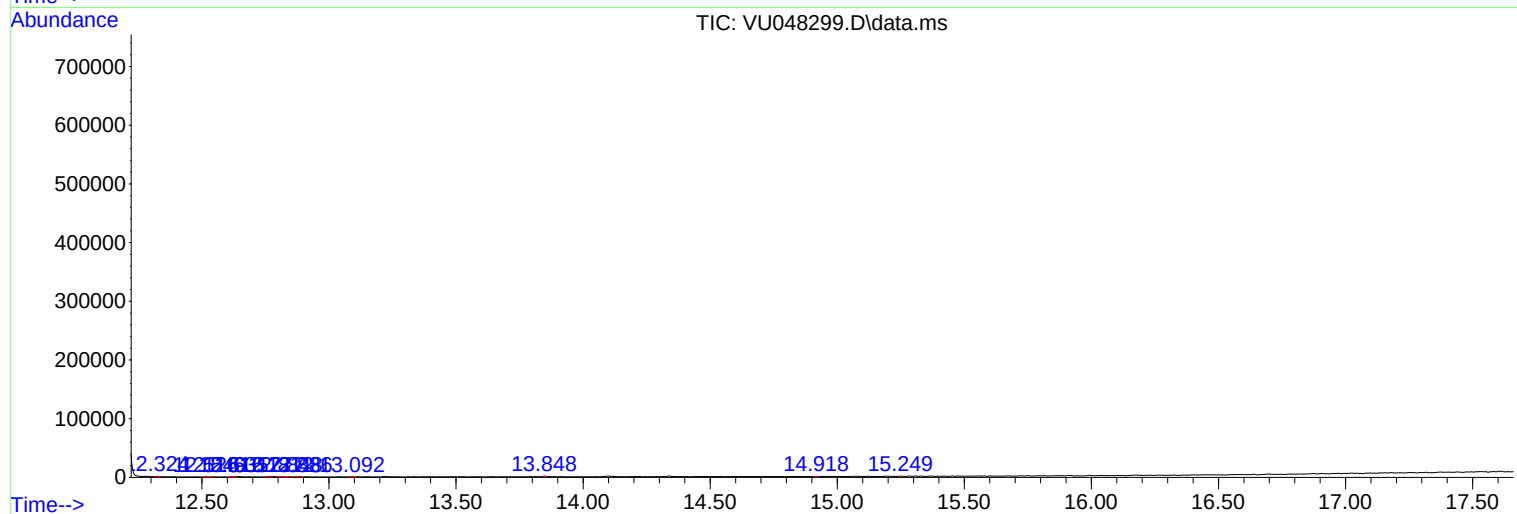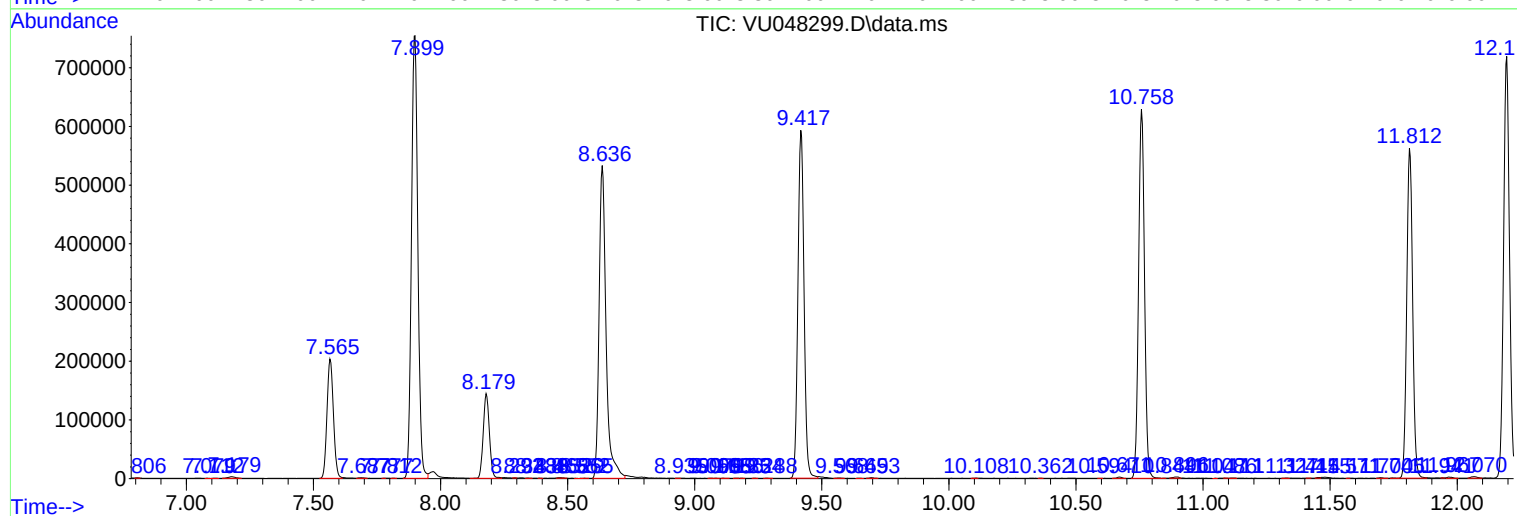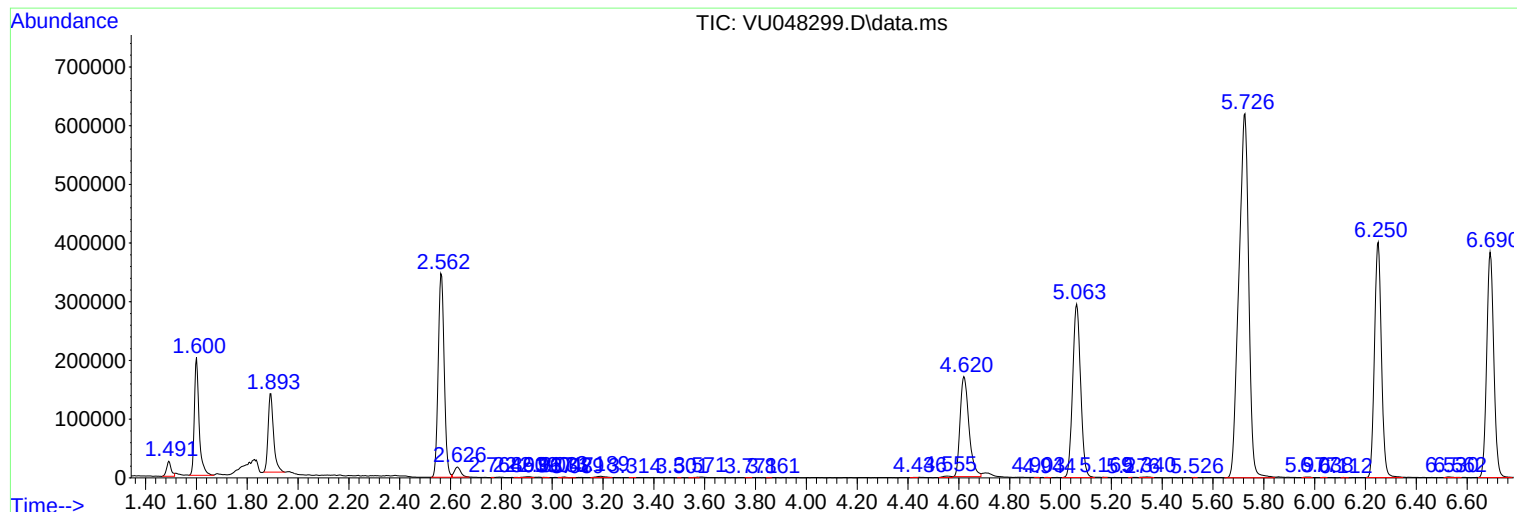

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048299.D
Acq On : 26 Apr 2022 14:18
Operator : SY/MD
Sample : N2518-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048299.D
Acq On : 26 Apr 2022 14:18
Operator : SY/MD
Sample : N2518-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------