

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048300.D
 Acq On : 26 Apr 2022 14:43
 Operator : SY/MD
 Sample : N2518-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	100	rBV	148175	189604	12.96%	1.759%
2	1.893	164	172	189	rVB	109682	161822	11.06%	1.501%
3	2.565	368	381	396	rBV	260106	430599	29.44%	3.994%
4	2.736	431	434	437	rBV2	433	362	0.02%	0.003%
5	2.774	437	446	448	rBV3	1046	1328	0.09%	0.012%
6	2.957	495	503	507	rBV3	338	509	0.03%	0.005%
7	3.048	522	531	545	rBV5	2416	4650	0.32%	0.043%
8	3.099	545	547	551	rVB2	236	142	0.01%	0.001%
9	3.128	551	556	560	rBV	317	377	0.03%	0.003%
10	3.183	560	573	597	rBV	24852	63429	4.34%	0.588%
11	3.289	601	606	607	rBV	185	137	0.01%	0.001%
12	3.356	624	627	630	rBV2	163	143	0.01%	0.001%
13	3.382	632	635	639	rVB2	327	212	0.01%	0.002%
14	3.591	697	700	707	rVB2	265	234	0.02%	0.002%
15	3.684	726	729	732	rBV2	247	146	0.01%	0.001%
16	3.729	737	743	745	rBV2	290	357	0.02%	0.003%
17	3.858	780	783	785	rBV	285	176	0.01%	0.002%
18	3.948	809	811	815	rVB2	267	188	0.01%	0.002%
19	3.990	821	824	827	rBV	234	145	0.01%	0.001%
20	4.041	838	840	843	rBV	216	147	0.01%	0.001%
21	4.186	877	885	888	rBV2	249	397	0.03%	0.004%
22	4.282	912	915	917	rVB2	242	148	0.01%	0.001%
23	4.301	917	921	925	rBV2	260	331	0.02%	0.003%
24	4.478	971	976	979	rBV	240	235	0.02%	0.002%
25	4.549	996	998	1002	rBV3	245	148	0.01%	0.001%
26	4.620	1006	1020	1044	rBV	169377	415326	28.39%	3.852%
27	5.064	1140	1158	1188	rBV	261901	571802	39.09%	5.304%
28	5.279	1223	1225	1229	rBV3	304	301	0.02%	0.003%
29	5.340	1236	1244	1255	rVB4	1275	2588	0.18%	0.024%
30	5.446	1274	1277	1283	rVB	207	145	0.01%	0.001%
31	5.478	1284	1287	1293	rBV2	162	177	0.01%	0.002%
32	5.726	1342	1364	1397	rBV2	525644	1462779	100.00%	13.569%
33	5.967	1434	1439	1440	rBV2	778	540	0.04%	0.005%
34	6.009	1449	1452	1454	rBV	235	159	0.01%	0.001%
35	6.250	1512	1527	1546	rBV	334730	637274	43.57%	5.911%
36	6.456	1585	1591	1592	rBV2	216	250	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048300.D
 Acq On : 26 Apr 2022 14:43
 Operator : SY/MD
 Sample : N2518-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.533	1608	1615	1621	rBV6	1014	1609	0.11%	0.015%
38	6.588	1628	1632	1634	rBV2	404	295	0.02%	0.003%
39	6.690	1650	1664	1693	rBV	344375	671691	45.92%	6.230%
40	6.803	1693	1699	1705	rVV6	1032	1500	0.10%	0.014%
41	6.983	1751	1755	1757	rBV2	209	165	0.01%	0.002%
42	7.041	1766	1773	1774	rBV	369	300	0.02%	0.003%
43	7.170	1802	1813	1814	rBV4	2220	2792	0.19%	0.026%
44	7.430	1883	1894	1896	rBV3	385	521	0.04%	0.005%
45	7.494	1910	1914	1916	rBV	235	175	0.01%	0.002%
46	7.510	1916	1919	1923	rVV2	177	165	0.01%	0.002%
47	7.565	1923	1936	1959	rVV	183444	318599	21.78%	2.955%
48	7.684	1968	1973	1975	rBV2	617	601	0.04%	0.006%
49	7.797	1992	2008	2020	rVB6	2541	5120	0.35%	0.047%
50	7.899	2026	2040	2055	rBV	622587	1081833	73.96%	10.035%
51	8.060	2087	2090	2093	rBV3	456	269	0.02%	0.002%
52	8.179	2111	2127	2151	rBV	129601	223765	15.30%	2.076%
53	8.462	2211	2215	2217	rBV2	496	471	0.03%	0.004%
54	8.636	2255	2269	2313	rBV	503293	975080	66.66%	9.045%
55	8.957	2366	2369	2371	rBV2	360	166	0.01%	0.002%
56	9.002	2381	2383	2386	rVV2	297	165	0.01%	0.002%
57	9.218	2446	2450	2452	rBV2	306	289	0.02%	0.003%
58	9.276	2465	2468	2472	rVB3	336	275	0.02%	0.003%
59	9.417	2497	2512	2547	rBV	510031	842319	57.58%	7.813%
60	9.645	2581	2583	2586	rVV2	216	144	0.01%	0.001%
61	9.694	2593	2598	2604	rBV3	729	829	0.06%	0.008%
62	9.886	2651	2658	2661	rBV2	268	393	0.03%	0.004%
63	9.935	2669	2673	2675	rBV	226	224	0.02%	0.002%
64	10.022	2697	2700	2704	rVB	196	160	0.01%	0.001%
65	10.099	2717	2724	2726	rBV3	468	566	0.04%	0.005%
66	10.259	2769	2774	2777	rBV2	241	197	0.01%	0.002%
67	10.282	2777	2781	2783	rBV2	267	238	0.02%	0.002%
68	10.321	2790	2793	2797	rVB	345	208	0.01%	0.002%
69	10.340	2797	2799	2802	rBV2	274	147	0.01%	0.001%
70	10.420	2822	2824	2833	rVB2	237	357	0.02%	0.003%
71	10.462	2833	2837	2840	rBV	321	297	0.02%	0.003%
72	10.488	2842	2845	2851	rVB2	635	481	0.03%	0.004%
73	10.546	2861	2863	2865	rBV	242	151	0.01%	0.001%
74	10.642	2889	2893	2895	rBV	223	207	0.01%	0.002%
75	10.674	2895	2903	2911	rVB3	1602	2271	0.16%	0.021%
76	10.758	2915	2929	2949	rBV	590334	957873	65.48%	8.885%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048300.D
 Acq On : 26 Apr 2022 14:43
 Operator : SY/MD
 Sample : N2518-14
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.857	2958	2960	2964	rBV2	289	143	0.01%	0.001%
78	10.883	2965	2968	2977	rVB3	764	902	0.06%	0.008%
79	10.954	2986	2990	2994	rBV2	212	228	0.02%	0.002%
80	11.092	3030	3033	3035	rBV2	402	242	0.02%	0.002%
81	11.111	3035	3039	3040	rBV2	284	167	0.01%	0.002%
82	11.173	3055	3058	3060	rVB	264	138	0.01%	0.001%
83	11.189	3060	3063	3068	rVB	214	184	0.01%	0.002%
84	11.417	3131	3134	3136	rVB	221	137	0.01%	0.001%
85	11.465	3140	3149	3154	rBV5	1320	2315	0.16%	0.021%
86	11.616	3193	3196	3200	rBV2	335	284	0.02%	0.003%
87	11.693	3213	3220	3226	rBV4	740	913	0.06%	0.008%
88	11.758	3235	3240	3242	rBV4	424	343	0.02%	0.003%
89	11.812	3245	3257	3278	rBV	473933	753395	51.50%	6.988%
90	11.970	3303	3306	3307	rBV2	630	411	0.03%	0.004%
91	12.195	3361	3376	3395	rBV	596057	977811	66.85%	9.070%
92	12.365	3427	3429	3430	rBV	396	207	0.01%	0.002%
93	12.398	3436	3439	3441	rBV2	400	289	0.02%	0.003%
94	12.510	3472	3474	3479	rBV2	325	237	0.02%	0.002%
95	12.558	3486	3489	3492	rBV	452	344	0.02%	0.003%
96	12.713	3535	3537	3540	rVB	293	148	0.01%	0.001%
97	12.870	3583	3586	3588	rBV	433	287	0.02%	0.003%
98	12.931	3601	3605	3608	rBV	794	755	0.05%	0.007%
99	13.838	3884	3887	3889	rBV3	385	276	0.02%	0.003%
100	15.516	4407	4409	4411	rBV3	663	322	0.02%	0.003%




Sum of corrected areas: 10780693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048300.D
Acq On : 26 Apr 2022 14:43
Operator : SY/MD
Sample : N2518-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

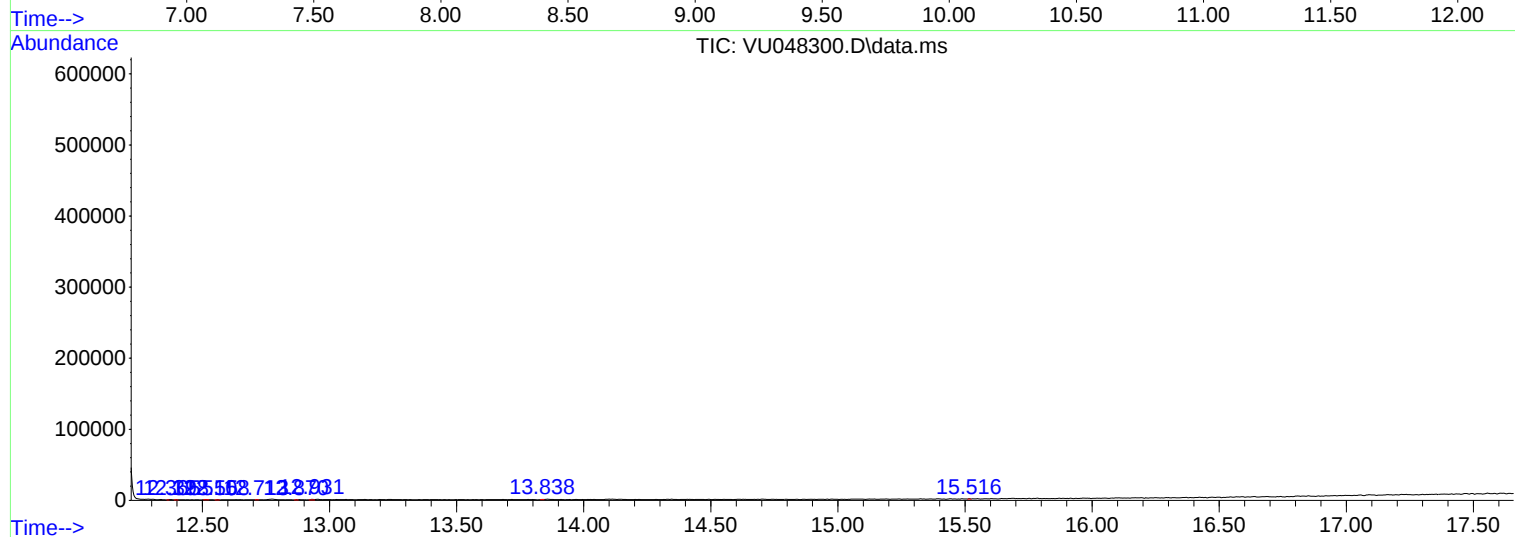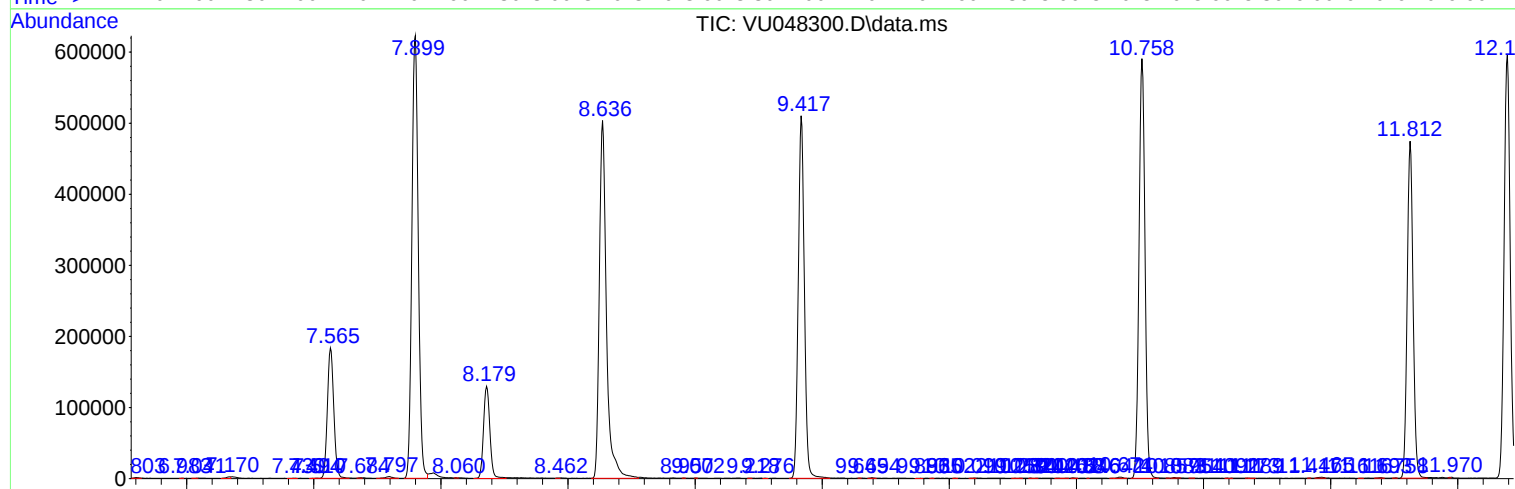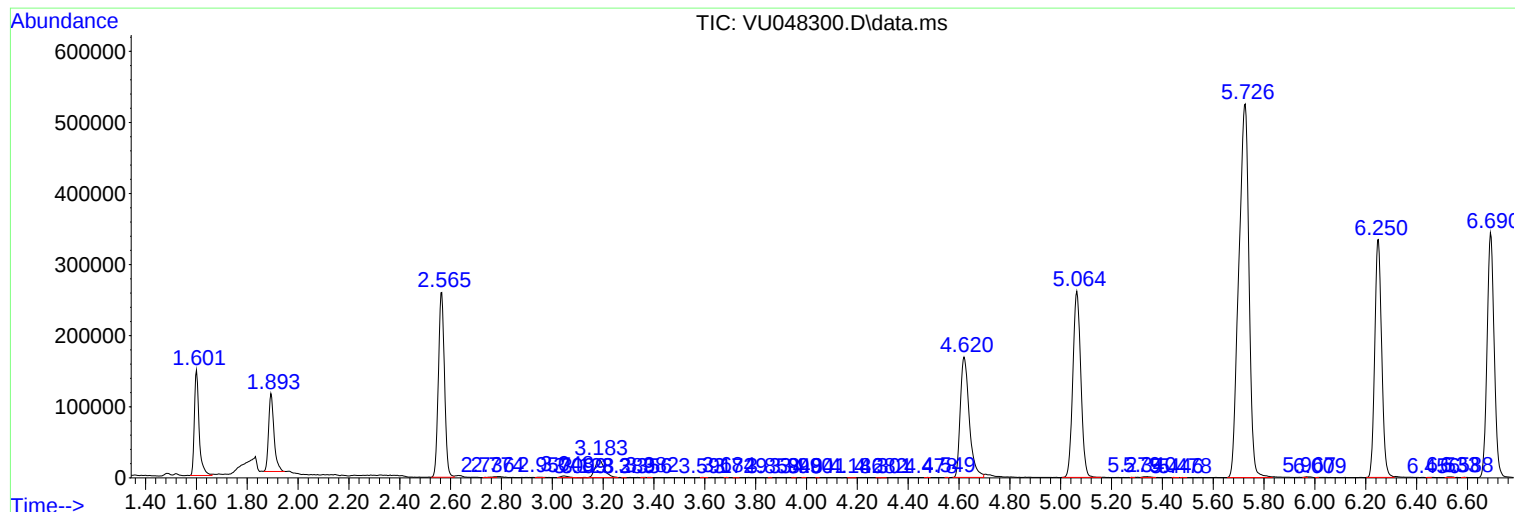

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048300.D
Acq On : 26 Apr 2022 14:43
Operator : SY/MD
Sample : N2518-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
Data File : VU048300.D
Acq On : 26 Apr 2022 14:43
Operator : SY/MD
Sample : N2518-14
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------