
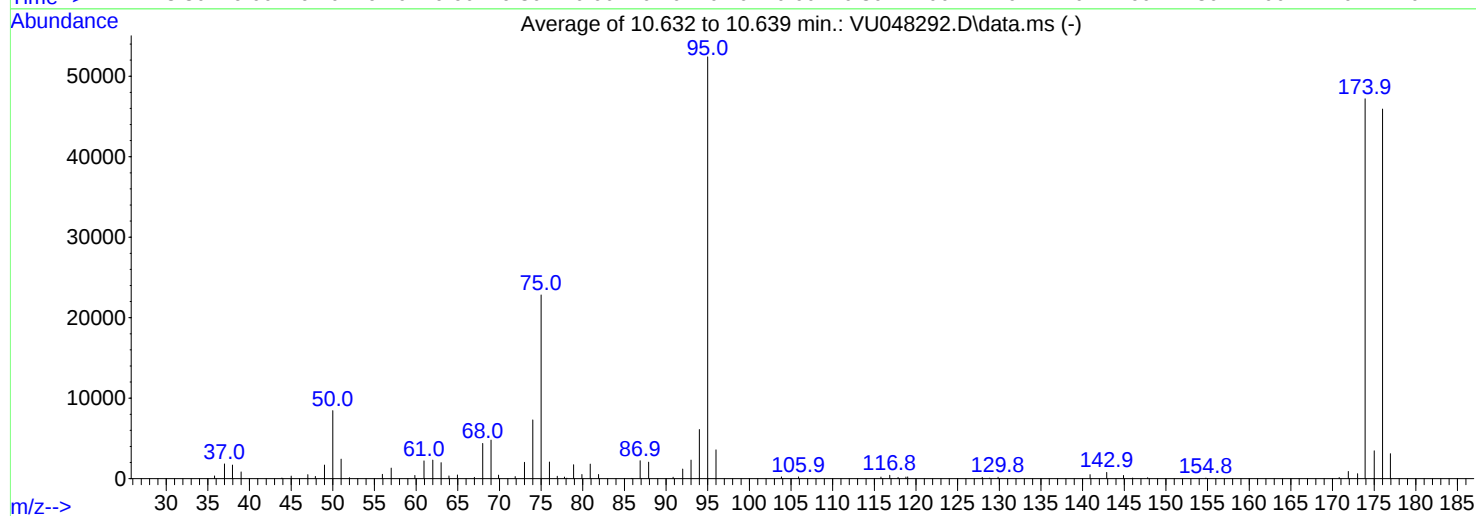


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042622\
 Data File : VU048292.D
 Acq On : 26 Apr 2022 08:59
 Operator : SY/MD
 Sample : BFB073
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB073

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 29 04:27:14 2022

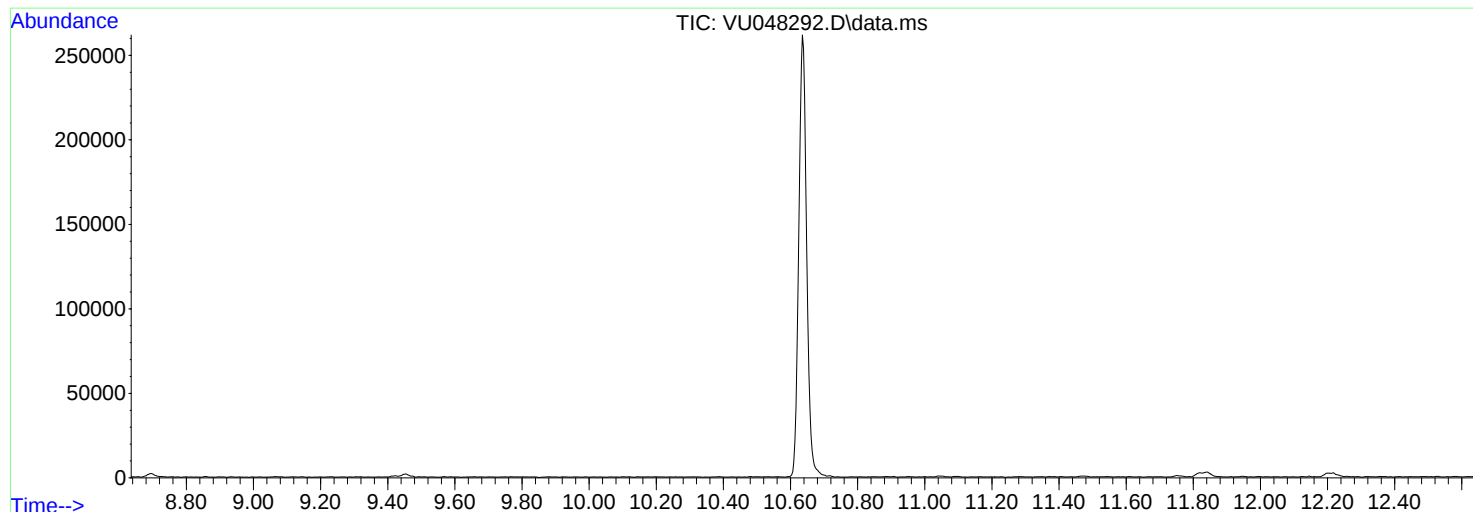

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	8455	PASS
75	95	30	80	43.6	22829	PASS
95	95	100	100	100.0	52408	PASS
96	95	5	9	6.8	3574	PASS
173	174	0.00	2	1.3	615	PASS
174	95	50	120	90.1	47205	PASS
175	174	5	9	7.3	3459	PASS
176	174	95	101	97.3	45920	PASS
177	176	5	9	6.8	3111	PASS

m/z	Abundance
39.80	228.0
43.90	536.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.80	269.0
37.00	1800.0
38.00	1654.0
39.00	859.0
39.90	211.0
43.90	613.0
45.00	323.0
47.00	465.0
47.90	277.0
49.00	1566.0
50.00	8207.0
51.00	2334.0
52.00	105.0
56.00	525.0
57.00	1274.0
59.80	480.0
60.90	2200.0
62.00	2239.0
63.00	1964.0
63.90	331.0
65.00	458.0
67.00	169.0
68.00	4391.0
69.00	4764.0
69.90	484.0
71.90	213.0
73.00	2061.0
74.00	7316.0
75.00	22264.0
76.00	2028.0
76.90	280.0
77.90	230.0
78.90	1707.0
79.90	498.0
80.90	1636.0
81.90	504.0
85.90	111.0
86.90	2183.0
87.90	1999.0
90.90	162.0
92.00	1208.0
93.00	2195.0
94.00	5815.0
95.00	50872.0
96.00	3588.0
103.80	193.0
105.90	209.0
115.80	178.0
116.80	347.0
117.80	147.0
118.80	288.0
127.90	160.0
130.00	176.0
140.90	466.0
142.90	693.0
144.90	401.0
147.80	118.0
170.70	151.0
171.90	815.0
173.00	575.0
173.90	45464.0
175.00	3244.0
176.00	43752.0
177.00	2952.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.80	361.0
37.00	1888.0
38.00	1730.0
39.00	878.0
39.90	214.0
43.90	640.0
45.00	342.0
47.00	507.0
47.90	298.0
49.00	1743.0
50.00	8747.0
51.00	2504.0
52.00	107.0
56.00	550.0
57.00	1376.0
59.90	418.0
61.00	2277.0
62.00	2353.0
63.00	2016.0
63.90	342.0
65.00	454.0
67.00	173.0
68.00	4523.0
69.00	4962.0
69.90	441.0
71.90	258.0
73.00	2128.0
74.00	7492.0
75.00	23456.0
76.00	2169.0
76.90	297.0
77.80	211.0
78.90	1786.0
79.90	555.0
80.90	1901.0
81.90	546.0
86.90	2326.0
87.90	2110.0
90.80	189.0
92.00	1191.0
93.00	2400.0
94.00	6322.0
95.00	54216.0
96.00	3741.0
103.80	217.0
105.90	219.0
115.80	223.0
116.90	433.0
117.90	163.0
118.80	310.0
119.00	315.0
128.00	172.0
128.80	116.0
129.80	181.0
140.90	505.0
142.90	786.0
144.90	413.0
146.00	130.0
147.80	141.0
154.80	111.0
170.80	158.0
171.90	937.0
173.00	645.0
173.90	48600.0
175.00	3559.0
176.00	47320.0
177.00	3214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073

m/z	Abundance
35.80	401.0
37.00	1820.0
37.90	1696.0
39.00	795.0
40.00	201.0
43.90	609.0
45.00	316.0
47.00	532.0
47.90	280.0
49.00	1764.0
50.00	8410.0
51.00	2433.0
52.00	130.0
55.90	564.0
57.00	1309.0
59.90	319.0
61.00	2157.0
62.00	2309.0
63.00	1990.0
64.00	338.0
64.90	448.0
67.00	144.0
68.00	4208.0
69.00	4668.0
69.90	382.0
71.90	303.0
73.00	1923.0
74.00	7102.0
75.00	22768.0
76.00	1990.0
77.00	317.0
77.70	176.0
78.10	173.0
78.90	1682.0
79.90	517.0
80.90	1888.0
81.90	529.0
86.90	2181.0
87.90	2043.0
90.90	198.0
92.00	1161.0
93.00	2309.0
94.00	6168.0
95.00	52136.0
96.00	3392.0
103.90	225.0
105.90	219.0
115.80	219.0
116.80	472.0
117.90	180.0
119.00	351.0
128.00	171.0
128.90	109.0
129.80	163.0
140.90	513.0
142.90	850.0
144.90	373.0
146.00	125.0
147.80	124.0
154.80	110.0
170.90	123.0
171.90	941.0
173.00	626.0
173.90	47552.0
175.00	3573.0
176.00	46688.0
176.90	3166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB073