

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
 Data File : VU053907.D
 Acq On : 26 Apr 2023 12:30
 Operator : JC/MD
 Sample : 02433-04DL 4X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE40DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	92	rVB	47498	56465	6.54%	1.090%
2	1.916	170	179	194	rBV	44228	61951	7.17%	1.196%
3	2.565	370	381	398	rVB	83891	137534	15.92%	2.656%
4	3.044	515	530	547	rVB2	23201	43789	5.07%	0.846%
5	4.639	1011	1026	1058	rBV4	51930	193807	22.44%	3.742%
6	5.057	1141	1156	1177	rVB	84143	184832	21.40%	3.569%
7	5.723	1342	1363	1388	rBV2	153343	399745	46.28%	7.719%
8	6.244	1511	1525	1552	rBV	389956	754928	87.41%	14.577%
9	6.539	1602	1617	1634	rBV2	107982	205704	23.82%	3.972%
10	6.687	1650	1663	1681	rBV2	96488	188249	21.80%	3.635%
11	7.562	1922	1935	1958	rBV	47220	85090	9.85%	1.643%
12	7.893	2019	2038	2058	rBV	194861	339241	39.28%	6.550%
13	8.176	2115	2126	2141	rBV2	28971	48843	5.66%	0.943%
14	8.465	2206	2216	2234	rBV3	7918	14720	1.70%	0.284%
15	8.629	2256	2267	2295	rBV	187006	354413	41.03%	6.843%
16	9.411	2497	2510	2536	rBV	519331	863711	100.00%	16.677%
17	10.751	2910	2927	2941	rBV	75029	118189	13.68%	2.282%
18	10.890	2958	2970	2981	rVB	11810	19128	2.21%	0.369%
19	11.806	3241	3255	3279	rBV	508549	812620	94.08%	15.691%
20	12.189	3362	3374	3396	rBV	179193	295999	34.27%	5.715%




Sum of corrected areas: 5178958

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053907.D
Acq On : 26 Apr 2023 12:30
Operator : JC/MD
Sample : 02433-04DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

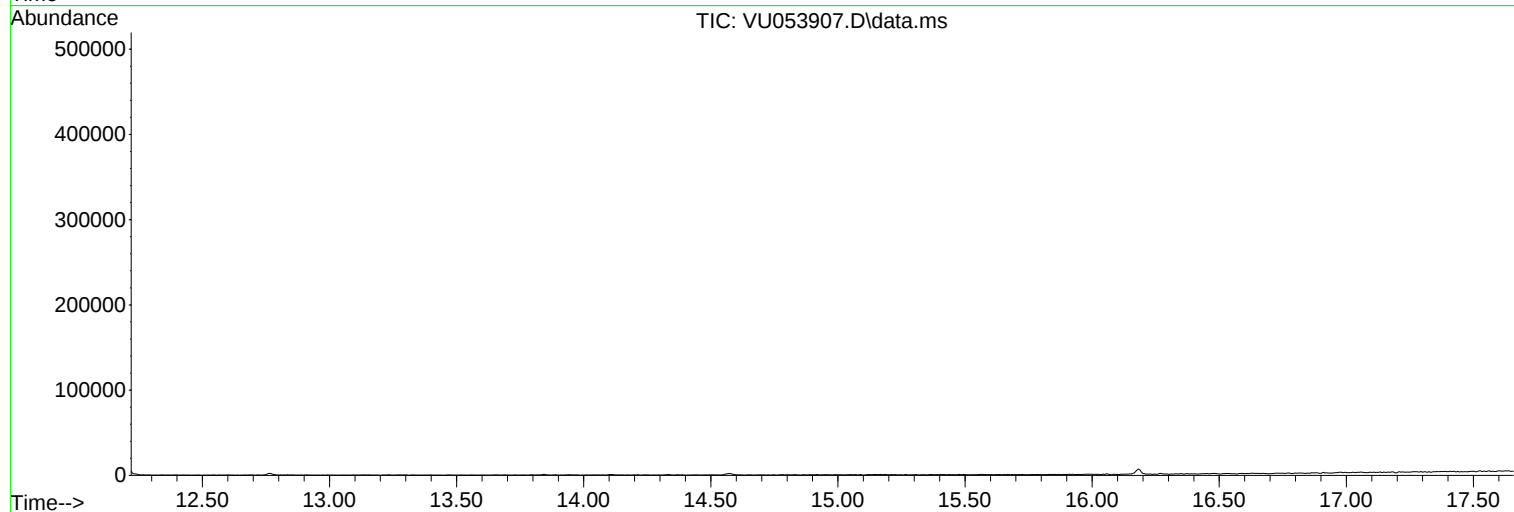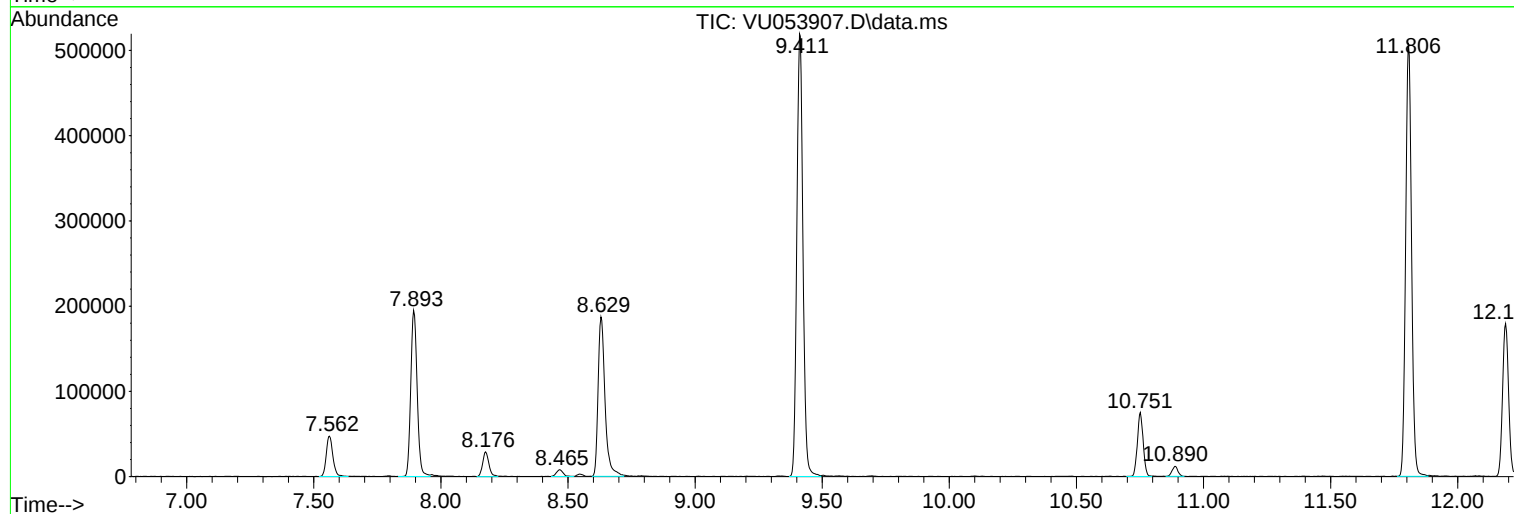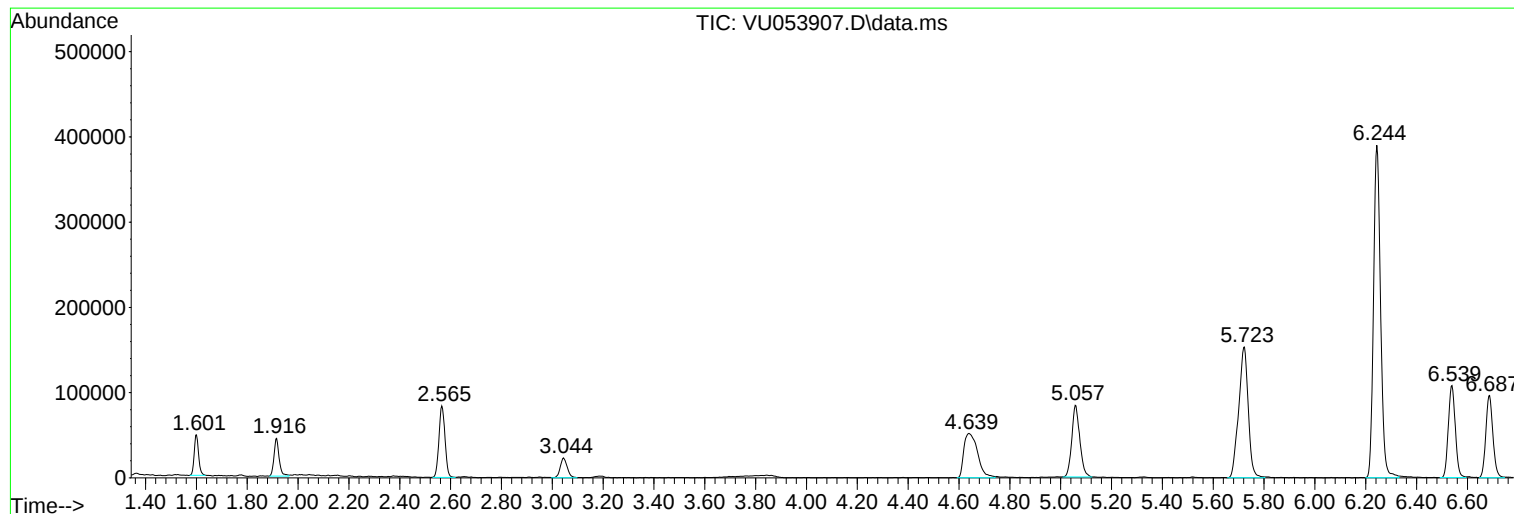

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053907.D
Acq On : 26 Apr 2023 12:30
Operator : JC/MD
Sample : 02433-04DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053907.D
Acq On : 26 Apr 2023 12:30
Operator : JC/MD
Sample : 02433-04DL 4X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------