

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
 Data File : VU053910.D
 Acq On : 26 Apr 2023 13:43
 Operator : JC/MD
 Sample : 02433-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE40

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rVB	40459	49514	3.11%	0.971%
2	1.916	171	179	190	rBV	39549	53082	3.33%	1.041%
3	2.568	370	382	399	rBV2	84658	156223	9.81%	3.064%
4	3.858	776	783	801	rVB4	7213	17248	1.08%	0.338%
5	4.655	1012	1031	1054	rBV4	56345	208556	13.10%	4.090%
6	5.060	1141	1157	1178	rBV	73131	166682	10.47%	3.269%
7	5.723	1343	1363	1382	rBV2	134593	347916	21.86%	6.823%
8	6.244	1509	1525	1546	rBV	155525	301911	18.97%	5.921%
9	6.539	1604	1617	1635	rBV2	106947	205038	12.88%	4.021%
10	6.687	1649	1663	1687	rVB2	85837	167031	10.49%	3.276%
11	7.562	1923	1935	1954	rBV2	41151	72216	4.54%	1.416%
12	7.893	2026	2038	2057	rBV	168956	294841	18.52%	5.782%
13	8.176	2114	2126	2142	rBV2	24336	39472	2.48%	0.774%
14	8.549	2229	2242	2257	rBV	935043	1591804	100.00%	31.218%
15	8.629	2257	2267	2293	rVB	164672	315363	19.81%	6.185%
16	9.414	2497	2511	2535	rBV	216072	372280	23.39%	7.301%
17	10.751	2914	2927	2939	rBV	64865	102273	6.42%	2.006%
18	10.886	2959	2969	2983	rBV3	12252	20255	1.27%	0.397%
19	11.806	3243	3255	3272	rBV	221131	360047	22.62%	7.061%
20	12.189	3358	3374	3395	rBV	156053	257289	16.16%	5.046%




Sum of corrected areas: 5099041

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053910.D
Acq On : 26 Apr 2023 13:43
Operator : JC/MD
Sample : 02433-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

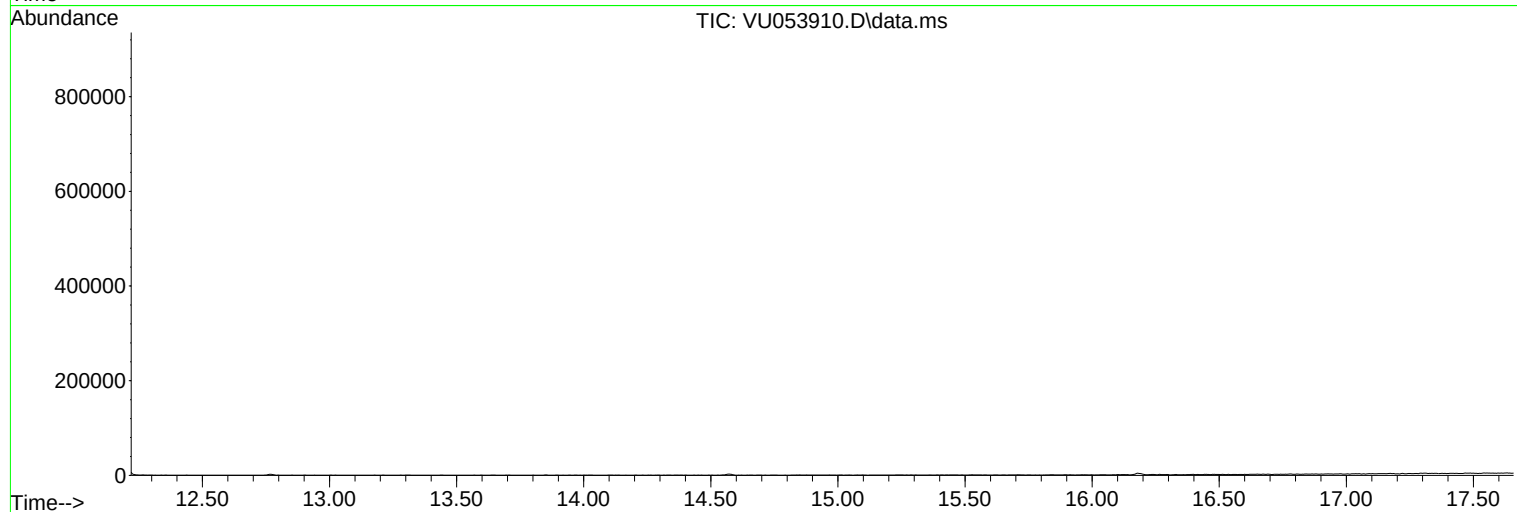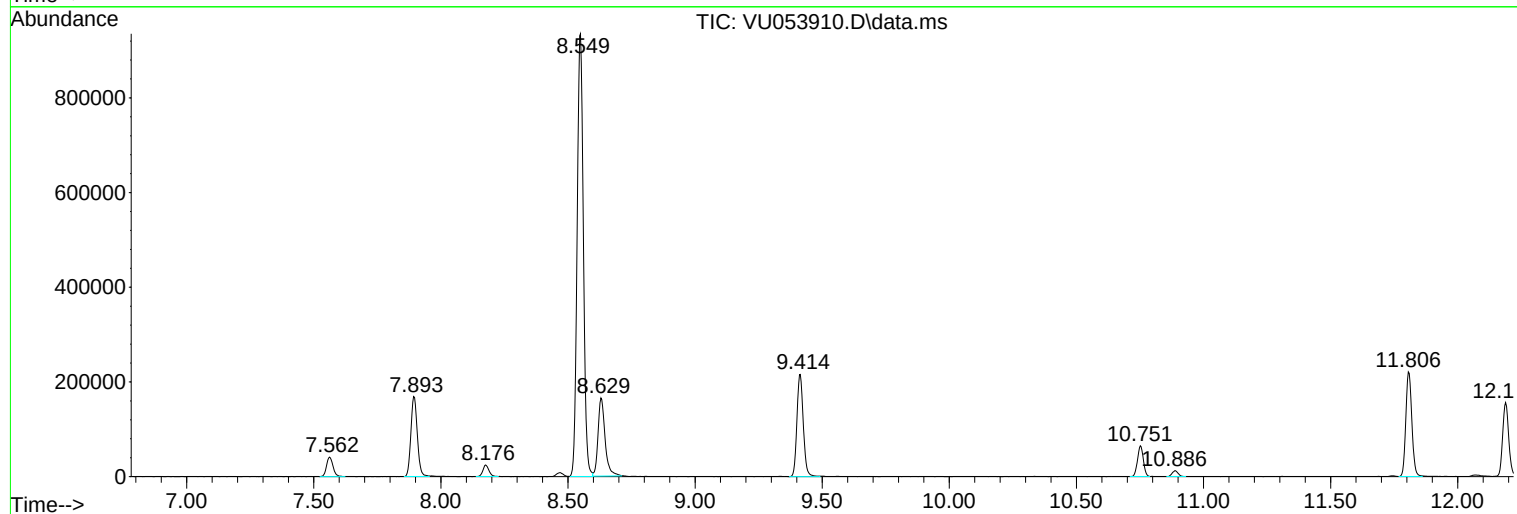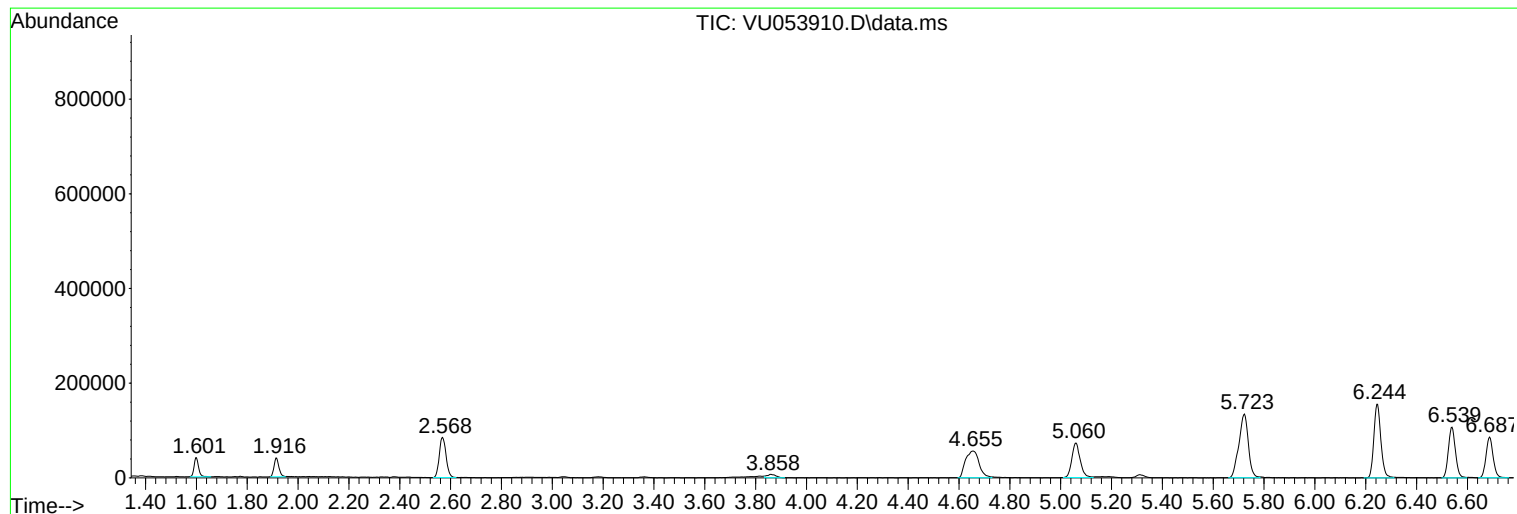

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053910.D
Acq On : 26 Apr 2023 13:43
Operator : JC/MD
Sample : 02433-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053910.D
Acq On : 26 Apr 2023 13:43
Operator : JC/MD
Sample : 02433-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc