

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
 Data File : VU053917.D
 Acq On : 26 Apr 2023 16:30
 Operator : JC/MD
 Sample : 02488-04 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE60

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053917.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	91	rBV	43663	51869	14.41%	1.678%
2	1.912	169	178	189	rBV	38089	53550	14.88%	1.733%
3	2.565	370	381	396	rBV	73593	122302	33.98%	3.957%
4	3.044	519	530	547	rVB	23598	45265	12.58%	1.465%
5	4.633	1013	1024	1058	rBV	38895	117094	32.54%	3.789%
6	5.057	1141	1156	1178	rVB2	67424	154352	42.89%	4.994%
7	5.723	1339	1363	1384	rBV3	129400	334222	92.87%	10.814%
8	6.247	1511	1526	1544	rBV	155422	300364	83.46%	9.719%
9	6.542	1609	1618	1627	rBV6	5119	9465	2.63%	0.306%
10	6.687	1650	1663	1682	rBV	81569	157986	43.90%	5.112%
11	7.562	1923	1935	1949	rBV2	39919	68766	19.11%	2.225%
12	7.893	2026	2038	2058	rBV	158820	279222	77.58%	9.035%
13	8.176	2111	2126	2143	rBV3	22172	38995	10.84%	1.262%
14	8.468	2207	2217	2229	rBV3	3309	6434	1.79%	0.208%
15	8.629	2254	2267	2302	rBV	152243	291948	81.12%	9.446%
16	9.414	2499	2511	2534	rBV	214830	359893	100.00%	11.645%
17	10.751	2916	2927	2943	rVB2	58988	95706	26.59%	3.097%
18	10.890	2961	2970	2977	rBV2	4975	7781	2.16%	0.252%
19	11.809	3244	3256	3282	rBV	218963	351914	97.78%	11.387%
20	12.189	3360	3374	3389	rBV	143275	238512	66.27%	7.717%
21	16.179	4608	4615	4622	rBV4	3507	4919	1.37%	0.159%




Sum of corrected areas: 3090559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053917.D
Acq On : 26 Apr 2023 16:30
Operator : JC/MD
Sample : 02488-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

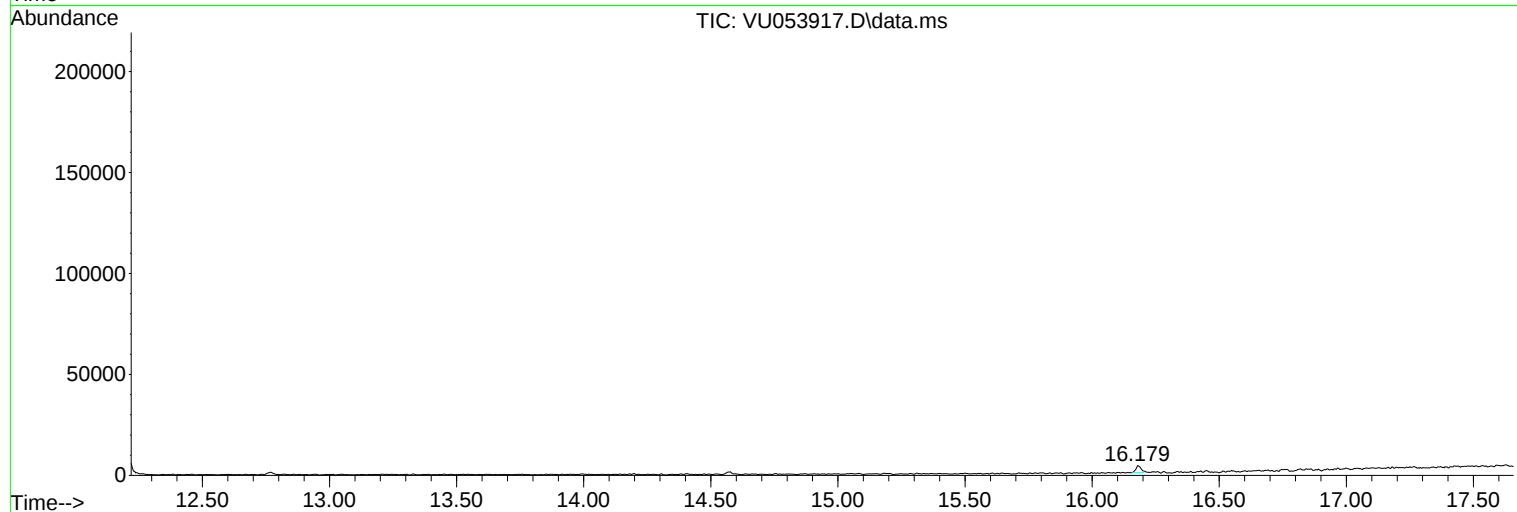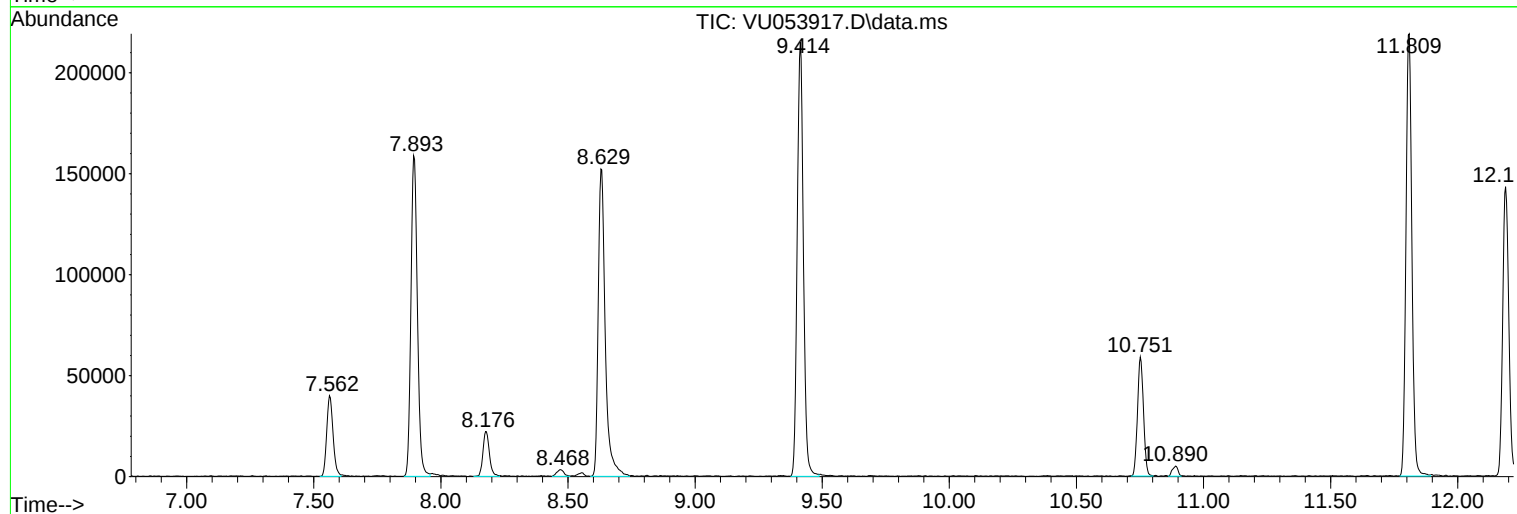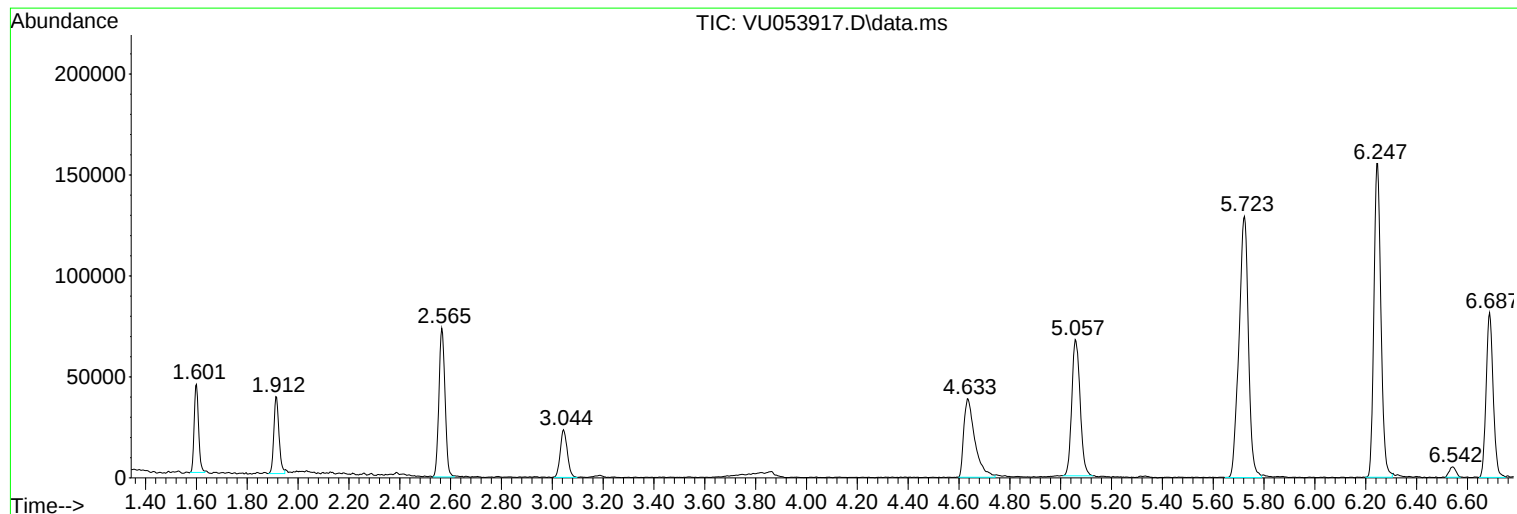

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053917.D
Acq On : 26 Apr 2023 16:30
Operator : JC/MD
Sample : 02488-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053917.D
Acq On : 26 Apr 2023 16:30
Operator : JC/MD
Sample : 02488-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE60

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------