

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
 Data File : VU053923.D
 Acq On : 26 Apr 2023 18:55
 Operator : JC/MD
 Sample : 02488-13 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE68

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053923.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	91	rBV	40457	47314	13.68%	1.527%
2	1.916	170	179	195	rBV	37016	53354	15.42%	1.722%
3	2.565	370	381	399	rVB	72488	116516	33.68%	3.761%
4	3.044	521	530	544	rVB2	7916	14427	4.17%	0.466%
5	4.633	1012	1024	1061	rBV	42490	126129	36.46%	4.071%
6	5.060	1136	1157	1175	rVB2	73386	163760	47.34%	5.286%
7	5.723	1341	1363	1380	rBV2	135656	345956	100.00%	11.166%
8	6.247	1511	1526	1544	rBV	149224	284128	82.13%	9.171%
9	6.687	1650	1663	1682	rBV2	85229	165182	47.75%	5.331%
10	7.562	1924	1935	1957	rVB3	40727	70998	20.52%	2.292%
11	7.893	2024	2038	2056	rBV	165917	288395	83.36%	9.308%
12	8.176	2116	2126	2142	rBV	24850	41127	11.89%	1.327%
13	8.472	2205	2218	2228	rBV3	6864	12180	3.52%	0.393%
14	8.629	2256	2267	2302	rBV	164313	313686	90.67%	10.125%
15	9.414	2498	2511	2539	rBV	206739	344974	99.72%	11.135%
16	10.751	2913	2927	2945	rBV2	64808	106468	30.78%	3.436%
17	10.889	2960	2970	2980	rVB2	7402	11734	3.39%	0.379%
18	11.809	3244	3256	3277	rBV	206160	333027	96.26%	10.749%
19	12.188	3360	3374	3392	rBV	153865	253457	73.26%	8.181%
20	16.185	4605	4617	4627	rBV	2727	5431	1.57%	0.175%




Sum of corrected areas: 3098243

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053923.D
Acq On : 26 Apr 2023 18:55
Operator : JC/MD
Sample : 02488-13 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

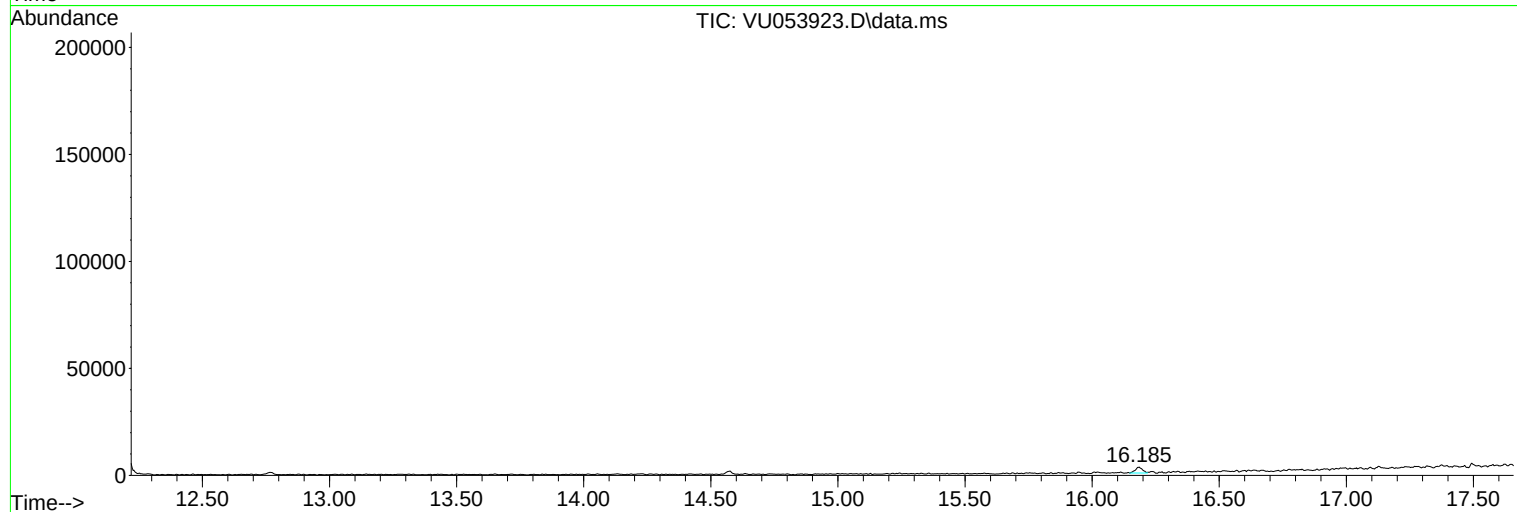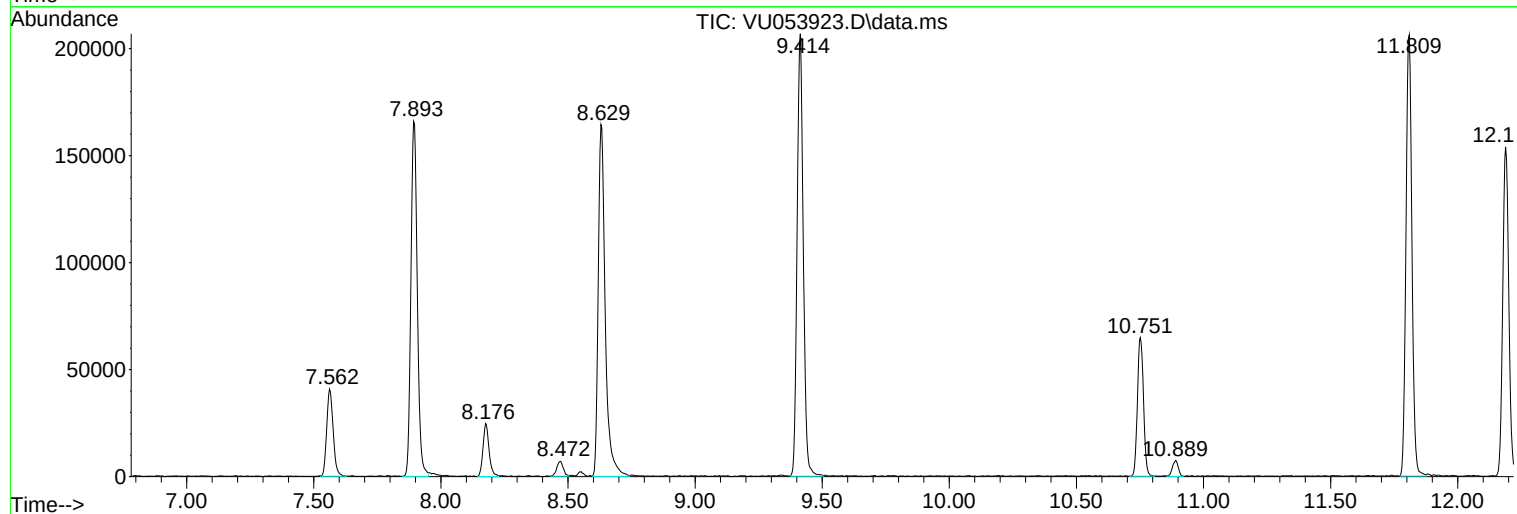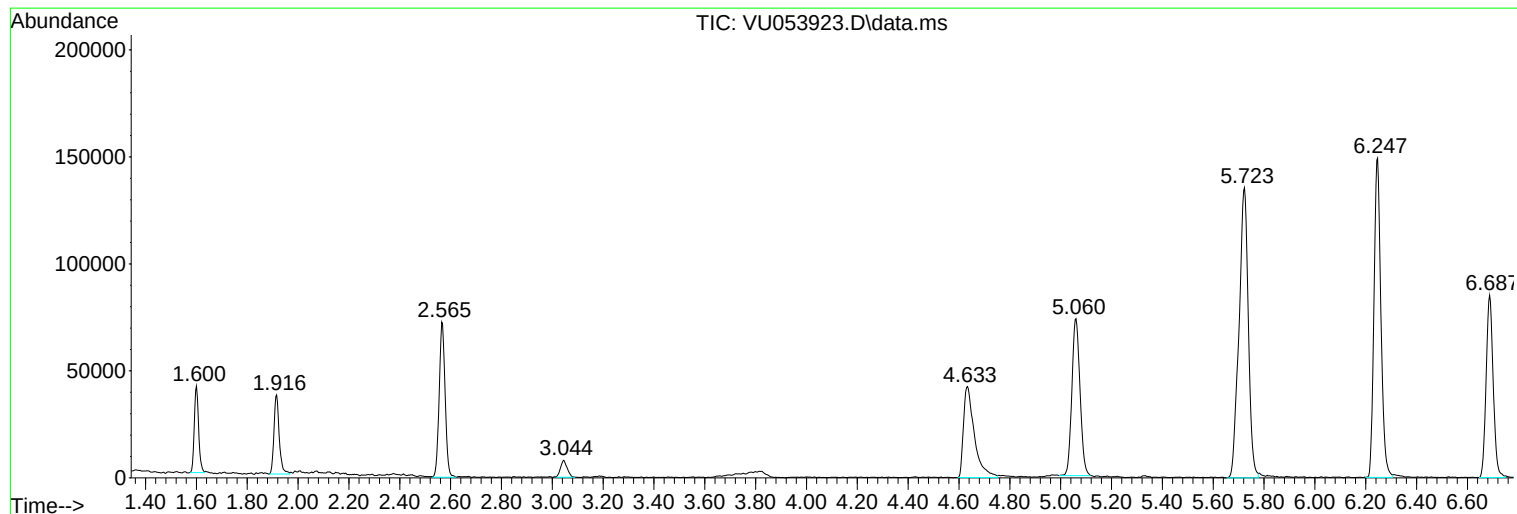

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053923.D
Acq On : 26 Apr 2023 18:55
Operator : JC/MD
Sample : 02488-13 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053923.D
Acq On : 26 Apr 2023 18:55
Operator : JC/MD
Sample : 02488-13 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc