
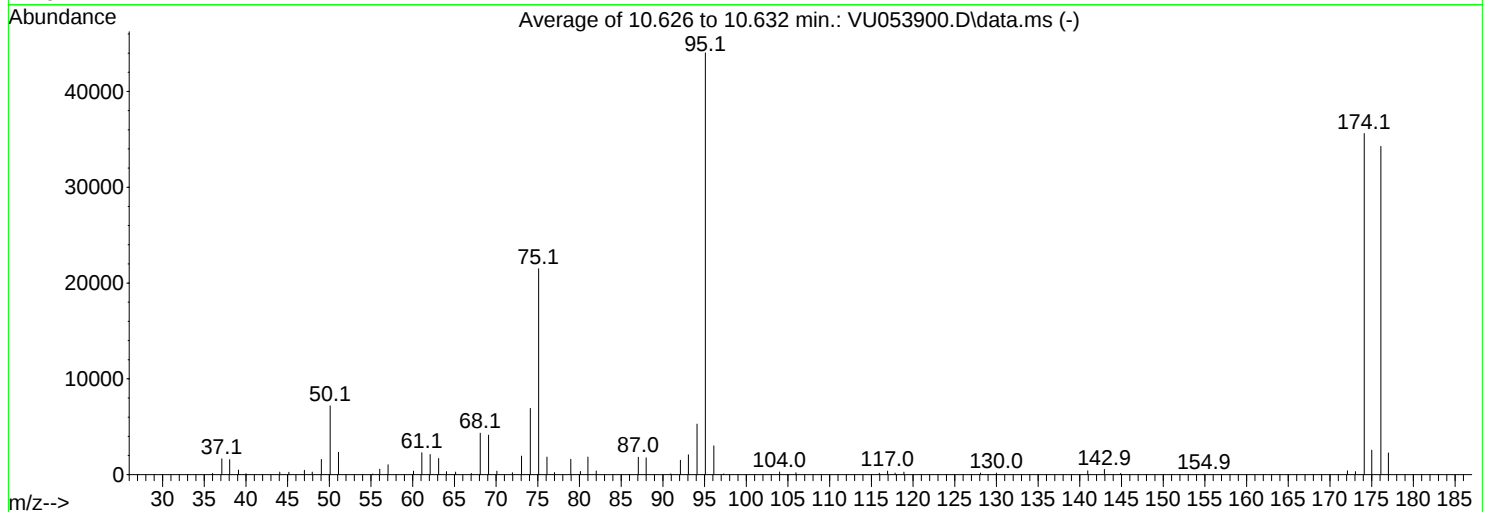


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042623\
Data File : VU053900.D
Acq On : 26 Apr 2023 09:08
Operator : JC/MD
Sample : BFB009
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB009

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 27 05:52:18 2023

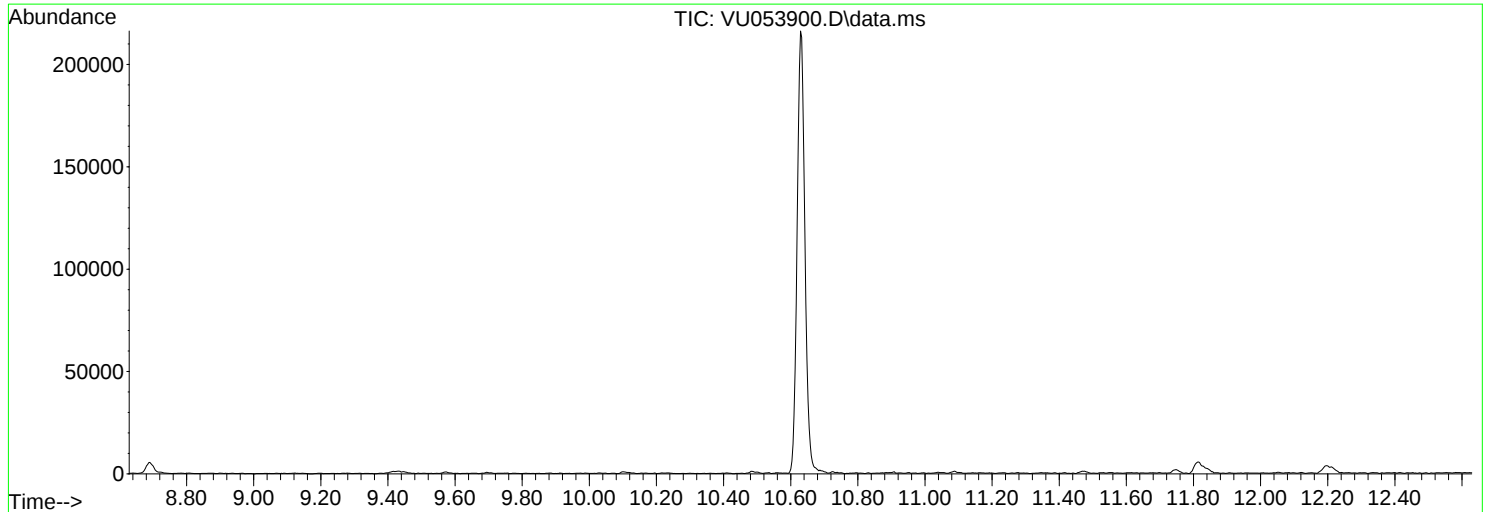

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	7188	PASS
75	95	30	80	48.8	21501	PASS
95	95	100	100	100.0	44029	PASS
96	95	5	9	6.8	3005	PASS
173	174	0.00	2	0.9	318	PASS
174	95	50	120	80.9	35613	PASS
175	174	5	9	7.2	2551	PASS
176	174	95	101	96.2	34277	PASS
177	176	5	9	6.7	2281	PASS

m/z	Abundance
36.00	211.0
44.10	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
36.00	315.0
37.10	1603.0
38.00	1444.0
39.10	425.0
44.00	395.0
45.10	278.0
47.00	496.0
47.90	273.0
49.10	1656.0
50.10	6852.0
51.10	2334.0
56.00	545.0
57.10	896.0
60.10	401.0
61.10	2232.0
62.10	2075.0
63.10	1640.0
64.00	317.0
65.20	287.0
67.10	115.0
68.10	4267.0
69.10	4248.0
70.10	329.0
71.90	222.0
73.00	1733.0
74.10	6654.0
75.10	20056.0
76.10	1863.0
77.00	180.0
78.90	1502.0
80.10	334.0
81.00	1881.0
82.00	429.0
87.00	1738.0
88.00	1502.0
91.00	144.0
92.10	1467.0
93.00	1968.0
94.10	4961.0
95.10	41936.0
96.10	2840.0
104.00	317.0
105.90	180.0
115.90	157.0
117.00	399.0
117.80	173.0
118.90	281.0
128.10	157.0
130.00	128.0
140.90	391.0
143.00	538.0
144.90	115.0
154.90	136.0
172.10	310.0
173.00	263.0
174.10	33032.0
175.00	2550.0
176.10	31552.0
177.00	2251.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
36.10	341.0
37.10	1702.0
38.10	1669.0
39.10	497.0
40.00	155.0
44.10	465.0
45.20	244.0
47.00	474.0
48.00	287.0
49.10	1638.0
50.10	7413.0
51.10	2379.0
55.20	107.0
56.00	589.0
57.00	1087.0
60.10	374.0
61.10	2435.0
62.10	2195.0
63.10	1759.0
64.00	314.0
65.10	274.0
67.10	113.0
68.10	4490.0
69.10	4277.0
70.10	392.0
72.00	211.0
73.10	1942.0
74.10	7060.0
75.10	22280.0
76.10	1945.0
77.00	214.0
79.00	1662.0
80.10	345.0
81.00	1886.0
82.00	388.0
87.10	1930.0
88.00	1793.0
90.90	120.0
92.10	1529.0
93.00	2183.0
94.10	5492.0
95.10	45560.0
96.10	3122.0
97.30	128.0
104.00	310.0
106.00	202.0
116.00	149.0
117.00	394.0
117.80	183.0
118.90	268.0
128.10	162.0
130.00	171.0
141.00	408.0
142.90	571.0
144.90	132.0
172.10	418.0
173.00	337.0
174.10	36784.0
175.00	2565.0
176.10	35456.0
177.00	2345.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009

m/z	Abundance
36.10	356.0
37.10	1632.0
38.10	1604.0
39.10	536.0
40.00	170.0
44.10	486.0
45.20	242.0
47.00	401.0
47.90	264.0
49.00	1485.0
50.10	7298.0
51.10	2298.0
55.20	112.0
56.10	578.0
57.10	1119.0
60.10	334.0
61.10	2188.0
62.10	2043.0
63.10	1652.0
64.10	306.0
65.10	264.0
67.00	108.0
68.10	4228.0
69.10	3852.0
70.10	370.0
72.00	171.0
73.10	2142.0
74.10	7035.0
75.10	22168.0
76.10	1703.0
77.00	264.0
79.00	1626.0
80.10	327.0
81.00	1762.0
82.00	322.0
87.10	1800.0
88.00	1989.0
92.10	1502.0
93.10	2082.0
94.10	5392.0
95.10	44592.0
96.10	3052.0
97.30	140.0
104.00	252.0
106.00	212.0
116.00	126.0
116.90	291.0
117.90	164.0
118.90	248.0
128.10	160.0
130.00	200.0
141.00	404.0
142.90	538.0
144.90	145.0
172.10	475.0
173.10	355.0
174.10	37024.0
175.00	2539.0
176.10	35824.0
177.00	2246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB009