




Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Manual Integrations
APPROVED

MMDadoda
4/29/2019 10:53:24 AM

Quant Time: Apr 27 00:25:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 00:11:31 2019
Response via : Initial Calibration

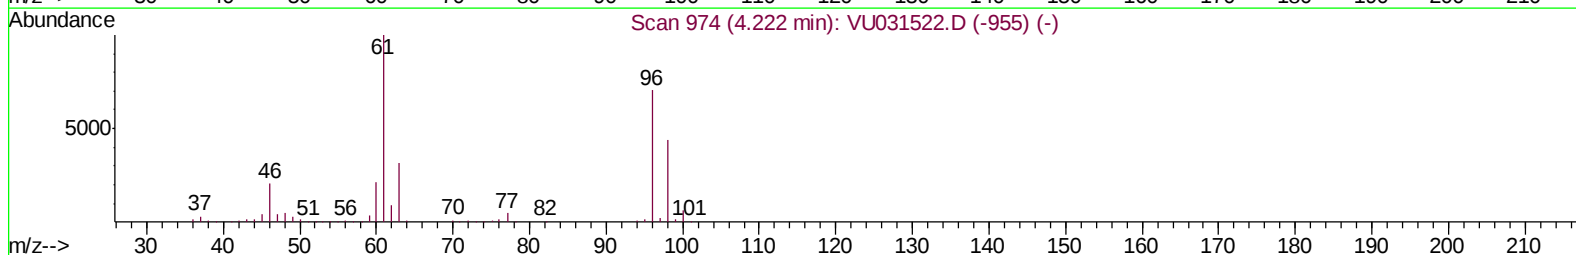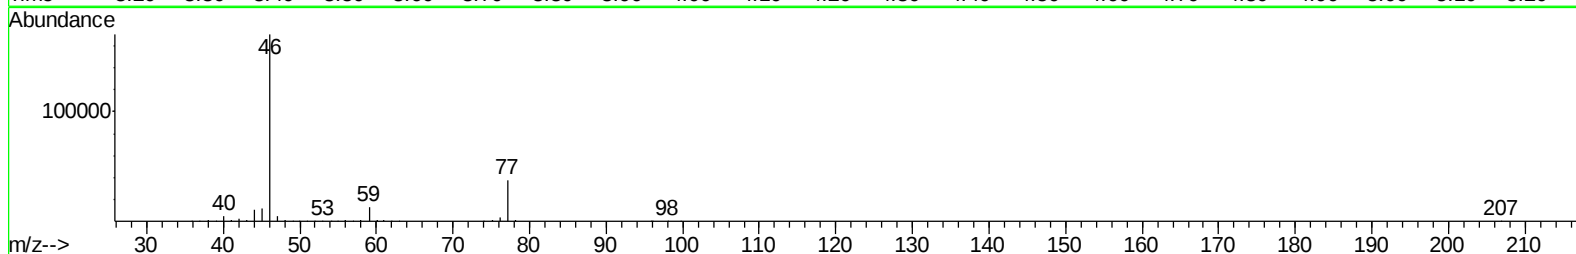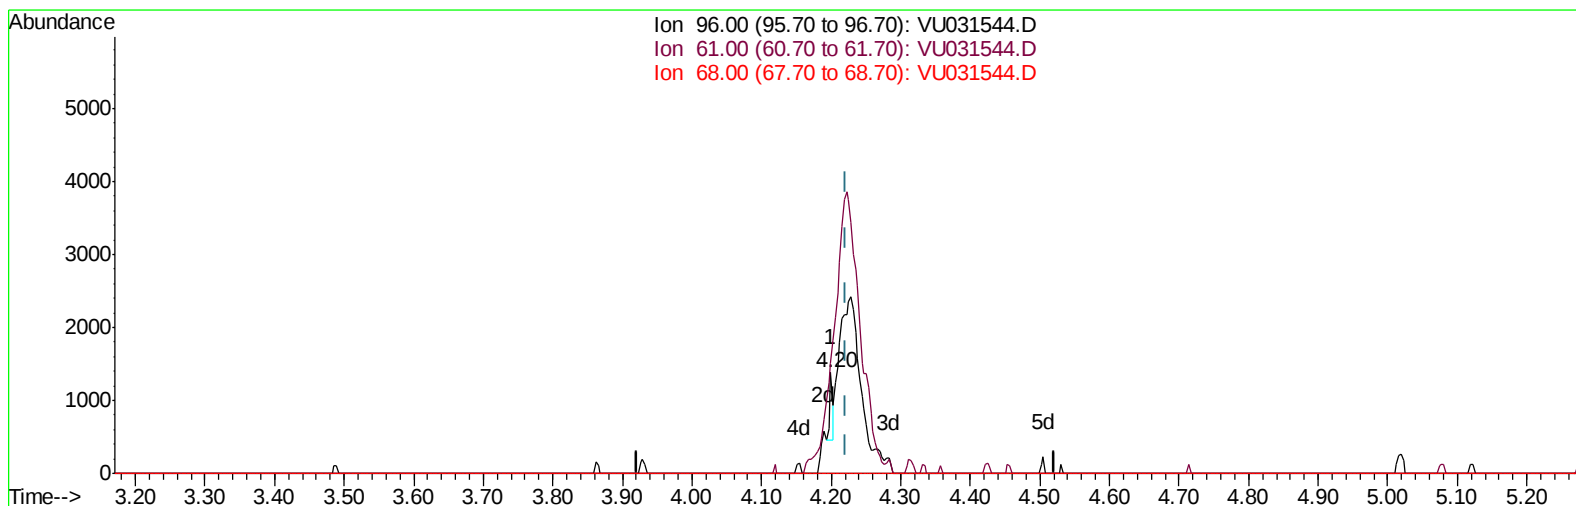

TIC: VU031544.D

(20) cis-1,2-Dichloroethene (T)

4.199min (-0.022) 0.04ug/L

response 297

Ion	Exp%	Act%
96.00	100	100
61.00	142.10	108.68
68.00	0.00	0.00
0.00	0.00	0.00




Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Manual Integrations
APPROVED

MMDadoda
4/29/2019 10:53:24 AM

Quant Time: Apr 27 00:25:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 00:11:31 2019
Response via : Initial Calibration

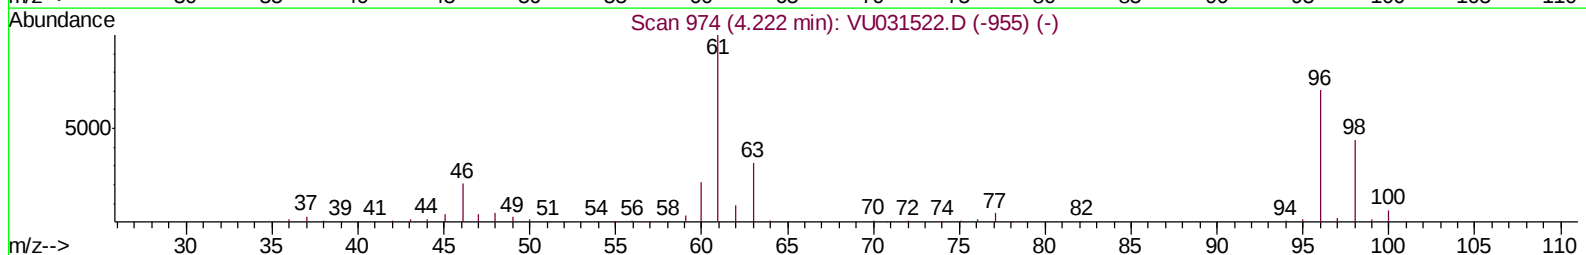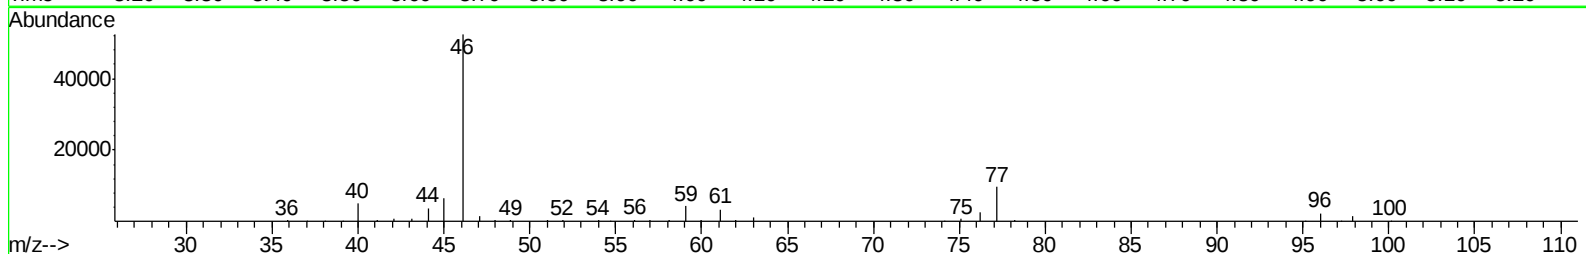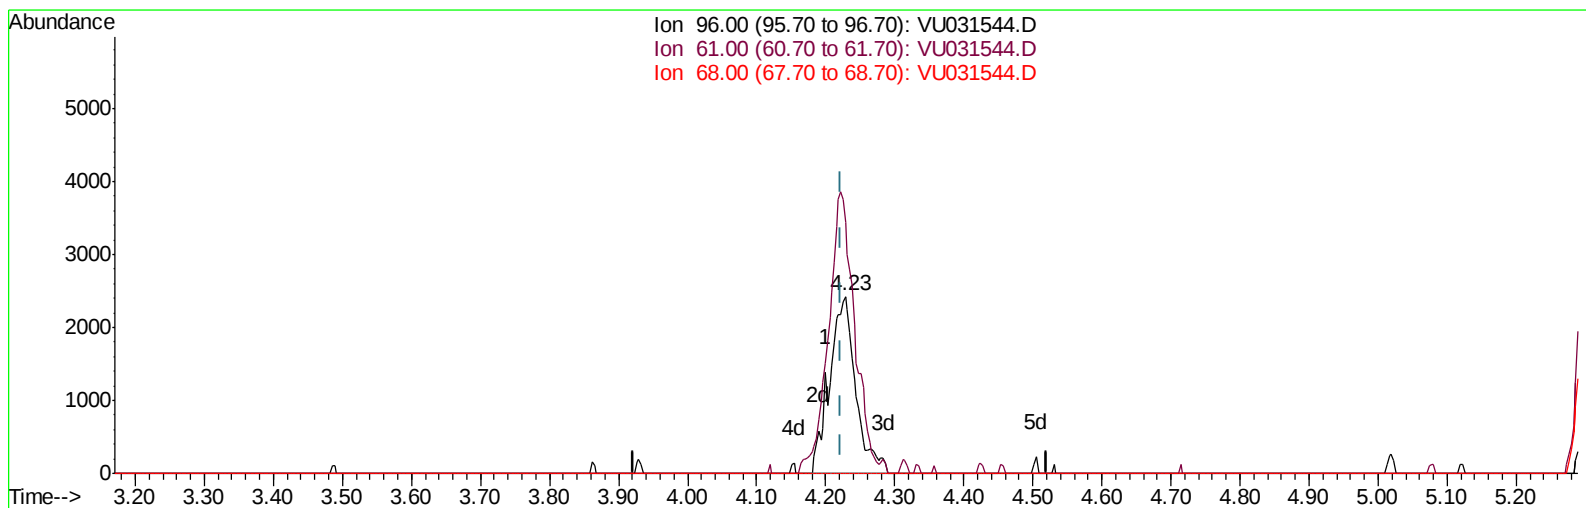

TIC: VU031544.D

(20) cis-1,2-Dichloroethene (T)

4.228min (+0.007) 0.81ug/L m

response 6363

Ion	Exp%	Act%
96.00	100	100
61.00	142.10	141.74
68.00	0.00	0.00
0.00	0.00	0.00

Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Manual Integrations
APPROVED

MMDadoda
4/29/2019 10:53:24 AM

Quant Time: Apr 27 03:27:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 00:11:31 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	895894	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	837336	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	338429	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	385995	51.48	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	102.96%
7) Chloroethane-d5	1.68	69	297347	51.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	102.64%
11) 1,1-Dichloroethene-d2	2.27	63	546931	36.63	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	73.26%
21) 2-Butanone-d5	4.18	46	677507	99.73	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.73%
24) Chloroform-d	4.64	84	629102	45.81	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.62%
26) 1,2-Dichloroethane-d4	5.31	65	408705	45.56	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.12%
32) Benzene-d6	5.33	84	1326261	51.58	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.16%
36) 1,2-Dichloropropane-d6	6.32	67	447241	49.44	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.88%
41) Toluene-d8	7.56	98	1124714	50.22	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.44%
43) trans-1,3-Dichloropropene-	7.85	79	186421	48.01	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.02%
47) 2-Hexanone-d5	8.31	63	449630	114.83	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	114.83%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	575910	47.44	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.88%
64) 1,2-Dichlorobenzene-d4	11.86	152	365039	51.29	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.58%

Target Compounds					Qvalue
20) cis-1,2-Dichloroethene	4.23	96	6363m	0.814 ug/L	
34) Trichloroethene	6.18	95	271320	36.358 ug/L	97
46) Tetrachloroethene	8.22	164	6946	1.365 ug/L	84

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Manual Integrations
APPROVED

MMDadoda
4/29/2019 10:53:24 AM

Quant Time: Apr 27 03:27:04 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 00:11:31 2019
Response via : Initial Calibration

