

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031557.D
 Acq On : 27 Apr 2019 01:49
 Operator : JC/SP
 Sample : K2592-10 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X03

Quant Time: Apr 27 04:23:32 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 27 03:26:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	850496	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	793774	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	311618	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	376258	52.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.72%
7) Chloroethane-d5	1.68	69	285799	51.96	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.92%
11) 1,1-Dichloroethene-d2	2.27	63	540521	38.13	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.26%
21) 2-Butanone-d5	4.19	46	692952	107.45	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.45%
24) Chloroform-d	4.64	84	620375	47.59	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.18%
26) 1,2-Dichloroethane-d4	5.31	65	415357	48.77	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.54%
32) Benzene-d6	5.34	84	1265003	51.90	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.80%
36) 1,2-Dichloropropane-d6	6.32	67	447245	52.15	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.30%
41) Toluene-d8	7.56	98	1080800	50.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.82%
43) trans-1,3-Dichloropropene-	7.85	79	172994	46.99	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.98%
47) 2-Hexanone-d5	8.31	63	433312	116.74	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.74%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	565852	49.17	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.34%
64) 1,2-Dichlorobenzene-d4	11.86	152	350011	53.41	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	106.82%


Target Compounds					Ovalue
9) Trichlorofluoromethane	1.88	101	45368	3.762 ug/L	98
34) Trichloroethene	6.18	95	1873418	264.821 ug/L	98
46) Tetrachloroethene	8.23	164	45143	9.360 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031557.D
Acq On : 27 Apr 2019 01:49
Operator : JC/SP
Sample : K2592-10 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X03

Quant Time: Apr 27 04:23:32 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 03:26:56 2019
Response via : Initial Calibration

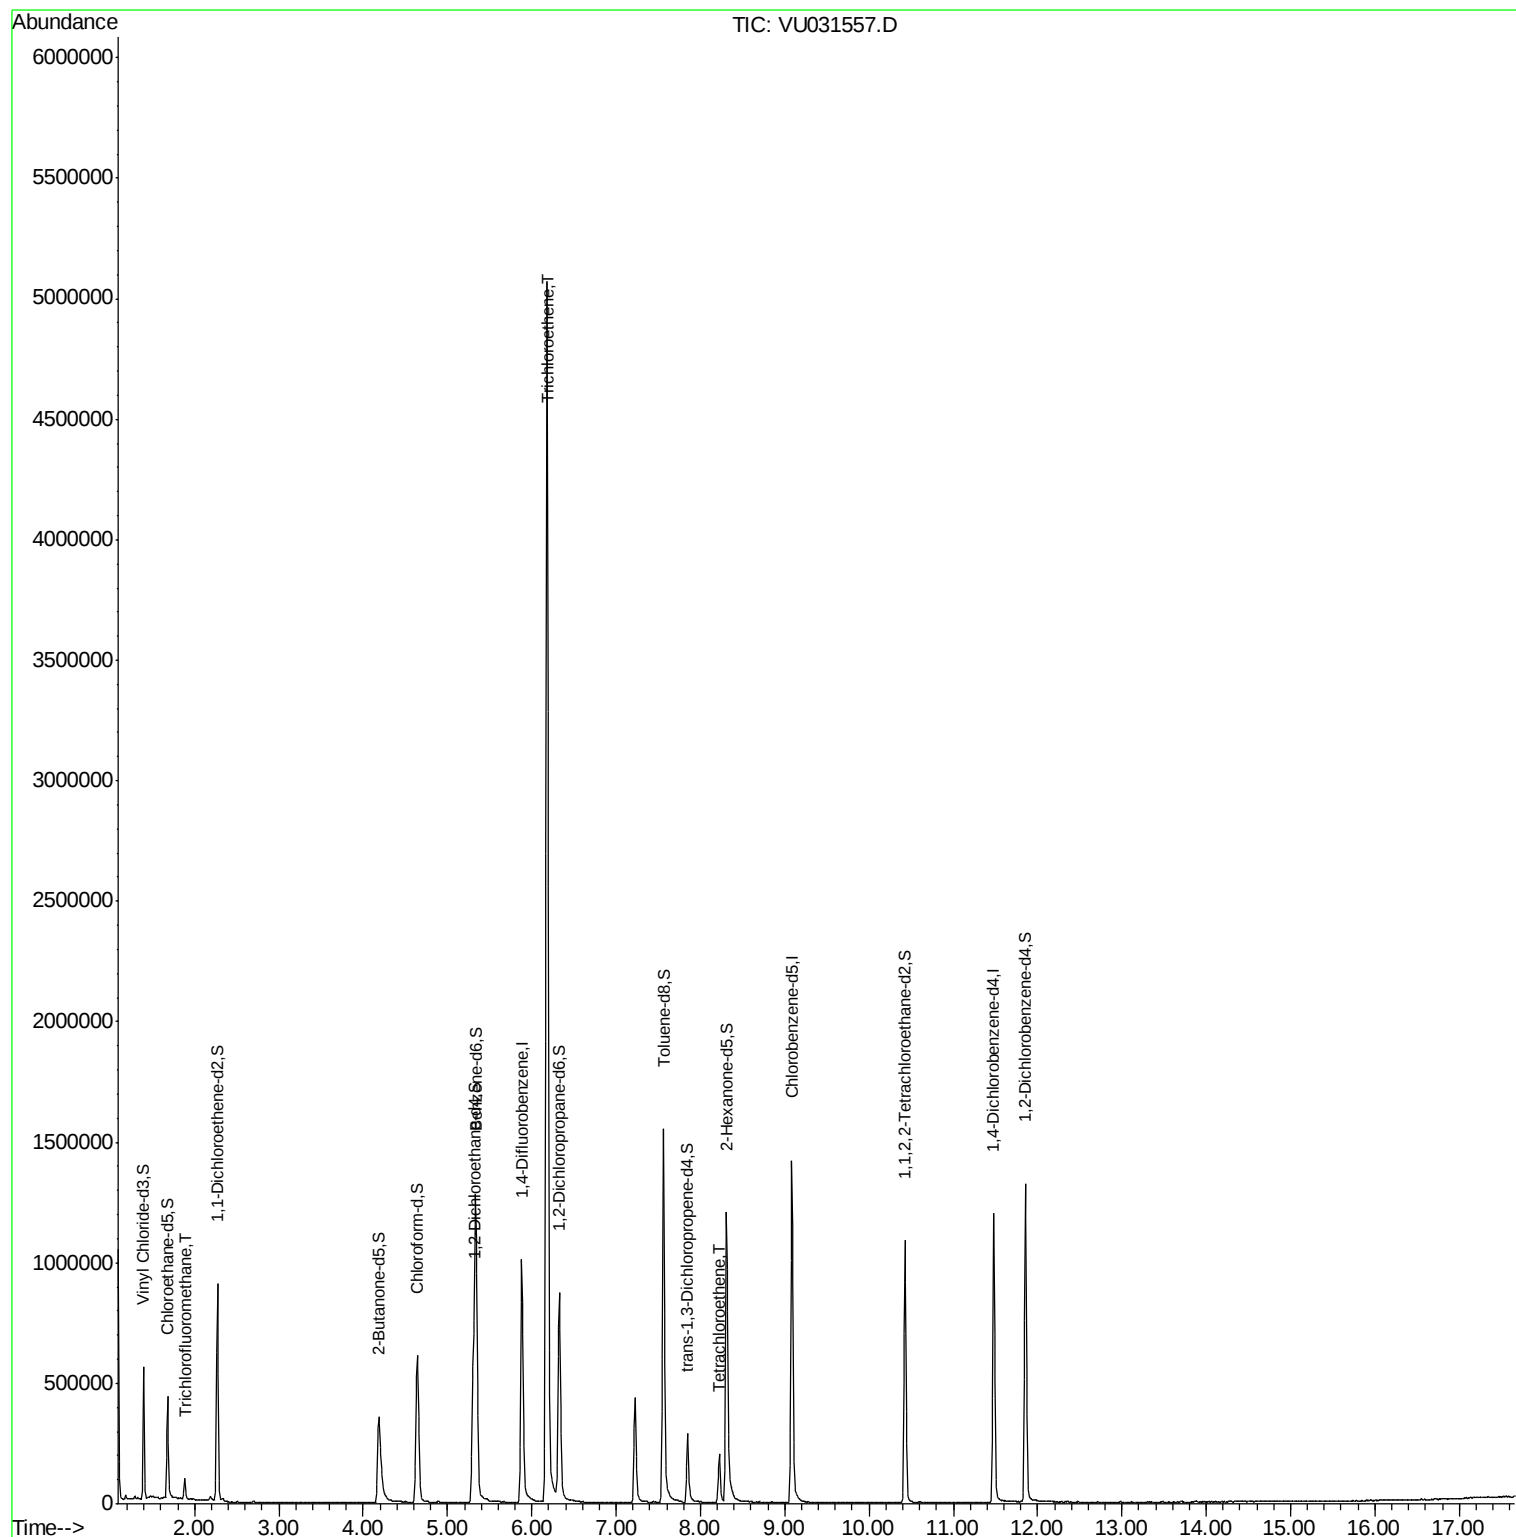




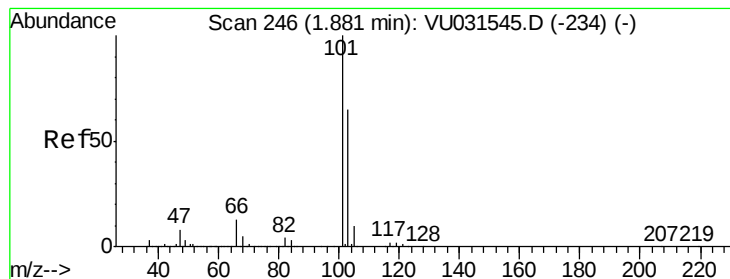


#9

Trichlorofluoromethane
 Concen: 3.762 ug/L
 RT: 1.88 min Scan# 246
 Delta R.T. 0.00 min
 Lab File: VU031557.D
 Acq: 27 Apr 2019 01:49

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X03




Tot Ion:101 Resp: 45368
 Ion Ratio Lower Upper
 101 100
 103 62.0 50.8 76.2

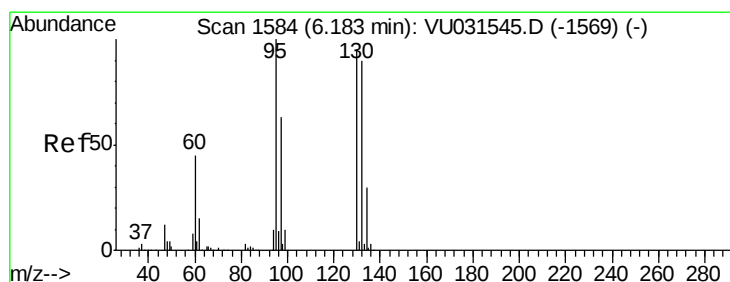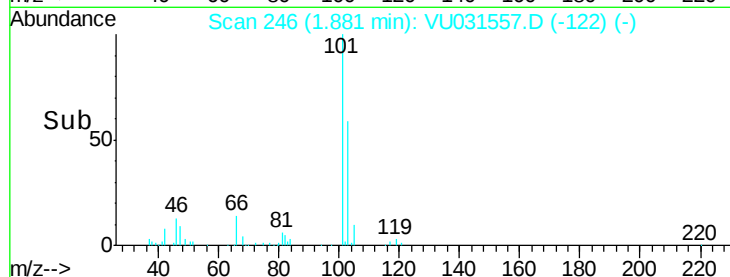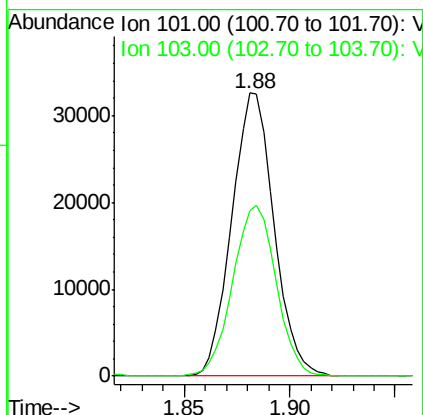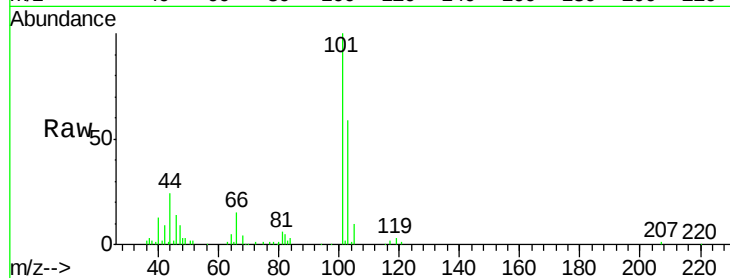


#34

Trichloroethene
 Concen: 264.821 ug/L
 RT: 6.18 min Scan# 1583
 Delta R.T. -0.00 min
 Lab File: VU031557.D
 Acq: 27 Apr 2019 01:49

Tgt Ion: 95 Resp: 1873418
 Ion Ratio Lower Upper
 95 100
 97 65.0 44.8 83.2
 132 88.6 63.1 117.1
 130 92.0 66.5 123.5

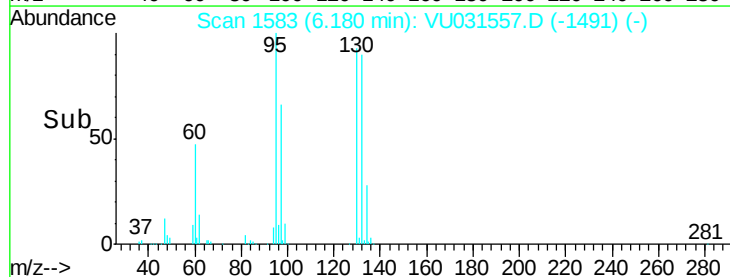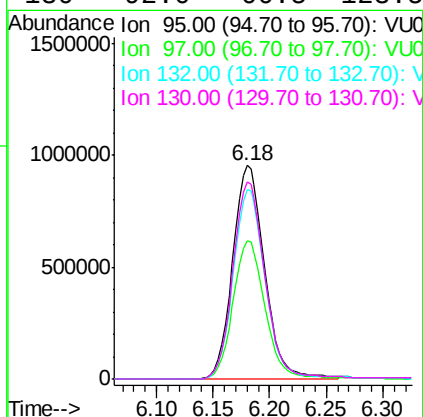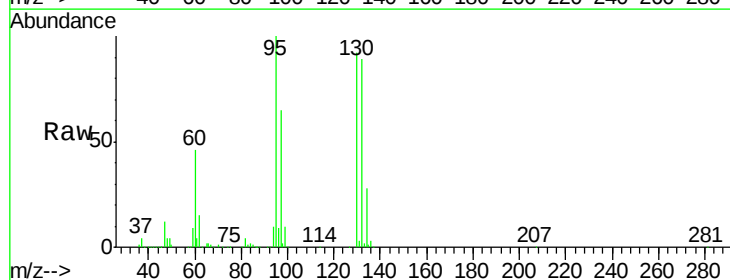

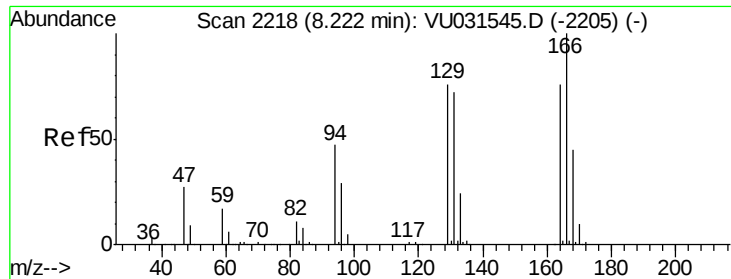

#46

Tetrachloroethene

Concen: 9.360 ug/L

RT: 8.23 min Scan# 2220

Delta R.T. 0.01 min

Lab File: VU031557.D

Acq: 27 Apr 2019 01:49

Instrument :

MSVOA_U

ClientSampleId :

C0X03

Tot Ion:164 Resp: 45143


Ion Ratio Lower Upper

164 100

129 100.3 71.5 132.9

131 98.6 69.0 128.2

166 134.1 93.7 173.9

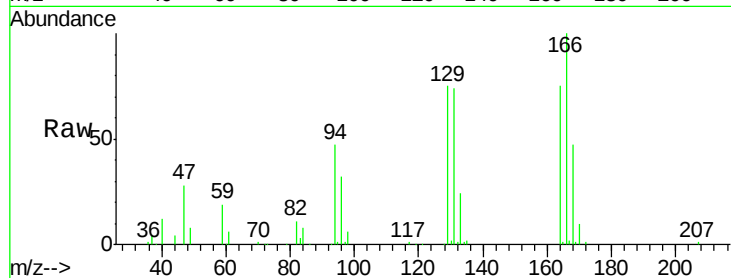

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

