

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031563.D
 Acq On : 27 Apr 2019 04:09
 Operator : JC/SP
 Sample : K2592-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X82

Quant Time: Apr 27 04:40:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 27 03:26:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	856377	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	783776	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	304457	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	361409	50.43	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.86%
7) Chloroethane-d5	1.68	69	287623	51.93	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.86%
11) 1,1-Dichloroethene-d2	2.27	63	535735	37.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.06%
21) 2-Butanone-d5	4.19	46	698570	107.57	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	107.57%
24) Chloroform-d	4.64	84	621041	47.31	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.62%
26) 1,2-Dichloroethane-d4	5.31	65	424922	49.55	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.10%
32) Benzene-d6	5.34	84	1281135	53.23	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	106.46%
36) 1,2-Dichloropropane-d6	6.32	67	443510	52.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	104.76%
41) Toluene-d8	7.56	98	1057090	50.43	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.86%
43) trans-1,3-Dichloropropene-	7.85	79	174796	48.09	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	96.18%
47) 2-Hexanone-d5	8.31	63	425448	116.08	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	116.08%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	560881	49.36	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.72%
64) 1,2-Dichlorobenzene-d4	11.86	152	339142	52.97	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	105.94%

Target Compounds


					Ovalue
13) Acetone	2.34	43	10089	1.379 ug/L	62
34) Trichloroethene	6.19	95	22739	3.255 ug/L	93
46) Tetrachloroethene	8.22	164	6074	1.276 ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031563.D
Acq On : 27 Apr 2019 04:09
Operator : JC/SP
Sample : K2592-16 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X82

Quant Time: Apr 27 04:40:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 27 03:26:56 2019
Response via : Initial Calibration

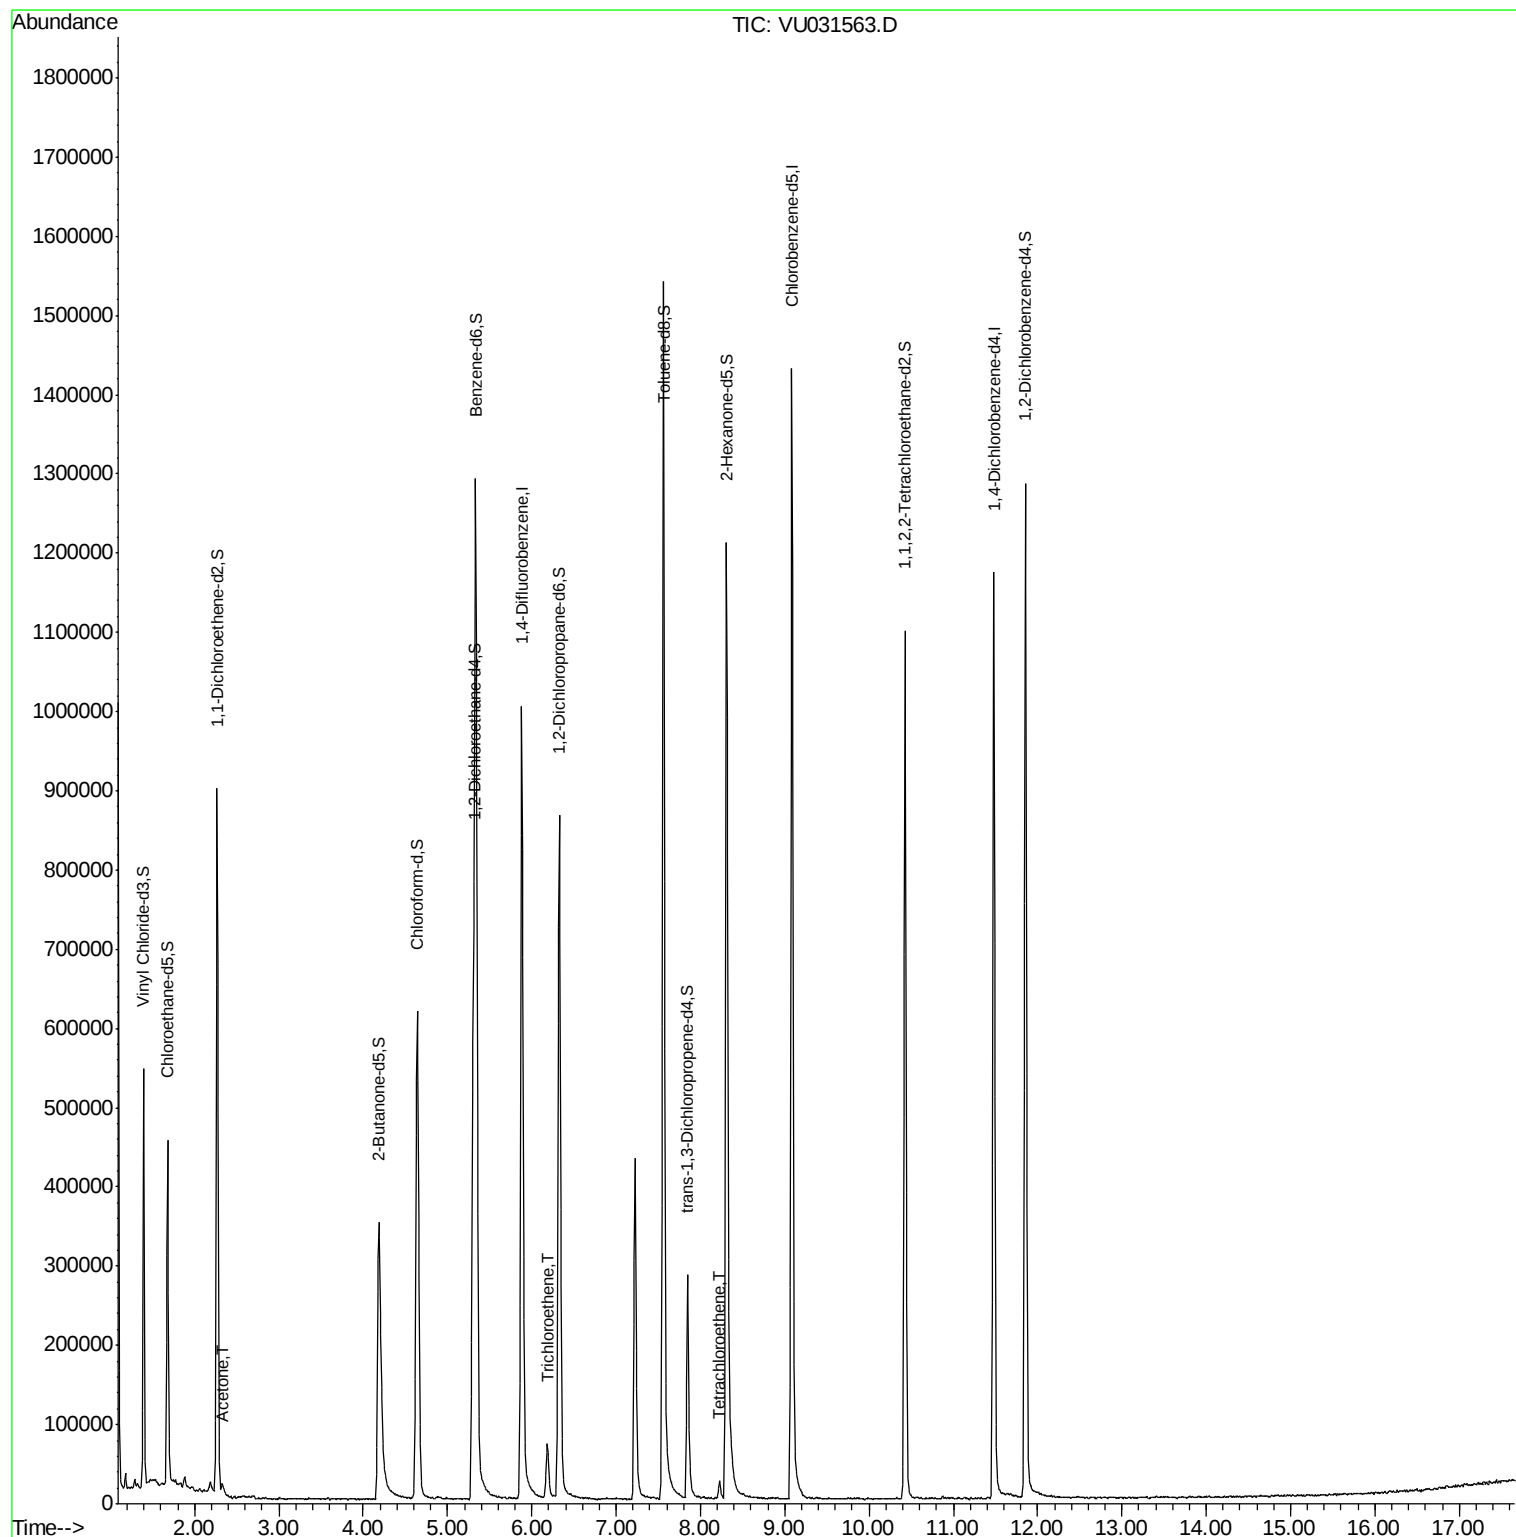

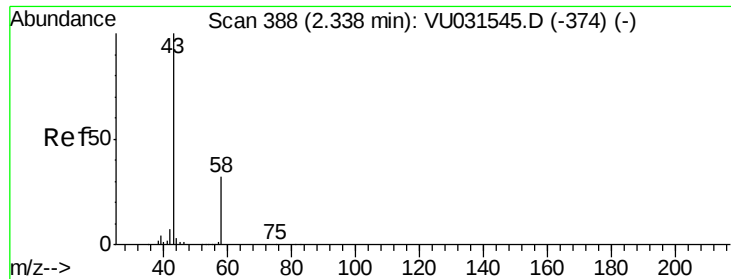

#13

Acetone

Concen: 1.379 ug/L

RT: 2.34 min Scan# 389

Delta R.T. 0.00 min

Lab File: VU031563.D

Acq: 27 Apr 2019 04:09

Instrument :

MSVOA_U

ClientSampleId :





C0X82

Tot Ion: 43 Resp: 10089

Ion Ratio Lower Upper

43 100

58 11.2 0.0 64.4

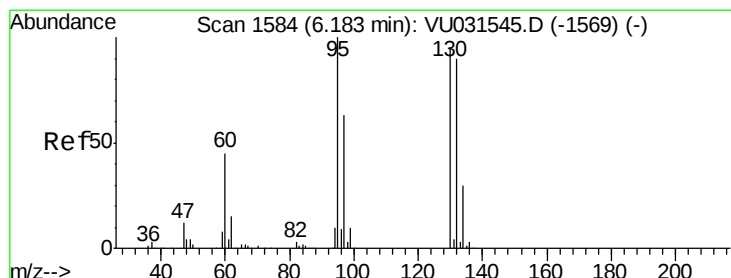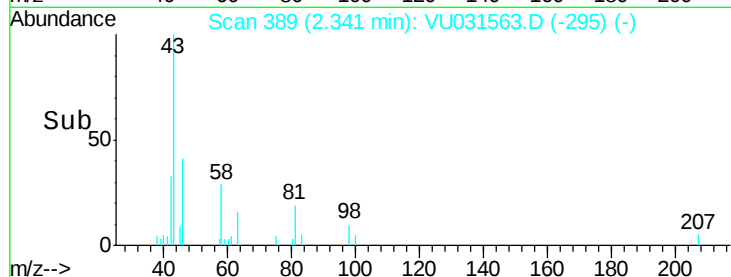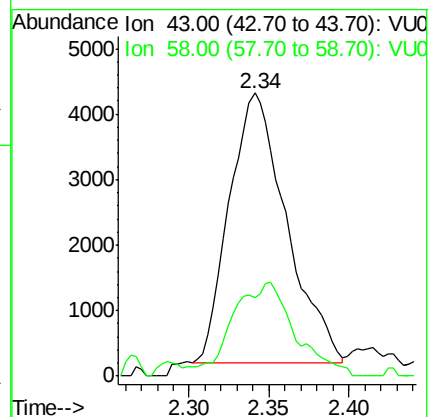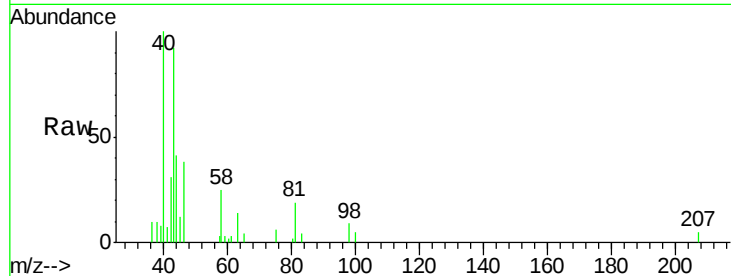

#34

Trichloroethene

Concen: 3.255 ug/L

RT: 6.19 min Scan# 1585

Delta R.T. 0.00 min

Lab File: VU031563.D

Acq: 27 Apr 2019 04:09

Tgt Ion: 95 Resp: 22739




Ion Ratio Lower Upper




95 100

97 58.2 44.8 83.2

132 96.1 63.1 117.1

130 88.8 66.5 123.5

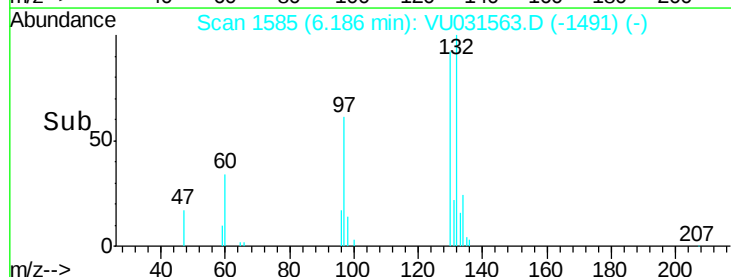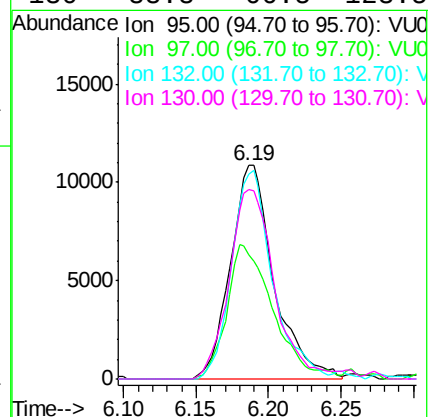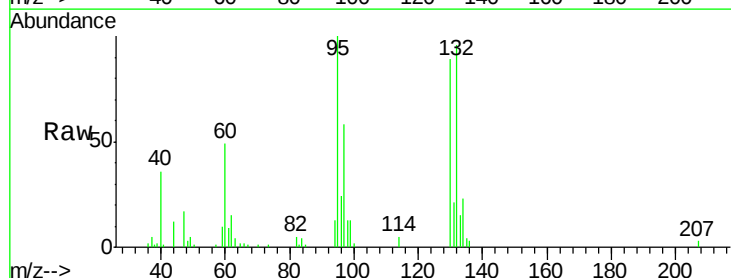

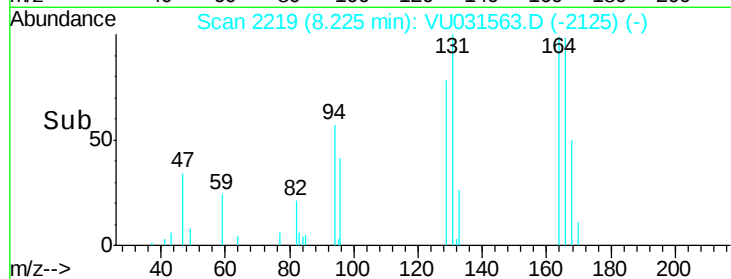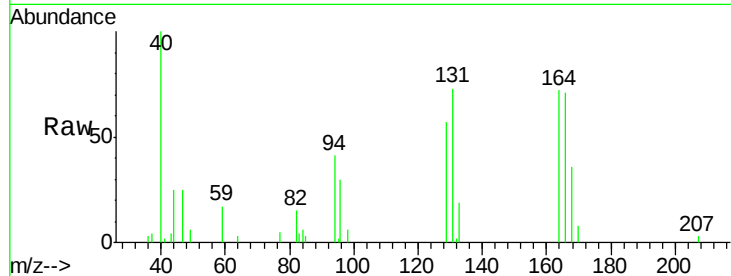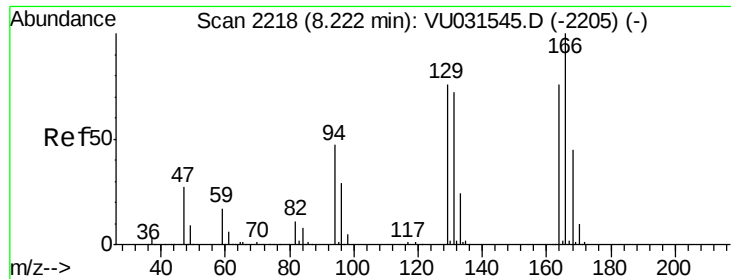

#46

Tetrachloroethene

Concen: 1.276 ug/L

RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU031563.D

Acq: 27 Apr 2019 04:09

Instrument :

MSVOA_U

ClientSampleId :

C0X82

Tot Ion:164 Resp: 6074

Ion Ratio Lower Upper

164 100

129 78.5 71.5 132.9

131 100.9 69.0 128.2

166 98.7 93.7 173.9

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

