

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031537.D
 Acq On : 26 Apr 2019 17:16
 Operator : JC/SP
 Sample : K2586-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	38	rVB2	22807	21232	0.53%	0.072%
2	1.396	87	95	108	rBV	578162	628995	15.76%	2.124%
3	1.679	175	183	199	rVB	444168	542605	13.60%	1.833%
4	2.267	356	366	380	rVB	943750	1448198	36.30%	4.891%
5	2.476	423	431	439	rVV2	5784	9153	0.23%	0.031%
6	2.560	453	457	461	rVB6	2089	1779	0.04%	0.006%
7	2.698	492	500	508	rBV8	4855	7484	0.19%	0.025%
8	2.942	572	576	579	rBV2	916	932	0.02%	0.003%
9	2.984	583	589	595	rVV8	3349	4798	0.12%	0.016%
10	3.132	627	635	641	rBV4	1699	2655	0.07%	0.009%
11	3.225	662	664	669	rVB3	1257	872	0.02%	0.003%
12	3.251	669	672	675	rBV2	1260	998	0.03%	0.003%
13	3.376	701	711	713	rBV6	1101	1781	0.04%	0.006%
14	3.389	713	715	718	rVV2	1291	756	0.02%	0.003%
15	3.408	718	721	724	rVB2	1046	718	0.02%	0.002%
16	3.550	762	765	769	rBV2	1464	1090	0.03%	0.004%
17	3.576	769	773	778	rVB4	1195	1200	0.03%	0.004%
18	3.604	778	782	785	rVB3	1487	1027	0.03%	0.003%
19	3.675	799	804	806	rBV3	882	752	0.02%	0.003%
20	3.759	827	830	834	rBV3	683	651	0.02%	0.002%
21	3.807	842	845	848	rBV3	1108	991	0.02%	0.003%
22	3.826	848	851	853	rVV2	1285	888	0.02%	0.003%
23	3.846	854	857	860	rVV3	1337	1022	0.03%	0.003%
24	3.965	890	894	897	rBV	1372	1060	0.03%	0.004%
25	4.067	922	926	929	rVB2	1409	996	0.02%	0.003%
26	4.087	929	932	938	rBV6	1413	1311	0.03%	0.004%
27	4.183	949	962	995	rBV	357488	1072457	26.88%	3.622%
28	4.643	1087	1105	1132	rVV	620770	1482474	37.16%	5.007%
29	4.958	1198	1203	1204	rBV2	1976	1523	0.04%	0.005%
30	4.984	1208	1211	1214	rBV2	2604	2110	0.05%	0.007%
31	5.080	1237	1241	1243	rBV4	1148	854	0.02%	0.003%
32	5.135	1254	1258	1260	rBV3	965	668	0.02%	0.002%
33	5.196	1274	1277	1282	rVB5	1217	881	0.02%	0.003%
34	5.334	1296	1320	1374	rBV2	1334375	3989917	100.00%	13.475%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031537.D
 Acq On : 26 Apr 2019 17:16
 Operator : JC/SP
 Sample : K2586-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.801	1463	1465	1471	rVB6	1609	1421	0.04%	0.005%
36	5.881	1476	1490	1514	rBV	1050984	2149584	53.88%	7.260%
37	6.186	1571	1585	1601	rBV4	98026	213479	5.35%	0.721%
38	6.325	1614	1628	1650	rBV	868283	1770349	44.37%	5.979%
39	6.653	1726	1730	1733	rBV3	1445	1282	0.03%	0.004%
40	6.730	1750	1754	1757	rBV4	761	636	0.02%	0.002%
41	6.755	1757	1762	1764	rVV2	831	761	0.02%	0.003%
42	6.794	1770	1774	1779	rVB3	1638	1419	0.04%	0.005%
43	6.891	1795	1804	1805	rBV6	2095	2588	0.06%	0.009%
44	6.952	1819	1823	1825	rBV3	1151	973	0.02%	0.003%
45	7.016	1840	1843	1846	rBV3	1284	876	0.02%	0.003%
46	7.125	1875	1877	1881	rVB2	1058	625	0.02%	0.002%
47	7.157	1881	1887	1891	rBV4	1144	1277	0.03%	0.004%
48	7.225	1894	1908	1935	rBV	469273	896615	22.47%	3.028%
49	7.469	1980	1984	1989	rVB5	4295	4169	0.10%	0.014%
50	7.563	2000	2013	2058	rBV	1651189	3083501	77.28%	10.414%
51	7.849	2091	2102	2124	rBV	321123	586729	14.71%	1.982%
52	8.071	2168	2171	2176	rVB5	1465	1471	0.04%	0.005%
53	8.170	2197	2202	2208	rBV8	1755	2159	0.05%	0.007%
54	8.202	2209	2212	2214	rBV2	1086	782	0.02%	0.003%
55	8.218	2214	2217	2218	rBV2	3212	1901	0.05%	0.006%
56	8.308	2234	2245	2295	rBV	1274478	2409037	60.38%	8.136%
57	8.588	2329	2332	2336	rBV5	2173	2037	0.05%	0.007%
58	8.733	2375	2377	2380	rBV3	1173	765	0.02%	0.003%
59	8.990	2452	2457	2459	rBV2	1047	1206	0.03%	0.004%
60	9.006	2460	2462	2466	rVB2	1067	779	0.02%	0.003%
61	9.087	2474	2487	2529	rVV	1475573	2597423	65.10%	8.772%
62	9.382	2572	2579	2588	rBV9	3835	7188	0.18%	0.024%
63	9.437	2594	2596	2598	rBV	1252	829	0.02%	0.003%
64	9.550	2629	2631	2636	rVB4	1634	1043	0.03%	0.004%
65	9.575	2636	2639	2642	rBV2	1870	1461	0.04%	0.005%
66	9.768	2696	2699	2700	rVV2	1180	676	0.02%	0.002%
67	9.794	2701	2707	2712	rVV8	2782	4246	0.11%	0.014%
68	9.868	2726	2730	2735	rBV3	1077	1325	0.03%	0.004%
69	9.916	2742	2745	2749	rVB2	1303	933	0.02%	0.003%
70	9.951	2754	2756	2759	rVV3	1112	814	0.02%	0.003%
71	9.971	2759	2762	2767	rVB2	1500	1504	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031537.D
 Acq On : 26 Apr 2019 17:16
 Operator : JC/SP
 Sample : K2586-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.022	2776	2778	2780	rBV3	1239	651	0.02%	0.002%
73	10.122	2806	2809	2812	rBV3	1435	1236	0.03%	0.004%
74	10.170	2818	2824	2833	rVB7	4259	6440	0.16%	0.022%
75	10.247	2845	2848	2850	rBV3	1652	1072	0.03%	0.004%
76	10.289	2854	2861	2866	rBV5	1680	2139	0.05%	0.007%
77	10.321	2867	2871	2872	rBV3	1318	840	0.02%	0.003%
78	10.331	2872	2874	2879	rVB4	1289	954	0.02%	0.003%
79	10.427	2891	2904	2936	rBV	1105145	1816517	45.53%	6.135%
80	10.582	2950	2952	2956	rBV3	1041	832	0.02%	0.003%
81	10.720	2989	2995	3001	rBV8	1440	2143	0.05%	0.007%
82	10.855	3035	3037	3042	rVB4	1121	761	0.02%	0.003%
83	11.273	3163	3167	3168	rBV2	1351	1149	0.03%	0.004%
84	11.305	3174	3177	3185	rVB6	2602	3102	0.08%	0.010%
85	11.347	3185	3190	3192	rBV3	1497	1329	0.03%	0.004%
86	11.398	3204	3206	3207	rBV2	1925	726	0.02%	0.002%
87	11.479	3220	3231	3253	rBV	1359614	2208958	55.36%	7.460%
88	11.746	3311	3314	3317	rBV3	1896	1403	0.04%	0.005%
89	11.855	3336	3348	3375	rBV	1459047	2431035	60.93%	8.210%
90	12.321	3490	3493	3495	rBV3	1753	1241	0.03%	0.004%
91	12.405	3517	3519	3523	rVB5	2137	1291	0.03%	0.004%
92	12.453	3531	3534	3539	rBV6	1621	1375	0.03%	0.005%
93	12.890	3666	3670	3677	rBV7	4693	6858	0.17%	0.023%
94	13.283	3789	3792	3793	rBV3	1830	952	0.02%	0.003%
95	13.321	3802	3804	3807	rBV3	1401	630	0.02%	0.002%
96	13.514	3857	3864	3867	rBV9	6810	10001	0.25%	0.034%
97	13.755	3932	3939	3945	rBV3	19300	32308	0.81%	0.109%
98	13.996	4005	4014	4024	rBV8	12896	29149	0.73%	0.098%
99	14.199	4074	4077	4081	rBV5	3645	3591	0.09%	0.012%
100	16.061	4650	4656	4663	rBV4	32074	51794	1.30%	0.175%


Sum of corrected areas: 29609168

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031537.D
Acq On : 26 Apr 2019 17:16
Operator : JC/SP
Sample : K2586-20 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0X66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

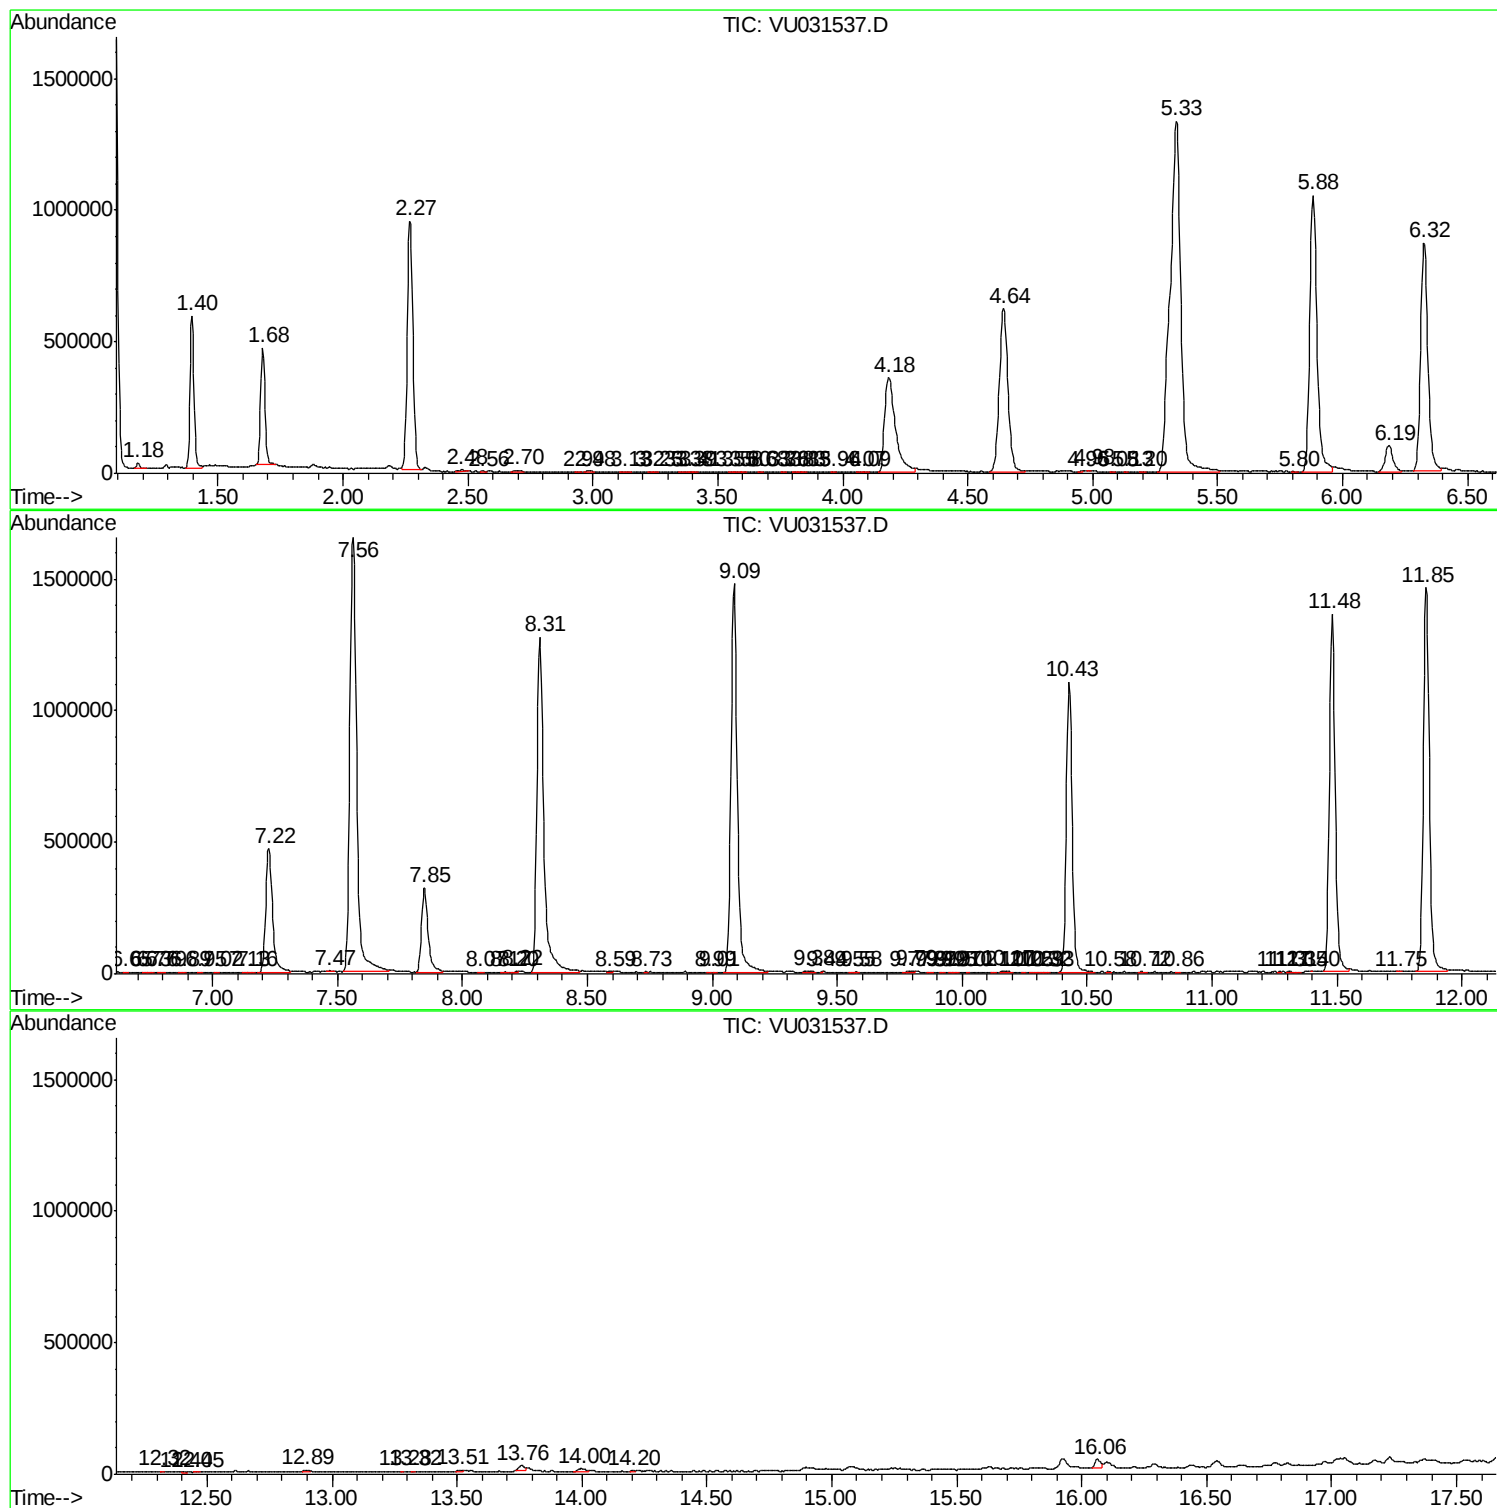

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031537.D
Acq On : 26 Apr 2019 17:16
Operator : JC/SP
Sample : K2586-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X66

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031537.D
Acq On : 26 Apr 2019 17:16
Operator : JC/SP
Sample : K2586-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X66

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
