

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031539.D
 Acq On : 26 Apr 2019 18:03
 Operator : JC/SP
 Sample : K2590-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rBV3	21732	23195	0.59%	0.081%
2	1.395	88	95	107	rBV	564551	607488	15.52%	2.125%
3	1.678	176	183	204	rVB	432349	547713	13.99%	1.916%
4	2.270	356	367	381	rVB	932224	1424417	36.39%	4.984%
5	2.453	421	424	426	rBV3	1552	881	0.02%	0.003%
6	2.479	426	432	436	rBV6	3301	4272	0.11%	0.015%
7	2.646	480	484	485	rBV3	1377	1108	0.03%	0.004%
8	2.701	491	501	511	rBV7	4059	8449	0.22%	0.030%
9	2.907	561	565	571	rVB3	1726	1539	0.04%	0.005%
10	2.964	579	583	586	rBV3	1251	1200	0.03%	0.004%
11	2.987	586	590	594	rVB5	809	805	0.02%	0.003%
12	3.087	618	621	626	rBV2	976	833	0.02%	0.003%
13	3.148	635	640	643	rBV2	1359	1182	0.03%	0.004%
14	3.373	702	710	713	rBV4	1232	1395	0.04%	0.005%
15	3.405	718	720	724	rVB2	1167	801	0.02%	0.003%
16	3.431	724	728	733	rVB2	1459	1240	0.03%	0.004%
17	3.517	751	755	760	rBV4	767	933	0.02%	0.003%
18	3.607	778	783	787	rBV5	1221	1136	0.03%	0.004%
19	3.707	810	814	817	rBV2	1170	1014	0.03%	0.004%
20	3.945	882	888	890	rBV3	881	766	0.02%	0.003%
21	3.977	895	898	902	rVB2	1043	769	0.02%	0.003%
22	4.022	907	912	915	rBV3	1294	1497	0.04%	0.005%
23	4.106	936	938	944	rVB3	1085	846	0.02%	0.003%
24	4.186	950	963	1003	rBV2	344842	1072409	27.40%	3.752%
25	4.556	1075	1078	1080	rBV3	1407	917	0.02%	0.003%
26	4.643	1089	1105	1133	rBV2	613694	1442797	36.86%	5.048%
27	4.826	1160	1162	1165	rBV3	1400	1021	0.03%	0.004%
28	4.929	1191	1194	1198	rVB4	1797	1542	0.04%	0.005%
29	5.070	1233	1238	1240	rBV3	1447	994	0.03%	0.003%
30	5.125	1251	1255	1257	rBV2	1406	929	0.02%	0.003%
31	5.144	1257	1261	1263	rVV2	982	769	0.02%	0.003%
32	5.334	1296	1320	1364	rVV2	1311736	3913851	100.00%	13.694%
33	5.759	1449	1452	1455	rVV3	2046	1619	0.04%	0.006%
34	5.781	1455	1459	1468	rVB8	1252	1744	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031539.D
 Acq On : 26 Apr 2019 18:03
 Operator : JC/SP
 Sample : K2590-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.884	1476	1491	1513	rBV	1023605	2123874	54.27%	7.431%
36	6.180	1576	1583	1602	rVB10	12338	27029	0.69%	0.095%
37	6.328	1614	1629	1651	rBV	839084	1727916	44.15%	6.046%
38	6.533	1689	1693	1698	rVB6	2204	2252	0.06%	0.008%
39	6.566	1698	1703	1705	rBV5	1288	1333	0.03%	0.005%
40	6.601	1711	1714	1716	rBV2	1254	928	0.02%	0.003%
41	6.659	1730	1732	1738	rBV6	903	944	0.02%	0.003%
42	6.794	1771	1774	1777	rBV2	986	790	0.02%	0.003%
43	6.823	1777	1783	1787	rBV6	2009	2018	0.05%	0.007%
44	6.868	1792	1797	1798	rBV3	1352	970	0.02%	0.003%
45	6.906	1807	1809	1813	rVB4	1870	1062	0.03%	0.004%
46	6.993	1834	1836	1839	rVV2	1512	900	0.02%	0.003%
47	7.016	1839	1843	1846	rVB2	1267	907	0.02%	0.003%
48	7.061	1855	1857	1861	rVB3	1435	803	0.02%	0.003%
49	7.086	1861	1865	1869	rVB3	1130	842	0.02%	0.003%
50	7.225	1896	1908	1935	rBV	461847	866786	22.15%	3.033%
51	7.504	1993	1995	1999	rBV3	1129	898	0.02%	0.003%
52	7.562	1999	2013	2062	rBV	1595619	3050010	77.93%	10.671%
53	7.848	2090	2102	2128	rBV	302122	566338	14.47%	1.981%
54	8.151	2193	2196	2199	rVB4	1427	902	0.02%	0.003%
55	8.173	2199	2203	2207	rVB6	1289	1284	0.03%	0.004%
56	8.225	2214	2219	2220	rBV5	3887	3074	0.08%	0.011%
57	8.308	2234	2245	2281	rBV	1223602	2311644	59.06%	8.088%
58	8.617	2339	2341	2346	rVB4	1484	893	0.02%	0.003%
59	8.684	2357	2362	2365	rBV4	1988	1508	0.04%	0.005%
60	8.701	2365	2367	2371	rBV2	1351	1068	0.03%	0.004%
61	8.752	2379	2383	2385	rBV2	1270	919	0.02%	0.003%
62	8.913	2427	2433	2435	rBV5	1540	1628	0.04%	0.006%
63	8.958	2444	2447	2451	rVB4	1211	869	0.02%	0.003%
64	9.086	2472	2487	2517	rBV	1446289	2546835	65.07%	8.911%
65	9.347	2566	2568	2574	rVB5	1712	1194	0.03%	0.004%
66	9.376	2574	2577	2579	rBV2	1733	1280	0.03%	0.004%
67	9.466	2600	2605	2608	rBV4	1637	1612	0.04%	0.006%
68	9.704	2673	2679	2681	rBV5	1257	1167	0.03%	0.004%
69	9.720	2681	2684	2686	rVV3	1539	971	0.02%	0.003%
70	9.733	2686	2688	2693	rVB3	1406	897	0.02%	0.003%
71	9.781	2700	2703	2706	rBV4	1076	874	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031539.D
 Acq On : 26 Apr 2019 18:03
 Operator : JC/SP
 Sample : K2590-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X96

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.980	2761	2765	2768	rBV4	1447	1442	0.04%	0.005%
73	10.135	2803	2813	2816	rBV6	1676	2113	0.05%	0.007%
74	10.164	2820	2822	2825	rBV4	1120	751	0.02%	0.003%
75	10.218	2836	2839	2845	rVB4	1610	1425	0.04%	0.005%
76	10.427	2891	2904	2924	rBV	1087048	1766831	45.14%	6.182%
77	10.530	2933	2936	2939	rBV4	1691	991	0.03%	0.003%
78	10.755	3002	3006	3009	rBV2	1676	1407	0.04%	0.005%
79	10.877	3040	3044	3049	rBV3	1669	1842	0.05%	0.006%
80	10.961	3066	3070	3072	rBV2	2061	1591	0.04%	0.006%
81	11.009	3079	3085	3087	rBV4	1925	1978	0.05%	0.007%
82	11.054	3095	3099	3101	rBV4	1439	1144	0.03%	0.004%
83	11.086	3101	3109	3112	rVV5	2359	3168	0.08%	0.011%
84	11.167	3131	3134	3138	rVB2	2459	1874	0.05%	0.007%
85	11.196	3138	3143	3145	rBV3	2387	2015	0.05%	0.007%
86	11.299	3172	3175	3178	rBV3	964	778	0.02%	0.003%
87	11.401	3203	3207	3208	rBV2	1117	778	0.02%	0.003%
88	11.421	3211	3213	3216	rVB4	1497	866	0.02%	0.003%
89	11.479	3216	3231	3258	rBV	1308098	2140012	54.68%	7.487%
90	11.855	3336	3348	3373	rBV	1380254	2308204	58.98%	8.076%
91	12.225	3460	3463	3468	rBV3	2080	2200	0.06%	0.008%
92	12.729	3617	3620	3624	rVB3	2390	1781	0.05%	0.006%
93	12.816	3644	3647	3650	rBV3	1424	1013	0.03%	0.004%
94	12.977	3693	3697	3698	rBV4	1523	931	0.02%	0.003%
95	13.060	3720	3723	3726	rVB4	1846	1201	0.03%	0.004%
96	13.446	3839	3843	3845	rBV5	1753	1379	0.04%	0.005%
97	13.520	3862	3866	3868	rBV3	1422	1143	0.03%	0.004%
98	13.623	3896	3898	3902	rVB3	1672	1059	0.03%	0.004%
99	13.642	3902	3904	3907	rBV2	1335	957	0.02%	0.003%
100	13.774	3942	3945	3948	rBV3	3502	3299	0.08%	0.012%


Sum of corrected areas: 28581463

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031539.D
Acq On : 26 Apr 2019 18:03
Operator : JC/SP
Sample : K2590-06 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

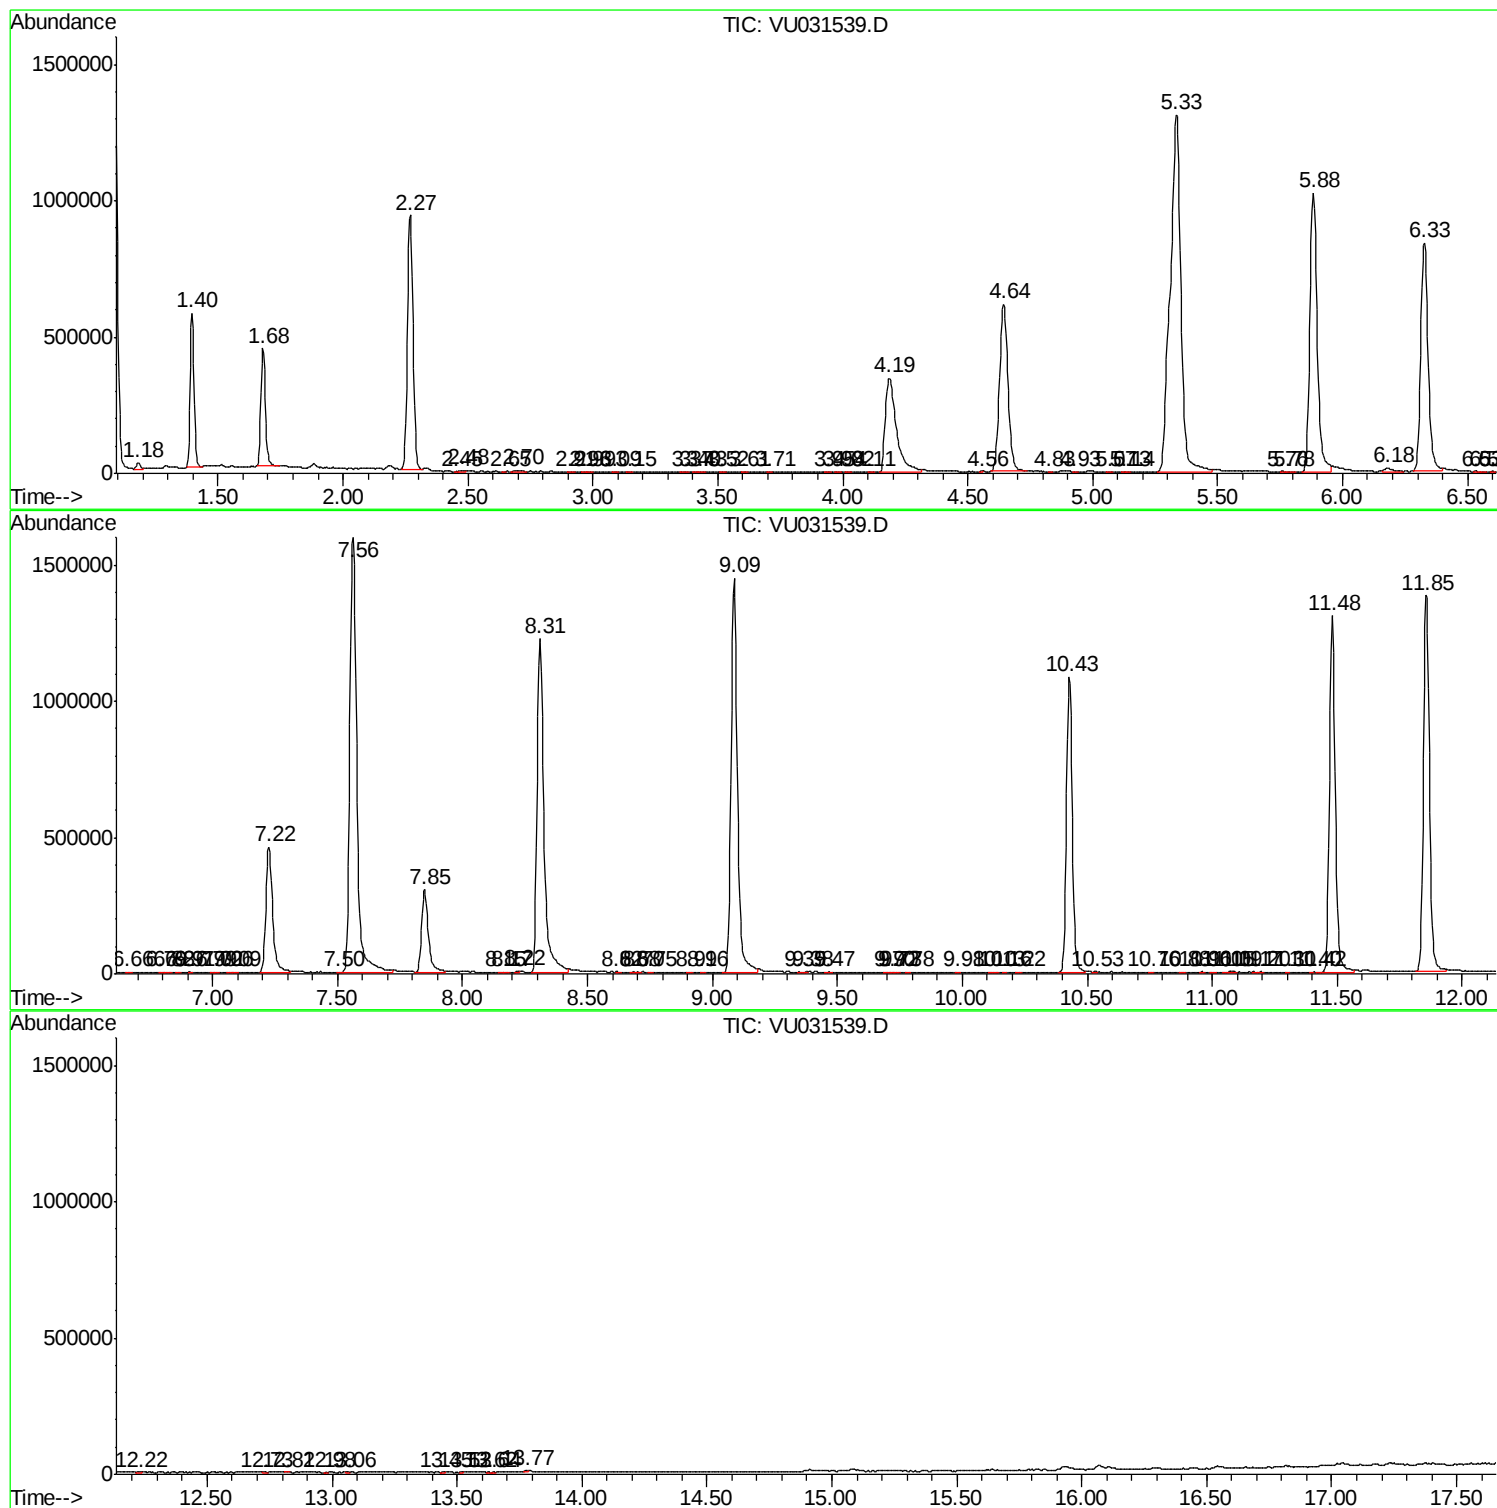

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031539.D
Acq On : 26 Apr 2019 18:03
Operator : JC/SP
Sample : K2590-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X96

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031539.D
Acq On : 26 Apr 2019 18:03
Operator : JC/SP
Sample : K2590-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X96

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc