

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031543.D
 Acq On : 26 Apr 2019 19:36
 Operator : JC/SP
 Sample : K2536-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rVB2	22902	21320	0.56%	0.072%
2	1.395	88	95	107	rBV	555205	583919	15.43%	1.962%
3	1.678	176	183	196	rBV	408689	510311	13.49%	1.715%
4	2.267	356	366	380	rVB	893927	1370490	36.22%	4.605%
5	2.456	421	425	426	rBV3	1571	1169	0.03%	0.004%
6	2.501	436	439	441	rBV4	1739	1133	0.03%	0.004%
7	2.559	451	457	462	rBV6	2542	3245	0.09%	0.011%
8	2.694	494	499	501	rBV5	2620	2663	0.07%	0.009%
9	2.823	535	539	543	rVB6	1612	1374	0.04%	0.005%
10	2.852	543	548	555	rBV6	1469	1620	0.04%	0.005%
11	2.971	582	585	590	rVB2	1694	1197	0.03%	0.004%
12	3.000	590	594	599	rVB2	2853	2254	0.06%	0.008%
13	3.042	604	607	612	rVB3	1562	1475	0.04%	0.005%
14	3.071	612	616	619	rBV2	1261	904	0.02%	0.003%
15	3.190	651	653	658	rVB2	1691	1210	0.03%	0.004%
16	3.218	658	662	663	rBV	1556	1128	0.03%	0.004%
17	3.267	673	677	680	rBV3	1440	1104	0.03%	0.004%
18	3.325	690	695	697	rBV2	1520	1088	0.03%	0.004%
19	3.341	697	700	705	rVV4	1606	1605	0.04%	0.005%
20	3.434	724	729	732	rVB5	1512	1186	0.03%	0.004%
21	3.460	732	737	739	rBV	1381	1190	0.03%	0.004%
22	3.498	745	749	751	rVV3	1009	892	0.02%	0.003%
23	3.546	761	764	769	rVV3	979	918	0.02%	0.003%
24	3.608	779	783	786	rBV2	1229	1064	0.03%	0.004%
25	3.675	800	804	809	rVB4	978	927	0.02%	0.003%
26	3.720	814	818	821	rBV	2013	1615	0.04%	0.005%
27	3.791	835	840	845	rBV4	888	857	0.02%	0.003%
28	3.826	845	851	852	rBV3	1007	1037	0.03%	0.003%
29	3.894	867	872	878	rBV	1554	2020	0.05%	0.007%
30	3.964	889	894	896	rBV3	964	842	0.02%	0.003%
31	4.019	905	911	915	rBV3	2062	2047	0.05%	0.007%
32	4.190	951	964	1003	rBV2	328481	1086137	28.70%	3.649%
33	4.643	1088	1105	1130	rBV	597492	1411061	37.29%	4.741%
34	4.871	1170	1176	1180	rBV6	2070	2988	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031543.D
 Acq On : 26 Apr 2019 19:36
 Operator : JC/SP
 Sample : K2536-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.964	1201	1205	1208	rBV4	2577	2596	0.07%	0.009%
36	5.074	1236	1239	1245	rVB3	1298	1052	0.03%	0.004%
37	5.218	1280	1284	1289	rVB5	1215	1486	0.04%	0.005%
38	5.334	1295	1320	1353	rBV2	1261746	3783970	100.00%	12.714%
39	5.768	1452	1455	1459	rBV4	1352	1166	0.03%	0.004%
40	5.788	1459	1461	1464	rBV2	1462	836	0.02%	0.003%
41	5.881	1477	1490	1525	rBV	1011731	2127572	56.23%	7.149%
42	6.183	1570	1584	1613	rBV	849271	1723153	45.54%	5.790%
43	6.328	1616	1629	1660	rVB	819843	1685443	44.54%	5.663%
44	6.598	1709	1713	1718	rVB8	2330	2744	0.07%	0.009%
45	6.630	1718	1723	1725	rBV3	1148	1132	0.03%	0.004%
46	6.681	1737	1739	1746	rVB7	1253	1257	0.03%	0.004%
47	6.726	1751	1753	1760	rVB6	1258	921	0.02%	0.003%
48	6.784	1766	1771	1777	rBV5	1530	2010	0.05%	0.007%
49	6.836	1782	1787	1791	rBV4	845	836	0.02%	0.003%
50	6.903	1803	1808	1814	rVB6	1237	1477	0.04%	0.005%
51	7.019	1841	1844	1847	rVB	1737	977	0.03%	0.003%
52	7.225	1896	1908	1936	rBV	447181	841361	22.23%	2.827%
53	7.562	1998	2013	2049	rBV	1558423	2932447	77.50%	9.853%
54	7.849	2091	2102	2130	rBV2	297958	551442	14.57%	1.853%
55	8.016	2151	2154	2157	rBV3	1135	986	0.03%	0.003%
56	8.032	2157	2159	2162	rVB2	1626	851	0.02%	0.003%
57	8.128	2186	2189	2195	rVB6	1273	1119	0.03%	0.004%
58	8.228	2209	2220	2235	rBV2	39092	73730	1.95%	0.248%
59	8.308	2235	2245	2280	rBV	1200865	2289801	60.51%	7.694%
60	8.752	2377	2383	2386	rBV4	1754	2257	0.06%	0.008%
61	8.871	2417	2420	2424	rVV	1686	1149	0.03%	0.004%
62	8.935	2435	2440	2442	rBV3	1396	1039	0.03%	0.003%
63	9.086	2474	2487	2524	rBV	1414952	2537765	67.07%	8.527%
64	9.414	2586	2589	2594	rVB5	2738	2218	0.06%	0.007%
65	9.443	2594	2598	2602	rBV5	1525	1315	0.03%	0.004%
66	9.533	2622	2626	2629	rBV2	1093	1036	0.03%	0.003%
67	9.829	2715	2718	2724	rBV4	1243	1286	0.03%	0.004%
68	9.903	2737	2741	2744	rBV3	2342	1804	0.05%	0.006%
69	10.057	2787	2789	2793	rVB3	1347	933	0.02%	0.003%
70	10.083	2793	2797	2800	rBV4	1285	981	0.03%	0.003%
71	10.109	2801	2805	2809	rVB5	1713	1456	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031543.D
 Acq On : 26 Apr 2019 19:36
 Operator : JC/SP
 Sample : K2536-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X05

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.164	2815	2822	2826	rBV4	3233	4156	0.11%	0.014%
73	10.369	2883	2886	2891	rVB2	1920	1415	0.04%	0.005%
74	10.427	2891	2904	2929	rBV	1063382	1752227	46.31%	5.887%
75	10.678	2978	2982	2984	rBV2	1312	972	0.03%	0.003%
76	10.755	3002	3006	3008	rBV4	1661	1059	0.03%	0.004%
77	10.800	3016	3020	3025	rBV5	1326	1397	0.04%	0.005%
78	10.861	3037	3039	3044	rVB3	1326	938	0.02%	0.003%
79	10.903	3048	3052	3055	rBV	1685	1600	0.04%	0.005%
80	10.964	3068	3071	3077	rVB4	1878	1761	0.05%	0.006%
81	11.000	3078	3082	3087	rBV5	1473	1646	0.04%	0.006%
82	11.138	3122	3125	3127	rBV3	1382	971	0.03%	0.003%
83	11.186	3138	3140	3144	rVB2	1185	832	0.02%	0.003%
84	11.276	3165	3168	3170	rBV2	1393	839	0.02%	0.003%
85	11.408	3205	3209	3216	rVB8	1952	2059	0.05%	0.007%
86	11.482	3216	3232	3255	rBV	1266642	2108567	55.72%	7.085%
87	11.855	3336	3348	3375	rBV	1334193	2255596	59.61%	7.579%
88	12.446	3527	3532	3536	rBV4	2053	2638	0.07%	0.009%
89	12.517	3551	3554	3556	rBV2	1516	1020	0.03%	0.003%
90	12.559	3563	3567	3570	rBV2	2211	1527	0.04%	0.005%
91	12.617	3582	3585	3587	rVB4	1688	853	0.02%	0.003%
92	12.877	3663	3666	3669	rBV3	1327	1188	0.03%	0.004%
93	12.942	3680	3686	3690	rBV6	1903	2370	0.06%	0.008%
94	13.192	3761	3764	3768	rBV	1324	901	0.02%	0.003%
95	13.260	3781	3785	3787	rBV2	1692	1352	0.04%	0.005%
96	13.755	3937	3939	3943	rBV3	1167	916	0.02%	0.003%
97	13.858	3967	3971	3977	rBV4	2127	2422	0.06%	0.008%
98	13.893	3980	3982	3985	rVV	1700	900	0.02%	0.003%
99	14.015	4017	4020	4023	rBV3	1705	1437	0.04%	0.005%
100	14.202	4076	4078	4081	rBV3	1576	947	0.03%	0.003%


Sum of corrected areas: 29762100

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031543.D
Acq On : 26 Apr 2019 19:36
Operator : JC/SP
Sample : K2536-17 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

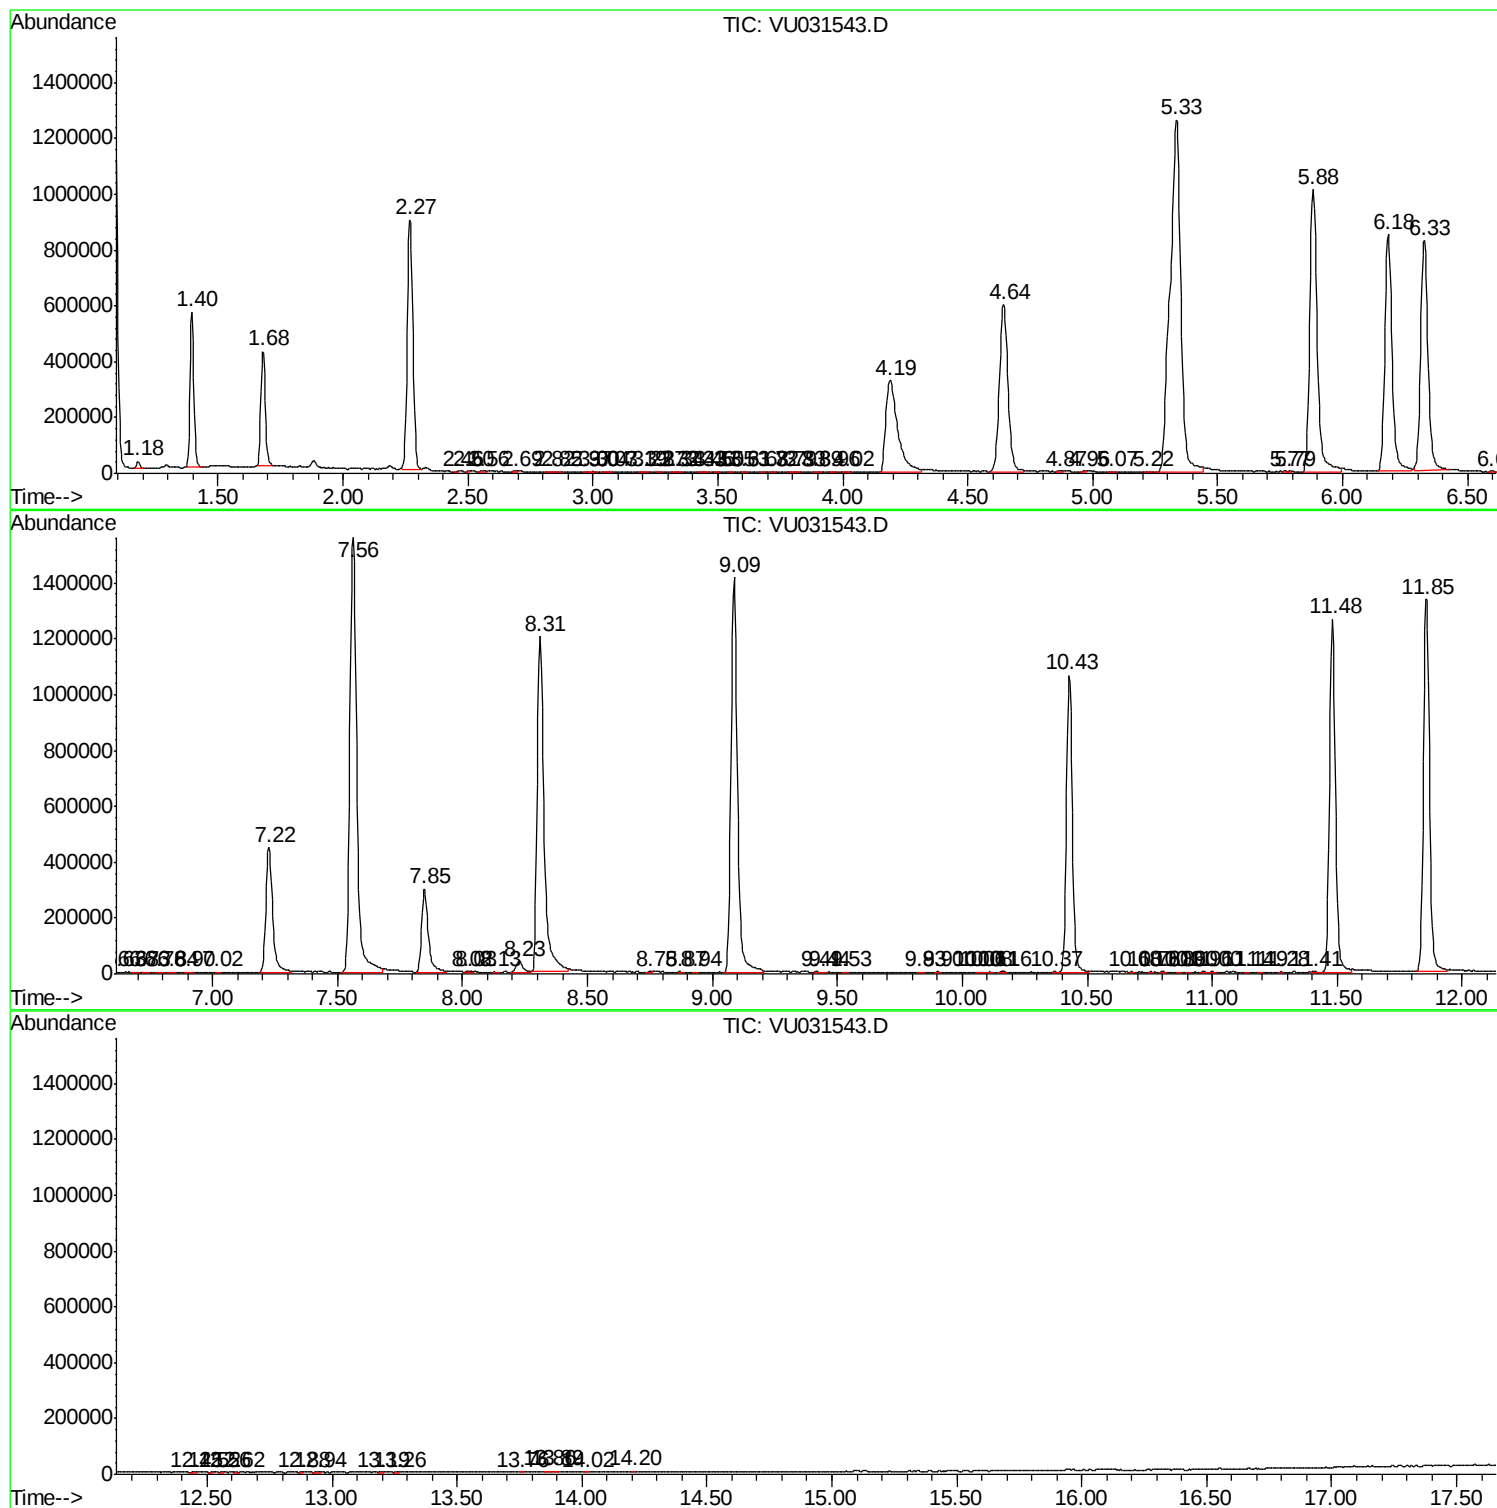

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031543.D
Acq On : 26 Apr 2019 19:36
Operator : JC/SP
Sample : K2536-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X05

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031543.D
Acq On : 26 Apr 2019 19:36
Operator : JC/SP
Sample : K2536-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X05

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
