

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031544.D
 Acq On : 26 Apr 2019 19:59
 Operator : JC/SP
 Sample : K2536-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	39	rVB3	24266	27121	0.69%	0.090%
2	1.289	59	62	67	rBV	11364	8616	0.22%	0.029%
3	1.396	87	95	108	rBV	573459	618536	15.74%	2.052%
4	1.679	175	183	194	rBV	426479	535615	13.63%	1.777%
5	2.267	355	366	381	rBV	924207	1413939	35.99%	4.692%
6	2.441	417	420	422	rBV2	1150	950	0.02%	0.003%
7	2.453	422	424	427	rVV3	1868	1141	0.03%	0.004%
8	2.473	427	430	435	rVB5	1735	1833	0.05%	0.006%
9	2.543	447	452	455	rBV4	1696	1559	0.04%	0.005%
10	2.695	494	499	502	rBV7	3051	3437	0.09%	0.011%
11	2.743	512	514	517	rBV2	1038	682	0.02%	0.002%
12	2.778	522	525	528	rVB3	1598	943	0.02%	0.003%
13	2.794	528	530	534	rBV	1228	735	0.02%	0.002%
14	2.833	539	542	545	rVB4	1181	703	0.02%	0.002%
15	2.926	567	571	574	rBV2	1141	785	0.02%	0.003%
16	3.103	623	626	630	rVB3	1189	805	0.02%	0.003%
17	3.132	630	635	638	rBV3	1769	1273	0.03%	0.004%
18	3.199	652	656	658	rBV2	1430	827	0.02%	0.003%
19	3.215	658	661	663	rBV	1203	789	0.02%	0.003%
20	3.373	707	710	712	rBV2	1324	845	0.02%	0.003%
21	3.412	719	722	730	rVB3	1317	1183	0.03%	0.004%
22	3.534	757	760	764	rVB2	1420	1184	0.03%	0.004%
23	3.633	789	791	796	rVB2	1110	879	0.02%	0.003%
24	3.839	852	855	857	rBV2	1612	1064	0.03%	0.004%
25	3.878	864	867	870	rBV	1063	773	0.02%	0.003%
26	3.929	877	883	886	rBV4	731	712	0.02%	0.002%
27	4.106	934	938	941	rBV3	1321	1110	0.03%	0.004%
28	4.186	949	963	999	rBV	345543	1106509	28.16%	3.672%
29	4.547	1072	1075	1077	rBV2	1232	874	0.02%	0.003%
30	4.643	1088	1105	1130	rBV	618569	1480986	37.69%	4.914%
31	4.990	1210	1213	1214	rBV2	1860	1069	0.03%	0.004%
32	5.125	1251	1255	1261	rVB3	1487	1548	0.04%	0.005%
33	5.241	1288	1291	1296	rVB3	1554	1047	0.03%	0.003%
34	5.334	1296	1320	1355	rBV2	1317794	3929098	100.00%	13.037%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031544.D
 Acq On : 26 Apr 2019 19:59
 Operator : JC/SP
 Sample : K2536-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.756	1448	1451	1454	rBV3	1833	1180	0.03%	0.004%
36	5.881	1477	1490	1520	rBV	1047658	2152026	54.77%	7.141%
37	6.119	1562	1564	1568	rVB5	1729	794	0.02%	0.003%
38	6.183	1570	1584	1614	rBV	715202	1452408	36.97%	4.819%
39	6.325	1615	1628	1649	rBV	844580	1718512	43.74%	5.702%
40	6.720	1747	1751	1758	rBV3	2164	2481	0.06%	0.008%
41	6.752	1758	1761	1763	rVV4	1115	714	0.02%	0.002%
42	6.765	1763	1765	1770	rVV3	944	725	0.02%	0.002%
43	6.916	1809	1812	1814	rBV	1412	780	0.02%	0.003%
44	7.022	1842	1845	1849	rBV2	1545	1126	0.03%	0.004%
45	7.061	1854	1857	1859	rBV	963	685	0.02%	0.002%
46	7.122	1871	1876	1881	rVB6	1753	1958	0.05%	0.006%
47	7.151	1881	1885	1887	rBV2	1447	1151	0.03%	0.004%
48	7.225	1896	1908	1940	rVV	457054	868934	22.12%	2.883%
49	7.485	1986	1989	1993	rBV3	1516	1304	0.03%	0.004%
50	7.563	1998	2013	2049	rBV	1602056	2990482	76.11%	9.923%
51	7.845	2090	2101	2130	rBV	302620	565582	14.39%	1.877%
52	8.080	2171	2174	2177	rBV4	1382	1133	0.03%	0.004%
53	8.119	2183	2186	2190	rVB3	2231	1603	0.04%	0.005%
54	8.183	2203	2206	2210	rVB3	1586	1225	0.03%	0.004%
55	8.225	2210	2219	2232	rBV4	27197	52297	1.33%	0.174%
56	8.308	2235	2245	2281	rBV	1240957	2355466	59.95%	7.816%
57	8.620	2339	2342	2345	rBV3	1542	1388	0.04%	0.005%
58	8.656	2350	2353	2355	rBV2	1247	916	0.02%	0.003%
59	8.749	2379	2382	2385	rBV4	1245	741	0.02%	0.002%
60	8.826	2403	2406	2410	rBV5	1589	1459	0.04%	0.005%
61	9.087	2474	2487	2517	rBV	1456679	2568028	65.36%	8.521%
62	9.337	2561	2565	2570	rBV4	1864	1833	0.05%	0.006%
63	9.389	2579	2581	2590	rVB8	1901	1626	0.04%	0.005%
64	9.614	2648	2651	2653	rBV2	1421	743	0.02%	0.002%
65	9.903	2738	2741	2742	rBV	1694	1097	0.03%	0.004%
66	9.974	2761	2763	2767	rVV3	1145	702	0.02%	0.002%
67	10.022	2772	2778	2781	rVB5	1631	1395	0.04%	0.005%
68	10.193	2829	2831	2838	rVB7	1551	1608	0.04%	0.005%
69	10.231	2838	2843	2846	rBV4	1121	1154	0.03%	0.004%
70	10.260	2846	2852	2855	rVB4	1587	1380	0.04%	0.005%
71	10.279	2855	2858	2860	rBV	1551	1027	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031544.D
 Acq On : 26 Apr 2019 19:59
 Operator : JC/SP
 Sample : K2536-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.305	2862	2866	2871	rVB3	2070	2200	0.06%	0.007%
73	10.347	2876	2879	2889	rVB6	1944	3067	0.08%	0.010%
74	10.427	2891	2904	2928	rBV	1114154	1795513	45.70%	5.958%
75	10.585	2950	2953	2956	rBV3	1322	1050	0.03%	0.003%
76	10.617	2960	2963	2967	rVB3	1755	1451	0.04%	0.005%
77	10.697	2985	2988	2991	rBV2	1540	1091	0.03%	0.004%
78	10.746	3000	3003	3009	rVB4	1550	1527	0.04%	0.005%
79	10.784	3009	3015	3018	rBV3	2294	2277	0.06%	0.008%
80	10.823	3024	3027	3032	rVB2	1245	1094	0.03%	0.004%
81	11.029	3089	3091	3095	rBV3	931	796	0.02%	0.003%
82	11.083	3103	3108	3113	rVB7	2244	2234	0.06%	0.007%
83	11.183	3135	3139	3141	rBV	1549	1265	0.03%	0.004%
84	11.276	3165	3168	3172	rBV3	1665	1337	0.03%	0.004%
85	11.299	3172	3175	3182	rVV5	1403	1402	0.04%	0.005%
86	11.376	3196	3199	3202	rBV2	1119	966	0.02%	0.003%
87	11.431	3213	3216	3218	rBV4	1138	831	0.02%	0.003%
88	11.479	3219	3231	3256	rBV	1265220	2104043	53.55%	6.982%
89	11.858	3335	3349	3374	rBV	1363011	2295421	58.42%	7.617%
90	12.431	3524	3527	3529	rBV3	2352	1716	0.04%	0.006%
91	12.556	3563	3566	3571	rVB3	1780	1437	0.04%	0.005%
92	12.582	3571	3574	3576	rBV3	1255	870	0.02%	0.003%
93	12.678	3601	3604	3609	rBV5	1684	1260	0.03%	0.004%
94	12.800	3640	3642	3646	rBV3	987	785	0.02%	0.003%
95	12.845	3653	3656	3659	rBV2	1545	1107	0.03%	0.004%
96	12.868	3661	3663	3666	rVV3	1330	839	0.02%	0.003%
97	13.131	3741	3745	3748	rBV4	1537	1358	0.03%	0.005%
98	13.813	3954	3957	3959	rBV3	1858	1125	0.03%	0.004%
99	13.913	3985	3988	3989	rBV2	1555	931	0.02%	0.003%
100	14.720	4236	4239	4242	rBV2	1938	1240	0.03%	0.004%


Sum of corrected areas: 30137066

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

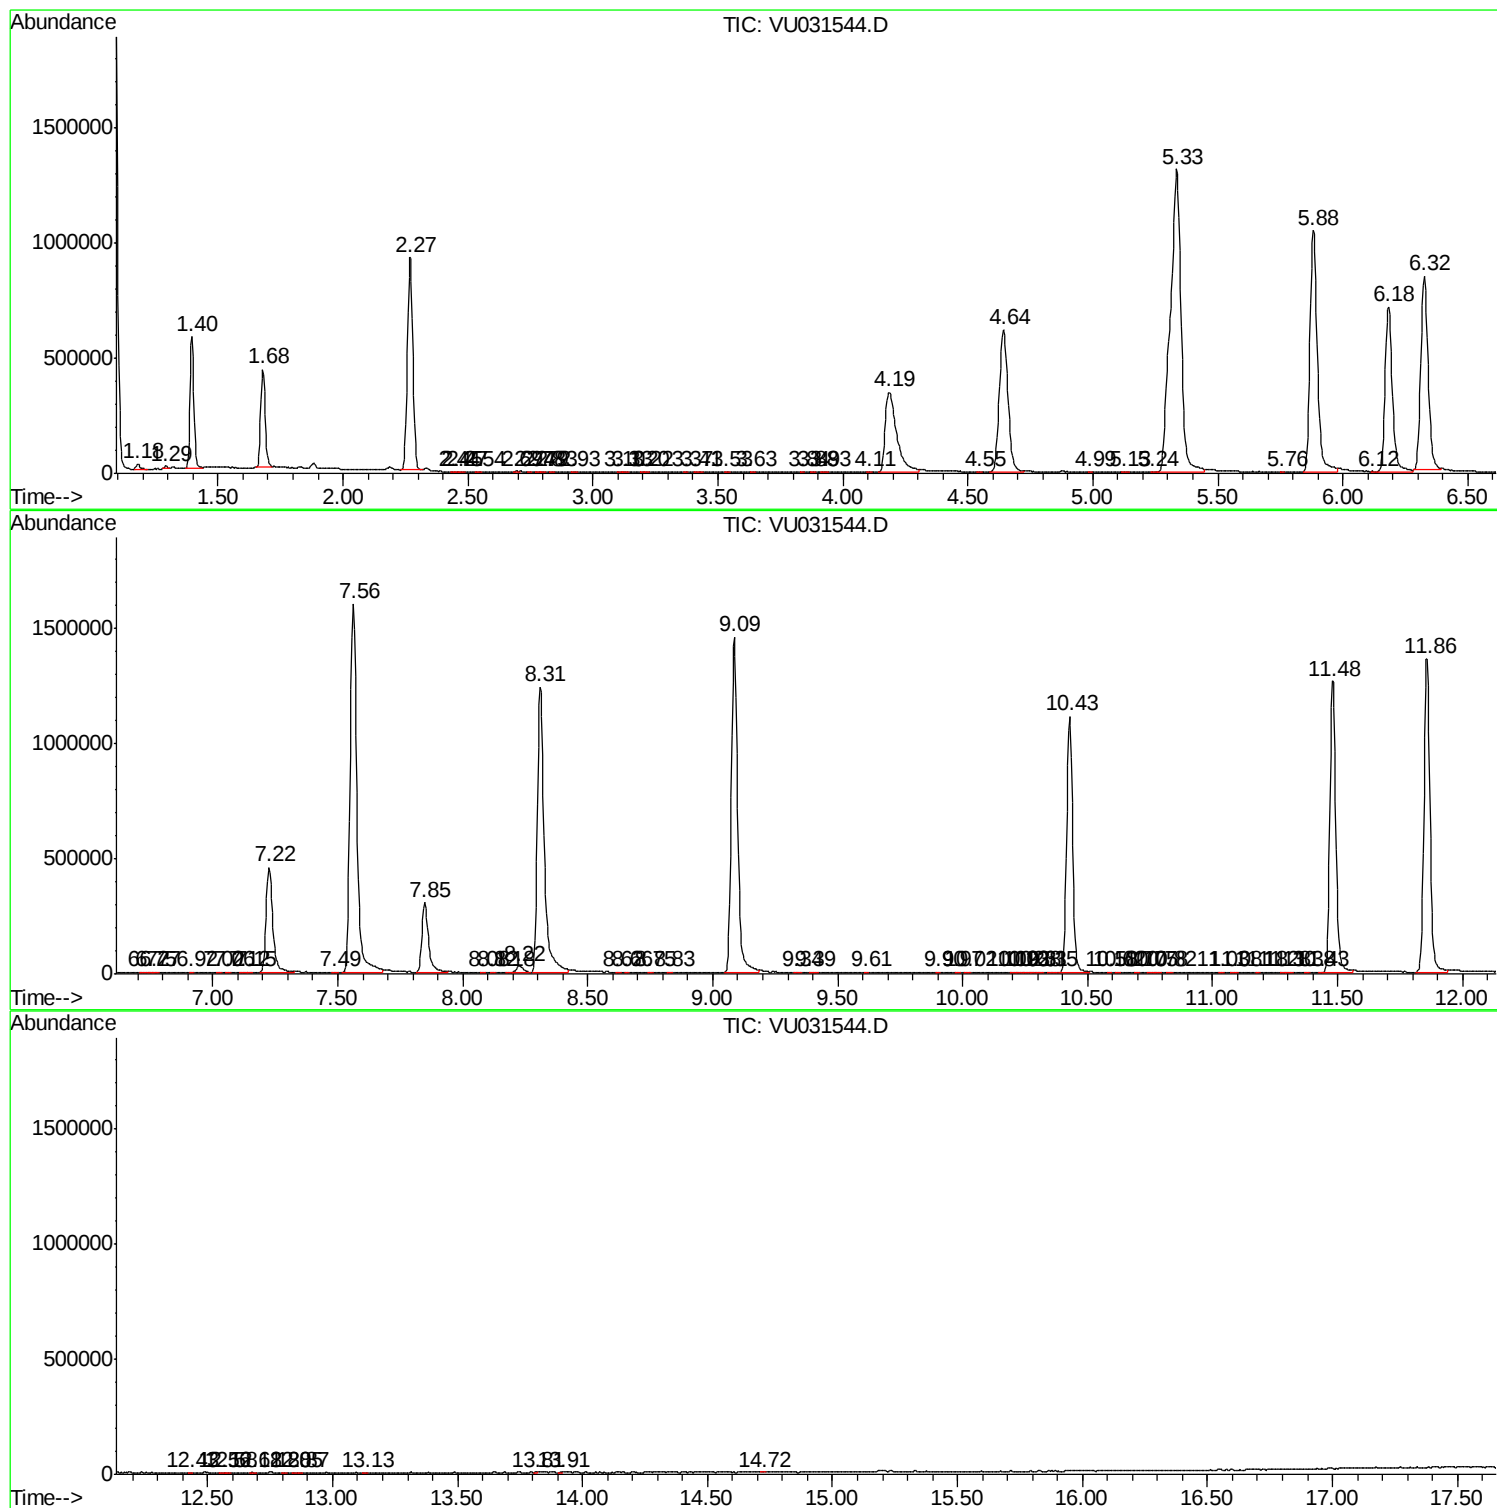

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031544.D
Acq On : 26 Apr 2019 19:59
Operator : JC/SP
Sample : K2536-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc