

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031547.D
 Acq On : 26 Apr 2019 21:56
 Operator : JC/SP
 Sample : K2536-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB2	22830	23127	0.61%	0.079%
2	1.396	87	95	108	rBV	531702	586500	15.47%	2.004%
3	1.678	176	183	200	rVB	424904	536079	14.14%	1.831%
4	2.183	336	340	348	rBV4	9943	12541	0.33%	0.043%
5	2.270	355	367	380	rBV	886805	1362981	35.96%	4.657%
6	2.469	426	429	436	rBV7	2344	2745	0.07%	0.009%
7	2.518	441	444	447	rBV5	1125	724	0.02%	0.002%
8	2.550	452	454	457	rBV2	1364	861	0.02%	0.003%
9	2.592	462	467	473	rVB4	2420	2720	0.07%	0.009%
10	2.691	494	498	499	rBV3	3151	1989	0.05%	0.007%
11	2.762	515	520	526	rVB5	1327	1497	0.04%	0.005%
12	2.791	526	529	534	rVB4	1304	1162	0.03%	0.004%
13	2.820	534	538	539	rBV3	1307	835	0.02%	0.003%
14	2.855	546	549	555	rVB5	1711	1492	0.04%	0.005%
15	2.887	555	559	563	rBV4	1190	914	0.02%	0.003%
16	2.968	577	584	585	rBV5	2055	1784	0.05%	0.006%
17	3.112	625	629	634	rBV3	861	901	0.02%	0.003%
18	3.215	659	661	665	rVB3	1369	809	0.02%	0.003%
19	3.254	670	673	676	rBV4	2027	1396	0.04%	0.005%
20	3.379	709	712	717	rVB3	1478	835	0.02%	0.003%
21	3.440	725	731	734	rBV2	1049	940	0.02%	0.003%
22	3.527	755	758	761	rBV	970	734	0.02%	0.003%
23	3.547	761	764	768	rVB6	1371	768	0.02%	0.003%
24	3.627	785	789	791	rBV3	1204	1065	0.03%	0.004%
25	3.643	791	794	798	rVV2	1126	839	0.02%	0.003%
26	3.675	802	804	807	rVB	1456	729	0.02%	0.002%
27	3.691	807	809	811	rBV2	1593	956	0.03%	0.003%
28	3.852	855	859	865	rBV2	1442	1342	0.04%	0.005%
29	3.881	865	868	871	rBV4	1113	763	0.02%	0.003%
30	4.055	918	922	927	rVV3	899	1048	0.03%	0.004%
31	4.141	944	949	951	rBV3	808	728	0.02%	0.002%
32	4.186	951	963	1003	rBV	336933	1102790	29.09%	3.768%
33	4.534	1068	1071	1074	rVB2	1665	923	0.02%	0.003%
34	4.643	1088	1105	1127	rBV	608231	1445313	38.13%	4.938%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031547.D
 Acq On : 26 Apr 2019 21:56
 Operator : JC/SP
 Sample : K2536-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.871	1173	1176	1179	rBV2	1576	1227	0.03%	0.004%
36	5.148	1257	1262	1266	rBV6	1242	1306	0.03%	0.004%
37	5.334	1297	1320	1345	rBV2	1277348	3790784	100.00%	12.951%
38	5.775	1454	1457	1461	rBV4	1259	984	0.03%	0.003%
39	5.810	1465	1468	1470	rBV	1193	780	0.02%	0.003%
40	5.881	1477	1490	1527	rBV	996627	2101797	55.44%	7.181%
41	6.183	1570	1584	1612	rBV	625766	1298093	34.24%	4.435%
42	6.325	1616	1628	1660	rVB	826797	1717685	45.31%	5.868%
43	6.550	1694	1698	1706	rVB6	3207	3570	0.09%	0.012%
44	6.585	1706	1709	1710	rBV2	1527	867	0.02%	0.003%
45	6.672	1734	1736	1743	rVV3	1264	1013	0.03%	0.003%
46	6.701	1743	1745	1750	rVB3	967	671	0.02%	0.002%
47	6.771	1762	1767	1770	rBV4	1605	1574	0.04%	0.005%
48	6.836	1783	1787	1791	rVB6	1504	1153	0.03%	0.004%
49	6.997	1833	1837	1841	rVB2	1546	1349	0.04%	0.005%
50	7.019	1841	1844	1850	rVB3	2462	1786	0.05%	0.006%
51	7.080	1861	1863	1869	rVB4	1305	936	0.02%	0.003%
52	7.225	1895	1908	1941	rBV2	444134	853572	22.52%	2.916%
53	7.431	1970	1972	1976	rBV4	1643	1164	0.03%	0.004%
54	7.479	1985	1987	1992	rVB3	1888	1432	0.04%	0.005%
55	7.562	2000	2013	2048	rBV	1545394	2893837	76.34%	9.887%
56	7.849	2091	2102	2129	rBV	294277	546176	14.41%	1.866%
57	8.151	2194	2196	2199	rBV2	1377	1022	0.03%	0.003%
58	8.225	2210	2219	2231	rBV6	20988	37877	1.00%	0.129%
59	8.312	2234	2246	2297	rBV	1173930	2334213	61.58%	7.975%
60	8.659	2351	2354	2359	rVB4	1052	894	0.02%	0.003%
61	8.826	2403	2406	2408	rBV4	1942	1280	0.03%	0.004%
62	8.858	2413	2416	2421	rVV6	1173	1138	0.03%	0.004%
63	8.884	2421	2424	2428	rVB4	1899	1523	0.04%	0.005%
64	8.968	2446	2450	2453	rBV4	1379	1177	0.03%	0.004%
65	9.025	2464	2468	2471	rBV3	1601	1365	0.04%	0.005%
66	9.087	2471	2487	2525	rBV	1402817	2515967	66.37%	8.596%
67	9.476	2603	2608	2613	rVB4	2150	2095	0.06%	0.007%
68	9.508	2613	2618	2619	rBV3	1251	919	0.02%	0.003%
69	9.533	2623	2626	2634	rVV7	1167	1722	0.05%	0.006%
70	9.614	2648	2651	2656	rVB4	2048	1585	0.04%	0.005%
71	9.765	2695	2698	2700	rBV3	1320	899	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031547.D
 Acq On : 26 Apr 2019 21:56
 Operator : JC/SP
 Sample : K2536-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.810	2709	2712	2717	rVB4	1193	1075	0.03%	0.004%
73	9.836	2717	2720	2724	rBV5	1518	1126	0.03%	0.004%
74	10.048	2783	2786	2792	rVB5	1345	1371	0.04%	0.005%
75	10.090	2796	2799	2802	rBV2	1098	707	0.02%	0.002%
76	10.218	2835	2839	2846	rVB6	1658	1843	0.05%	0.006%
77	10.427	2891	2904	2930	rVV	1089137	1762912	46.51%	6.023%
78	10.623	2960	2965	2967	rBV2	930	932	0.02%	0.003%
79	10.704	2988	2990	2994	rVB2	1490	909	0.02%	0.003%
80	10.723	2994	2996	2999	rBV3	893	737	0.02%	0.003%
81	10.868	3038	3041	3045	rVB2	1100	710	0.02%	0.002%
82	10.922	3056	3058	3065	rVB3	1045	919	0.02%	0.003%
83	11.016	3082	3087	3088	rBV	911	682	0.02%	0.002%
84	11.045	3092	3096	3101	rVB3	1267	1174	0.03%	0.004%
85	11.077	3101	3106	3107	rBV2	2152	1874	0.05%	0.006%
86	11.125	3118	3121	3127	rVB4	1583	1229	0.03%	0.004%
87	11.164	3131	3133	3136	rVB2	1485	690	0.02%	0.002%
88	11.295	3169	3174	3179	rBV6	1412	1600	0.04%	0.005%
89	11.418	3208	3212	3219	rBV6	1938	2949	0.08%	0.010%
90	11.482	3219	3232	3254	rBV	1225347	2020502	53.30%	6.903%
91	11.730	3306	3309	3311	rBV4	1757	1271	0.03%	0.004%
92	11.810	3331	3334	3335	rBV2	1899	1068	0.03%	0.004%
93	11.855	3336	3348	3373	rVV	1321787	2227179	58.75%	7.609%
94	12.279	3477	3480	3482	rBV2	1564	1164	0.03%	0.004%
95	12.447	3529	3532	3536	rBV4	1570	1537	0.04%	0.005%
96	12.890	3667	3670	3673	rVB2	2511	1542	0.04%	0.005%
97	13.479	3847	3853	3856	rBV3	2288	2618	0.07%	0.009%
98	13.688	3913	3918	3922	rBV5	1992	2117	0.06%	0.007%
99	13.742	3932	3935	3936	rBV2	1186	754	0.02%	0.003%
100	13.810	3954	3956	3959	rBV3	1484	1023	0.03%	0.003%


Sum of corrected areas: 29270476

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031547.D
Acq On : 26 Apr 2019 21:56
Operator : JC/SP
Sample : K2536-19 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

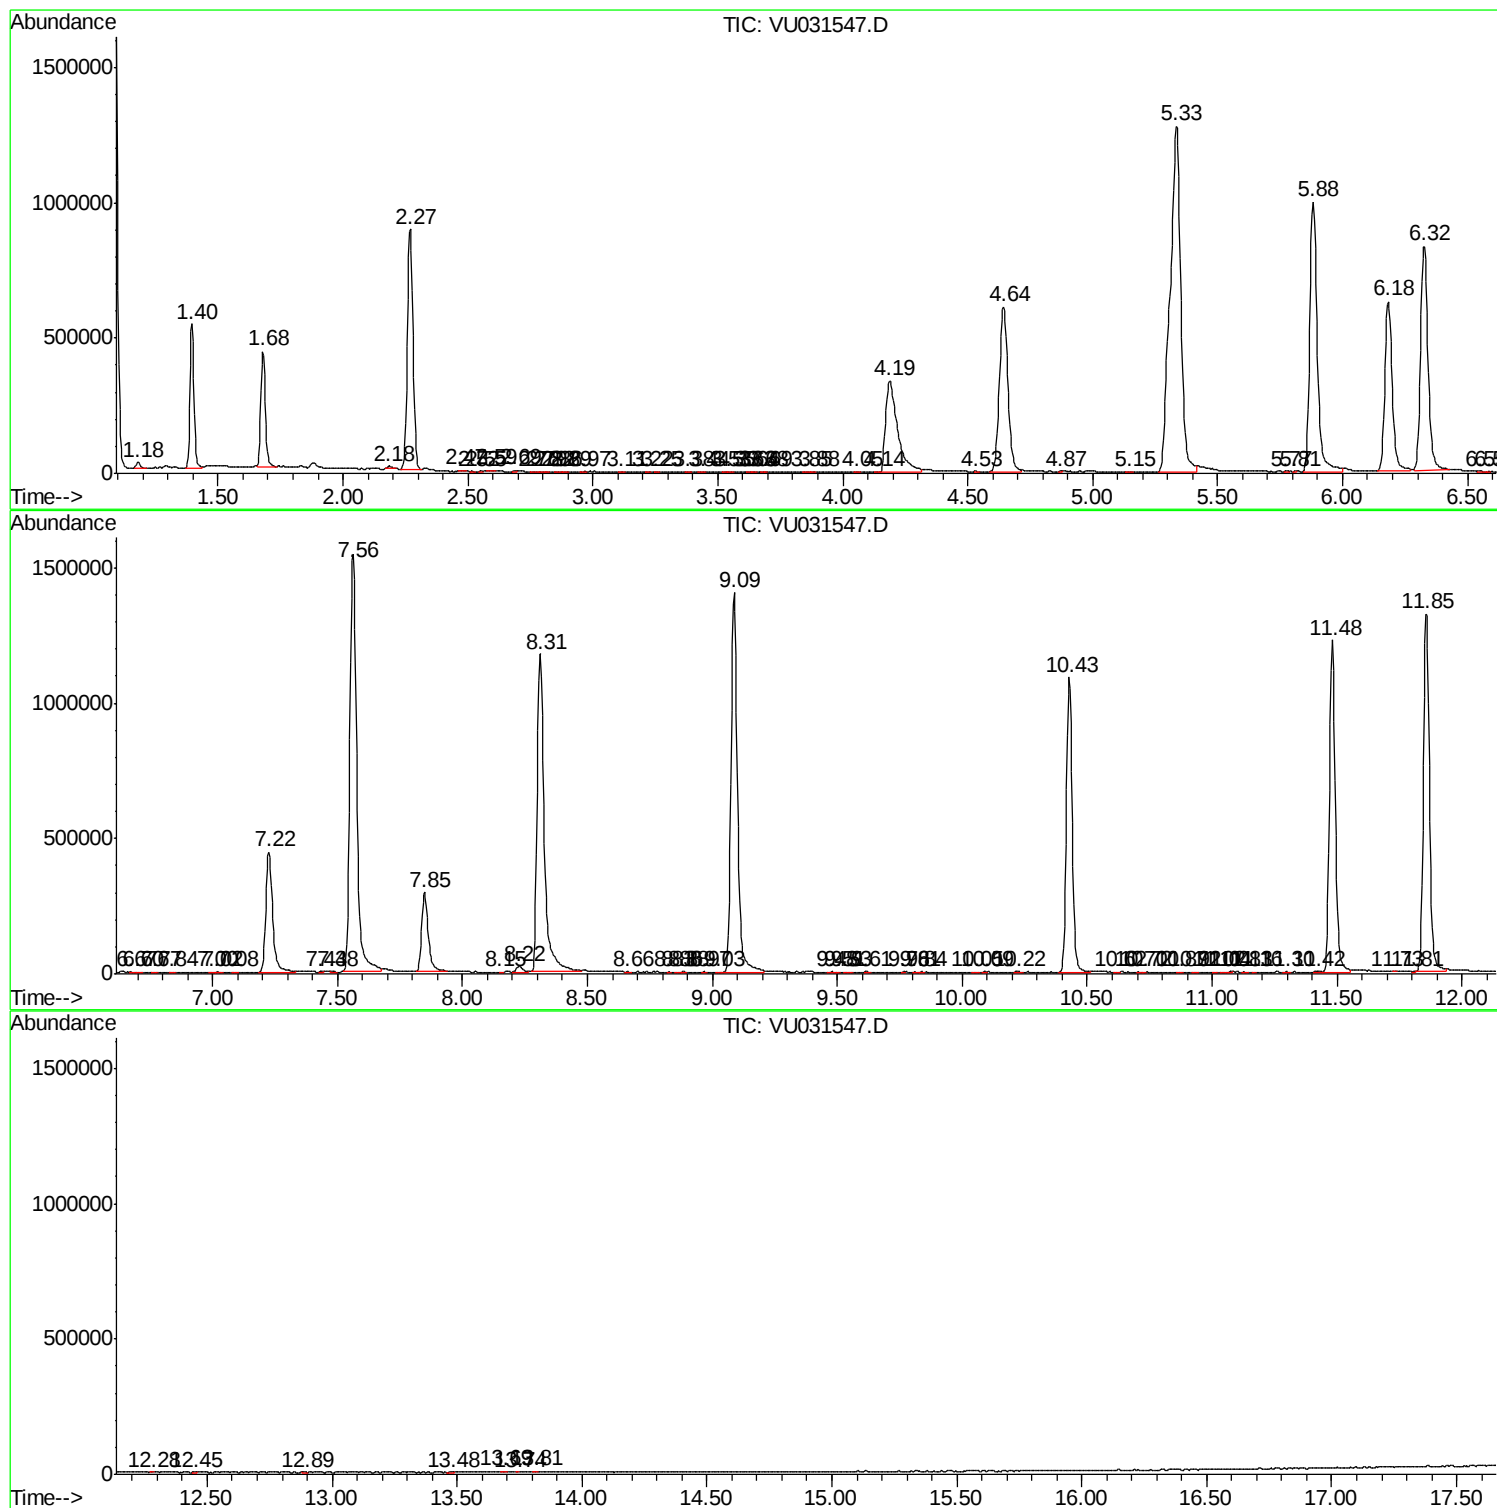

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031547.D
Acq On : 26 Apr 2019 21:56
Operator : JC/SP
Sample : K2536-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X07

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031547.D
Acq On : 26 Apr 2019 21:56
Operator : JC/SP
Sample : K2536-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X07

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
