

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031548.D
 Acq On : 26 Apr 2019 22:20
 Operator : JC/SP
 Sample : K2536-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB2	18989	16681	0.43%	0.060%
2	1.395	87	95	109	rBV	541311	589422	15.37%	2.110%
3	1.678	175	183	202	rVB	431100	527947	13.77%	1.890%
4	2.270	356	367	381	rVB	879051	1345890	35.10%	4.818%
5	2.418	411	413	418	rVB3	1464	1329	0.03%	0.005%
6	2.463	423	427	431	rBV6	1867	2362	0.06%	0.008%
7	2.524	443	446	447	rBV3	1761	890	0.02%	0.003%
8	2.659	483	488	494	rBV5	1566	1757	0.05%	0.006%
9	2.698	494	500	501	rBV4	3881	3966	0.10%	0.014%
10	2.823	535	539	542	rBV4	1479	1276	0.03%	0.005%
11	2.910	560	566	569	rBV4	1410	1602	0.04%	0.006%
12	3.022	597	601	604	rVB4	1284	1070	0.03%	0.004%
13	3.505	746	751	756	rVV6	1094	1006	0.03%	0.004%
14	3.582	772	775	778	rBV2	1020	808	0.02%	0.003%
15	3.691	805	809	813	rBV3	1156	1251	0.03%	0.004%
16	3.714	813	816	821	rVV3	831	830	0.02%	0.003%
17	3.890	865	871	879	rVB4	1406	1606	0.04%	0.006%
18	3.923	879	881	886	rBV3	1079	899	0.02%	0.003%
19	4.013	907	909	914	rVB2	1233	878	0.02%	0.003%
20	4.038	914	917	923	rBV4	1190	946	0.02%	0.003%
21	4.077	923	929	931	rBV5	985	1048	0.03%	0.004%
22	4.183	949	962	1007	rBV	358443	1097859	28.63%	3.930%
23	4.527	1065	1069	1072	rBV3	1589	1256	0.03%	0.004%
24	4.550	1073	1076	1079	rVV3	1356	844	0.02%	0.003%
25	4.643	1086	1105	1126	rBV	608994	1432124	37.35%	5.127%
26	4.829	1160	1163	1166	rBV4	1767	1640	0.04%	0.006%
27	4.887	1179	1181	1187	rVB4	2955	2567	0.07%	0.009%
28	4.932	1192	1195	1199	rVB3	1492	1278	0.03%	0.005%
29	4.968	1200	1206	1209	rBV5	1988	2424	0.06%	0.009%
30	4.990	1209	1213	1218	rVB6	1859	1958	0.05%	0.007%
31	5.035	1223	1227	1228	rBV2	1148	950	0.02%	0.003%
32	5.116	1248	1252	1258	rBV6	1367	1478	0.04%	0.005%
33	5.218	1281	1284	1288	rBV3	1293	954	0.02%	0.003%
34	5.334	1296	1320	1363	rBV2	1282516	3834784	100.00%	13.727%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031548.D
 Acq On : 26 Apr 2019 22:20
 Operator : JC/SP
 Sample : K2536-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.884	1476	1491	1531	rBV	1002184	2114857	55.15%	7.571%
36	6.180	1574	1583	1599	rVB9	12868	29596	0.77%	0.106%
37	6.324	1614	1628	1658	rBV	828800	1704658	44.45%	6.102%
38	6.595	1708	1712	1718	rVB6	2056	2676	0.07%	0.010%
39	6.633	1718	1724	1726	rBV5	1767	1963	0.05%	0.007%
40	6.672	1734	1736	1745	rVB6	1859	1833	0.05%	0.007%
41	6.723	1745	1752	1754	rBV5	1030	996	0.03%	0.004%
42	6.871	1793	1798	1800	rBV2	1615	1244	0.03%	0.004%
43	6.974	1826	1830	1836	rBV6	1275	1192	0.03%	0.004%
44	7.041	1847	1851	1856	rVB4	1719	1564	0.04%	0.006%
45	7.087	1856	1865	1868	rBV4	1433	2133	0.06%	0.008%
46	7.138	1877	1881	1885	rVB2	1286	925	0.02%	0.003%
47	7.225	1895	1908	1934	rBV	434207	831481	21.68%	2.976%
48	7.440	1972	1975	1977	rBV3	1406	885	0.02%	0.003%
49	7.562	1996	2013	2044	rBV	1535336	2892489	75.43%	10.354%
50	7.849	2092	2102	2131	rVV	292278	539545	14.07%	1.931%
51	8.016	2151	2154	2157	rBV3	1788	1128	0.03%	0.004%
52	8.173	2198	2203	2209	rBV7	2725	3658	0.10%	0.013%
53	8.247	2223	2226	2234	rVB6	1390	1717	0.04%	0.006%
54	8.308	2234	2245	2284	rBV	1218334	2336921	60.94%	8.365%
55	8.607	2335	2338	2342	rVV4	1402	1098	0.03%	0.004%
56	8.717	2368	2372	2376	rVB3	2062	1665	0.04%	0.006%
57	8.746	2376	2381	2383	rBV4	2099	1923	0.05%	0.007%
58	8.884	2418	2424	2425	rBV2	1238	973	0.03%	0.003%
59	8.945	2440	2443	2448	rBV4	1270	1125	0.03%	0.004%
60	8.971	2448	2451	2455	rBV3	1541	1082	0.03%	0.004%
61	9.086	2474	2487	2515	rBV	1431233	2497248	65.12%	8.939%
62	9.321	2555	2560	2565	rVB6	1620	1721	0.04%	0.006%
63	9.475	2604	2608	2611	rBV5	1330	1040	0.03%	0.004%
64	9.598	2643	2646	2649	rBV4	1225	1035	0.03%	0.004%
65	9.643	2655	2660	2663	rBV3	2010	1651	0.04%	0.006%
66	9.678	2667	2671	2672	rBV3	1494	1126	0.03%	0.004%
67	9.781	2698	2703	2705	rBV3	1522	1213	0.03%	0.004%
68	9.810	2706	2712	2715	rVV6	1336	1636	0.04%	0.006%
69	9.836	2715	2720	2723	rVV7	939	1005	0.03%	0.004%
70	9.987	2764	2767	2770	rVB2	1488	954	0.02%	0.003%
71	10.016	2772	2776	2781	rBV4	1012	1008	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031548.D
 Acq On : 26 Apr 2019 22:20
 Operator : JC/SP
 Sample : K2536-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X08

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.054	2784	2788	2791	rVV3	1215	1148	0.03%	0.004%
73	10.102	2799	2803	2806	rVB3	1024	806	0.02%	0.003%
74	10.138	2811	2814	2817	rBV2	1413	934	0.02%	0.003%
75	10.164	2818	2822	2823	rBV2	1512	973	0.03%	0.003%
76	10.209	2832	2836	2843	rBV4	1389	1551	0.04%	0.006%
77	10.321	2866	2871	2873	rBV3	1629	1347	0.04%	0.005%
78	10.334	2873	2875	2877	rVV2	1862	1151	0.03%	0.004%
79	10.350	2877	2880	2889	rVB5	2080	3232	0.08%	0.012%
80	10.427	2889	2904	2932	rBV	1085100	1763475	45.99%	6.313%
81	10.633	2964	2968	2971	rBV3	1213	1008	0.03%	0.004%
82	11.244	3154	3158	3160	rVV2	1512	987	0.03%	0.004%
83	11.270	3163	3166	3169	rVB2	1422	958	0.02%	0.003%
84	11.340	3185	3188	3193	rVB2	1094	837	0.02%	0.003%
85	11.408	3204	3209	3212	rBV4	1461	1458	0.04%	0.005%
86	11.479	3219	3231	3262	rBV	1218286	2040000	53.20%	7.303%
87	11.787	3324	3327	3334	rVB6	1542	1157	0.03%	0.004%
88	11.855	3334	3348	3374	rBV	1296414	2225089	58.02%	7.965%
89	12.524	3553	3556	3559	rBV2	1616	810	0.02%	0.003%
90	12.655	3593	3597	3600	rBV3	1238	1307	0.03%	0.005%
91	12.903	3671	3674	3676	rVB2	1753	975	0.03%	0.003%
92	12.922	3676	3680	3685	rBV5	1621	2051	0.05%	0.007%
93	13.003	3702	3705	3709	rBV2	1457	1389	0.04%	0.005%
94	13.758	3936	3940	3946	rBV4	1810	2059	0.05%	0.007%
95	13.929	3990	3993	3995	rBV3	1379	860	0.02%	0.003%
96	13.942	3995	3997	4000	rVV2	2001	1279	0.03%	0.005%
97	14.009	4015	4018	4021	rBV2	1533	1079	0.03%	0.004%
98	14.093	4041	4044	4046	rBV	1964	1461	0.04%	0.005%
99	14.176	4067	4070	4073	rVB	1886	1065	0.03%	0.004%
100	15.257	4403	4406	4411	rVB2	2753	2373	0.06%	0.008%


Sum of corrected areas: 27935363

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031548.D
Acq On : 26 Apr 2019 22:20
Operator : JC/SP
Sample : K2536-20 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X08

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

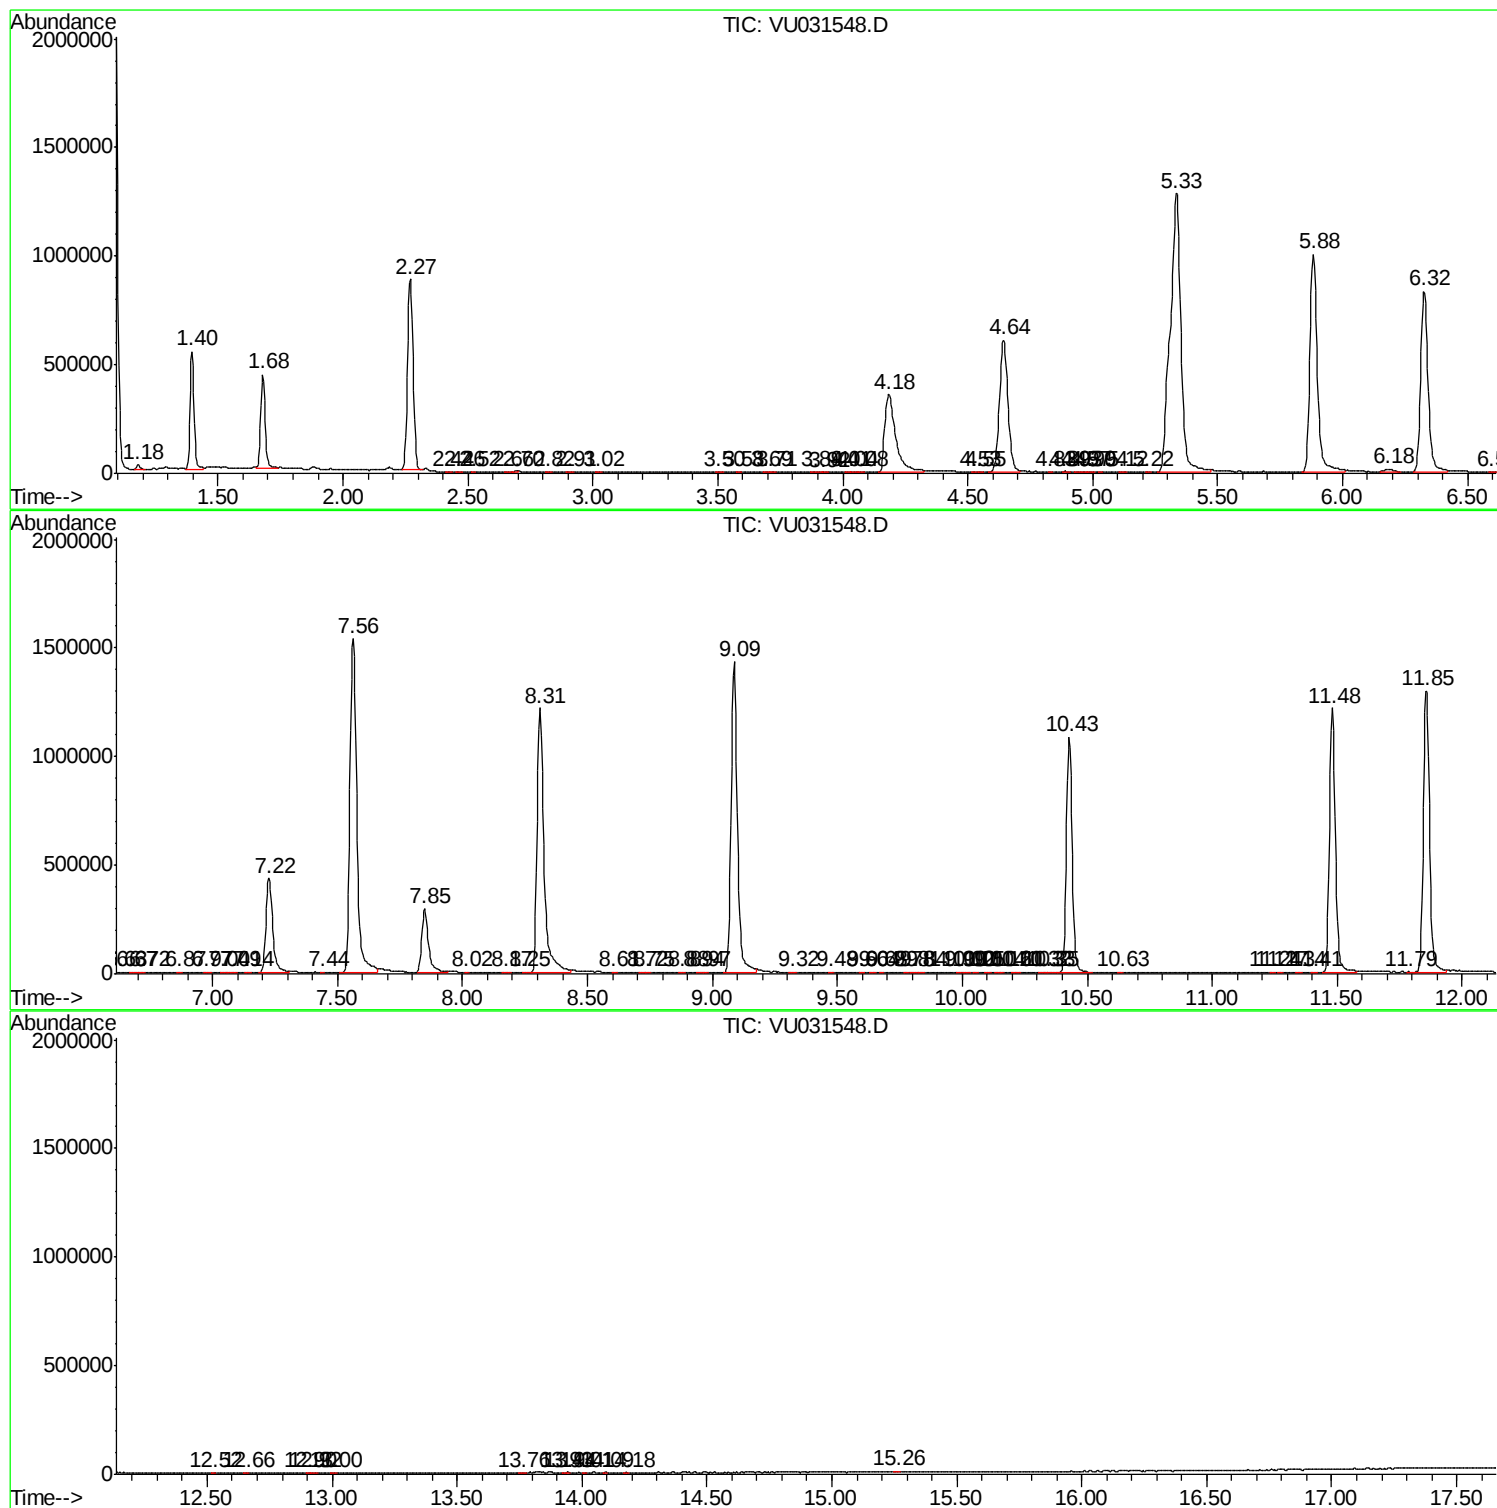

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031548.D
Acq On : 26 Apr 2019 22:20
Operator : JC/SP
Sample : K2536-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X08

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031548.D
Acq On : 26 Apr 2019 22:20
Operator : JC/SP
Sample : K2536-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X08

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc