

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031549.D
 Acq On : 26 Apr 2019 22:43
 Operator : JC/SP
 Sample : K2536-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB3	20183	19253	0.49%	0.067%
2	1.395	88	95	107	rBV	547800	583812	14.91%	2.043%
3	1.678	176	183	196	rVB	444081	542058	13.85%	1.897%
4	2.270	356	367	381	rVB	911371	1393084	35.58%	4.874%
5	2.463	423	427	428	rBV5	1788	1123	0.03%	0.004%
6	2.524	443	446	450	rVV4	1164	890	0.02%	0.003%
7	2.569	457	460	463	rBV3	1876	1216	0.03%	0.004%
8	2.707	492	503	512	rVB9	5276	9591	0.24%	0.034%
9	2.746	512	515	522	rBV7	1575	1874	0.05%	0.007%
10	2.829	536	541	543	rBV3	1066	1135	0.03%	0.004%
11	2.913	564	567	573	rVB4	1423	973	0.02%	0.003%
12	2.977	583	587	590	rBV3	1529	1074	0.03%	0.004%
13	3.006	591	596	598	rBV2	1364	956	0.02%	0.003%
14	3.051	608	610	615	rBV2	968	1019	0.03%	0.004%
15	3.212	657	660	665	rVV3	1657	1440	0.04%	0.005%
16	3.280	677	681	689	rBV3	2085	2918	0.07%	0.010%
17	3.373	706	710	717	rVB4	1505	2015	0.05%	0.007%
18	3.411	717	722	723	rBV2	1059	930	0.02%	0.003%
19	3.444	727	732	734	rBV	1164	902	0.02%	0.003%
20	3.492	741	747	752	rBV2	1122	997	0.03%	0.003%
21	3.736	820	823	830	rVB4	1101	1004	0.03%	0.004%
22	3.923	875	881	885	rBV4	973	1019	0.03%	0.004%
23	3.987	899	901	908	rVB4	1039	816	0.02%	0.003%
24	4.071	924	927	935	rBV3	1440	1439	0.04%	0.005%
25	4.119	937	942	944	rBV3	1015	794	0.02%	0.003%
26	4.190	951	964	998	rBV	333748	1069595	27.32%	3.743%
27	4.643	1087	1105	1139	rBV	624499	1489081	38.03%	5.210%
28	4.810	1154	1157	1160	rVB3	1681	986	0.03%	0.003%
29	4.842	1164	1167	1170	rVB4	1389	797	0.02%	0.003%
30	5.048	1226	1231	1233	rBV2	1247	1114	0.03%	0.004%
31	5.334	1296	1320	1355	rBV2	1294133	3915177	100.00%	13.699%
32	5.778	1455	1458	1462	rVB3	2772	1887	0.05%	0.007%
33	5.804	1462	1466	1471	rBV2	1385	1464	0.04%	0.005%
34	5.881	1475	1490	1523	rBV	1015006	2129151	54.38%	7.450%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031549.D
 Acq On : 26 Apr 2019 22:43
 Operator : JC/SP
 Sample : K2536-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.183	1572	1584	1604	rBV2	121325	258287	6.60%	0.904%
36	6.325	1614	1628	1663	rBV	845432	1760500	44.97%	6.160%
37	6.559	1698	1701	1704	rVB2	1696	1123	0.03%	0.004%
38	6.579	1704	1707	1714	rVB4	1422	1234	0.03%	0.004%
39	6.894	1802	1805	1807	rVV3	1336	1117	0.03%	0.004%
40	6.923	1810	1814	1817	rVV3	1974	1902	0.05%	0.007%
41	6.984	1830	1833	1839	rBV4	1305	1379	0.04%	0.005%
42	7.042	1846	1851	1853	rBV3	1541	1160	0.03%	0.004%
43	7.083	1858	1864	1867	rVB5	1274	1174	0.03%	0.004%
44	7.151	1883	1885	1891	rVB4	918	856	0.02%	0.003%
45	7.225	1896	1908	1933	rBV	452403	849103	21.69%	2.971%
46	7.370	1949	1953	1955	rBV3	1987	1403	0.04%	0.005%
47	7.562	2000	2013	2048	rBV	1560835	2936880	75.01%	10.276%
48	7.849	2091	2102	2125	rBV	295645	543896	13.89%	1.903%
49	8.038	2159	2161	2166	rBV5	1131	1021	0.03%	0.004%
50	8.125	2183	2188	2190	rBV6	1223	1140	0.03%	0.004%
51	8.180	2202	2205	2210	rVB4	2073	1612	0.04%	0.006%
52	8.228	2211	2220	2232	rVB10	9853	21743	0.56%	0.076%
53	8.308	2232	2245	2285	rBV	1202510	2363232	60.36%	8.269%
54	8.569	2322	2326	2330	rBV5	2376	2269	0.06%	0.008%
55	8.730	2372	2376	2380	rBV5	1399	1338	0.03%	0.005%
56	8.768	2385	2388	2391	rVB4	1552	1069	0.03%	0.004%
57	8.810	2399	2401	2407	rVB4	1229	900	0.02%	0.003%
58	8.935	2437	2440	2444	rBV2	1484	1503	0.04%	0.005%
59	9.009	2460	2463	2467	rVB3	2252	1777	0.05%	0.006%
60	9.032	2467	2470	2473	rBV3	1196	982	0.03%	0.003%
61	9.086	2473	2487	2517	rBV	1435985	2519754	64.36%	8.817%
62	9.337	2562	2565	2568	rBV5	1317	910	0.02%	0.003%
63	9.389	2579	2581	2588	rVB5	2012	2274	0.06%	0.008%
64	9.595	2642	2645	2648	rBV3	1644	1107	0.03%	0.004%
65	9.636	2655	2658	2662	rBV3	1119	1175	0.03%	0.004%
66	9.662	2663	2666	2670	rVV2	1132	984	0.03%	0.003%
67	9.726	2682	2686	2689	rBV4	1627	1412	0.04%	0.005%
68	9.900	2738	2740	2744	rVB2	1421	844	0.02%	0.003%
69	9.939	2749	2752	2756	rBV3	1682	1204	0.03%	0.004%
70	9.964	2756	2760	2763	rBV2	903	849	0.02%	0.003%
71	10.093	2796	2800	2803	rBV4	1733	1490	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031549.D
 Acq On : 26 Apr 2019 22:43
 Operator : JC/SP
 Sample : K2536-21 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.427	2891	2904	2924	rBV	1092751	1781145	45.49%	6.232%
73	10.546	2936	2941	2943	rVB2	1349	1052	0.03%	0.004%
74	10.562	2943	2946	2950	rBV4	1398	1107	0.03%	0.004%
75	10.643	2968	2971	2976	rBV3	1532	1400	0.04%	0.005%
76	10.697	2982	2988	2992	rVB5	1574	1718	0.04%	0.006%
77	10.733	2994	2999	3003	rBV5	1936	1798	0.05%	0.006%
78	10.858	3036	3038	3041	rBV3	1499	846	0.02%	0.003%
79	10.980	3072	3076	3079	rBV3	1410	1094	0.03%	0.004%
80	11.025	3087	3090	3092	rBV3	1093	850	0.02%	0.003%
81	11.077	3099	3106	3109	rBV5	1733	2027	0.05%	0.007%
82	11.138	3122	3125	3130	rBV4	1434	1176	0.03%	0.004%
83	11.250	3156	3160	3163	rBV3	1255	1205	0.03%	0.004%
84	11.289	3169	3172	3178	rBV4	1141	1101	0.03%	0.004%
85	11.344	3186	3189	3193	rBV2	1420	1013	0.03%	0.004%
86	11.418	3209	3212	3217	rVB5	1527	1008	0.03%	0.004%
87	11.479	3217	3231	3258	rBV	1246214	2053304	52.44%	7.185%
88	11.855	3336	3348	3371	rBV	1340431	2238403	57.17%	7.832%
89	12.395	3513	3516	3518	rBV3	1381	896	0.02%	0.003%
90	12.665	3597	3600	3604	rBV	1242	1352	0.03%	0.005%
91	12.749	3623	3626	3629	rVV4	1500	964	0.02%	0.003%
92	12.826	3644	3650	3653	rBV4	1902	1861	0.05%	0.007%
93	12.932	3680	3683	3685	rBV2	1236	798	0.02%	0.003%
94	13.260	3782	3785	3787	rBV3	1195	914	0.02%	0.003%
95	13.405	3825	3830	3833	rVB5	1514	1496	0.04%	0.005%
96	13.424	3833	3836	3842	rBV5	1585	1504	0.04%	0.005%
97	13.681	3913	3916	3920	rBV3	1409	1357	0.03%	0.005%
98	13.855	3967	3970	3972	rBV3	1892	1077	0.03%	0.004%
99	13.961	3998	4003	4009	rBV7	2574	3609	0.09%	0.013%
100	14.723	4238	4240	4244	rBV2	1455	1050	0.03%	0.004%


Sum of corrected areas: 28579312

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031549.D
Acq On : 26 Apr 2019 22:43
Operator : JC/SP
Sample : K2536-21 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

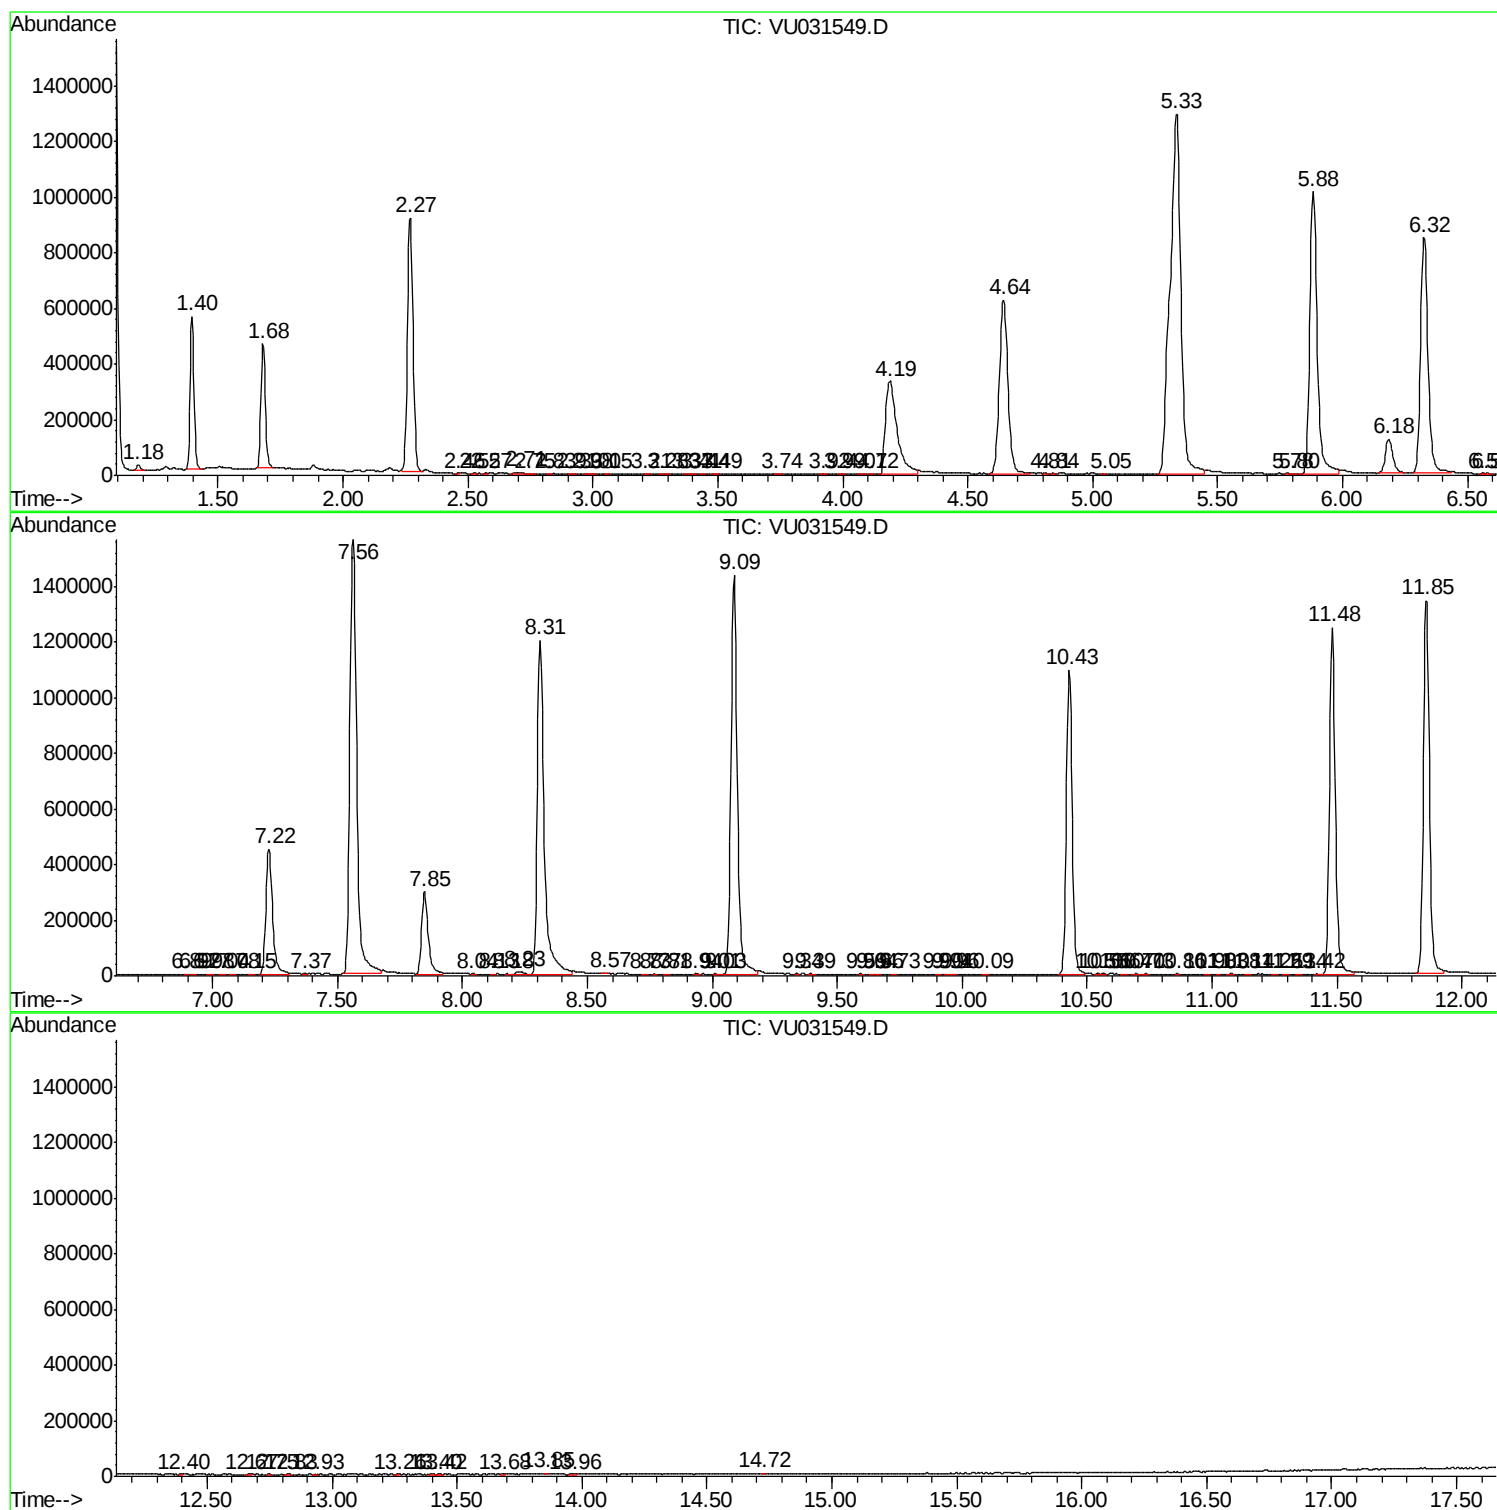

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031549.D
Acq On : 26 Apr 2019 22:43
Operator : JC/SP
Sample : K2536-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031549.D
Acq On : 26 Apr 2019 22:43
Operator : JC/SP
Sample : K2536-21 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc