

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031550.D
 Acq On : 26 Apr 2019 23:06
 Operator : JC/SP
 Sample : K2536-22 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	33	rBV2	20893	19926	0.53%	0.071%
2	1.396	88	95	107	rBV	531144	571916	15.10%	2.038%
3	1.679	176	183	196	rVB	424655	512511	13.53%	1.827%
4	1.884	242	247	255	rVB4	18889	22503	0.59%	0.080%
5	2.270	356	367	380	rVB	880091	1349218	35.61%	4.808%
6	2.691	491	498	501	rBV7	3442	4395	0.12%	0.016%
7	2.740	509	513	520	rBV7	1397	1648	0.04%	0.006%
8	2.785	523	527	530	rBV3	713	728	0.02%	0.003%
9	2.810	530	535	537	rBV3	1484	1113	0.03%	0.004%
10	2.913	563	567	571	rBV3	1994	1653	0.04%	0.006%
11	2.968	581	584	587	rBV3	1152	939	0.02%	0.003%
12	3.260	671	675	680	rBV4	952	1329	0.04%	0.005%
13	3.283	680	682	685	rVV2	1278	774	0.02%	0.003%
14	3.363	703	707	710	rBV3	1397	1269	0.03%	0.005%
15	3.383	710	713	718	rVB3	1159	988	0.03%	0.004%
16	3.466	736	739	744	rBV2	1677	1466	0.04%	0.005%
17	3.492	744	747	753	rVB4	1355	1364	0.04%	0.005%
18	3.585	770	776	779	rBV2	1522	1760	0.05%	0.006%
19	3.672	798	803	804	rBV4	840	730	0.02%	0.003%
20	3.752	825	828	834	rBV4	1132	912	0.02%	0.003%
21	3.897	867	873	878	rBV3	1683	1978	0.05%	0.007%
22	4.087	927	932	934	rBV2	1045	952	0.03%	0.003%
23	4.106	934	938	941	rBV3	1024	725	0.02%	0.003%
24	4.186	950	963	1005	rBV2	343695	1078204	28.46%	3.843%
25	4.572	1080	1083	1085	rBV4	1505	1100	0.03%	0.004%
26	4.643	1089	1105	1128	rVV2	604870	1436161	37.91%	5.118%
27	4.778	1144	1147	1150	rBV2	1926	1651	0.04%	0.006%
28	4.865	1169	1174	1175	rBV3	1151	984	0.03%	0.004%
29	4.984	1208	1211	1213	rBV3	909	688	0.02%	0.002%
30	5.000	1214	1216	1221	rVB4	2111	1261	0.03%	0.004%
31	5.055	1231	1233	1238	rVB5	917	716	0.02%	0.003%
32	5.129	1251	1256	1258	rBV3	1944	1531	0.04%	0.005%
33	5.145	1258	1261	1265	rVB3	1113	850	0.02%	0.003%
34	5.225	1282	1286	1290	rVB3	681	737	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031550.D
 Acq On : 26 Apr 2019 23:06
 Operator : JC/SP
 Sample : K2536-22 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1296	1320	1353	rBV2	1266176	3788754	100.00%	13.503%
36	5.775	1454	1457	1460	rVV4	1746	982	0.03%	0.003%
37	5.801	1463	1465	1469	rVB3	1699	891	0.02%	0.003%
38	5.881	1477	1490	1538	rBV	992863	2088385	55.12%	7.443%
39	6.183	1571	1584	1614	rBV2	197697	431745	11.40%	1.539%
40	6.328	1615	1629	1663	rVV	817548	1696803	44.79%	6.047%
41	6.762	1759	1764	1770	rVB5	1540	1471	0.04%	0.005%
42	6.862	1792	1795	1798	rVB2	1146	687	0.02%	0.002%
43	6.881	1798	1801	1804	rBV2	1375	990	0.03%	0.004%
44	7.022	1842	1845	1848	rBV3	1072	850	0.02%	0.003%
45	7.038	1848	1850	1854	rBV3	1502	897	0.02%	0.003%
46	7.170	1887	1891	1894	rBV4	1524	1192	0.03%	0.004%
47	7.225	1895	1908	1939	rBV	432907	819062	21.62%	2.919%
48	7.421	1966	1969	1970	rBV2	1406	840	0.02%	0.003%
49	7.563	1999	2013	2041	rBV	1514478	2821415	74.47%	10.055%
50	7.849	2091	2102	2132	rBV	280923	526945	13.91%	1.878%
51	8.138	2188	2192	2195	rVB4	1065	734	0.02%	0.003%
52	8.164	2195	2200	2205	rBV4	1384	1514	0.04%	0.005%
53	8.228	2210	2220	2234	rBV2	31501	55042	1.45%	0.196%
54	8.309	2234	2245	2293	rBV	1190949	2312201	61.03%	8.240%
55	8.794	2391	2396	2399	rBV4	2408	2545	0.07%	0.009%
56	9.087	2474	2487	2528	rBV	1405361	2488973	65.69%	8.870%
57	9.353	2566	2570	2573	rBV3	1301	1012	0.03%	0.004%
58	9.469	2604	2606	2612	rVB3	1120	803	0.02%	0.003%
59	9.514	2617	2620	2622	rBV3	1287	898	0.02%	0.003%
60	9.585	2638	2642	2644	rBV3	1103	782	0.02%	0.003%
61	9.636	2655	2658	2661	rVB3	1890	983	0.03%	0.004%
62	9.743	2687	2691	2693	rBV3	1577	1016	0.03%	0.004%
63	9.784	2700	2704	2705	rBV3	1721	1093	0.03%	0.004%
64	9.916	2742	2745	2747	rBV2	1283	817	0.02%	0.003%
65	9.974	2760	2763	2766	rVB2	1112	726	0.02%	0.003%
66	10.067	2788	2792	2797	rBV4	2066	1811	0.05%	0.006%
67	10.125	2807	2810	2813	rBV2	985	763	0.02%	0.003%
68	10.186	2826	2829	2830	rVV	1324	782	0.02%	0.003%
69	10.199	2830	2833	2838	rVV3	1656	1573	0.04%	0.006%
70	10.289	2858	2861	2866	rVB2	1083	1030	0.03%	0.004%
71	10.350	2876	2880	2883	rVB2	1705	1373	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031550.D
 Acq On : 26 Apr 2019 23:06
 Operator : JC/SP
 Sample : K2536-22 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X10

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.376	2883	2888	2889	rBV	944	694	0.02%	0.002%
73	10.427	2891	2904	2929	rBV	1072100	1736763	45.84%	6.190%
74	10.543	2937	2940	2945	rBV2	1416	1034	0.03%	0.004%
75	10.697	2984	2988	2991	rBV5	948	805	0.02%	0.003%
76	10.726	2994	2997	2999	rBV2	1148	713	0.02%	0.003%
77	10.990	3074	3079	3083	rVB4	1009	986	0.03%	0.004%
78	11.022	3083	3089	3090	rBV3	927	807	0.02%	0.003%
79	11.064	3099	3102	3106	rBV2	1062	685	0.02%	0.002%
80	11.083	3106	3108	3110	rBV2	1281	819	0.02%	0.003%
81	11.324	3180	3183	3188	rBV4	1229	1135	0.03%	0.004%
82	11.350	3188	3191	3193	rBV	1121	694	0.02%	0.002%
83	11.366	3193	3196	3201	rVB4	1021	883	0.02%	0.003%
84	11.479	3219	3231	3265	rBV	1200947	2014167	53.16%	7.178%
85	11.855	3336	3348	3369	rBV	1288107	2192154	57.86%	7.813%
86	12.357	3500	3504	3512	rBV9	2212	2737	0.07%	0.010%
87	12.646	3591	3594	3603	rVB5	1992	2498	0.07%	0.009%
88	12.685	3603	3606	3610	rBV2	1730	1287	0.03%	0.005%
89	12.996	3701	3703	3706	rBV2	1411	1030	0.03%	0.004%
90	13.199	3759	3766	3768	rBV4	1844	1922	0.05%	0.007%
91	13.395	3825	3827	3830	rVV2	1417	682	0.02%	0.002%
92	13.530	3865	3869	3873	rBV4	2113	1717	0.05%	0.006%
93	13.559	3876	3878	3883	rVV3	1376	981	0.03%	0.003%
94	13.601	3888	3891	3897	rVB2	1682	1734	0.05%	0.006%
95	13.646	3903	3905	3908	rBV	1259	1033	0.03%	0.004%
96	13.736	3931	3933	3937	rVB4	2582	1830	0.05%	0.007%
97	13.974	4004	4007	4008	rBV3	2072	1058	0.03%	0.004%
98	14.196	4071	4076	4080	rBV4	2347	2419	0.06%	0.009%
99	14.315	4110	4113	4115	rBV	2486	1542	0.04%	0.005%
100	14.852	4277	4280	4282	rBV3	2229	1671	0.04%	0.006%


Sum of corrected areas: 28059540

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031550.D
Acq On : 26 Apr 2019 23:06
Operator : JC/SP
Sample : K2536-22 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X10

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

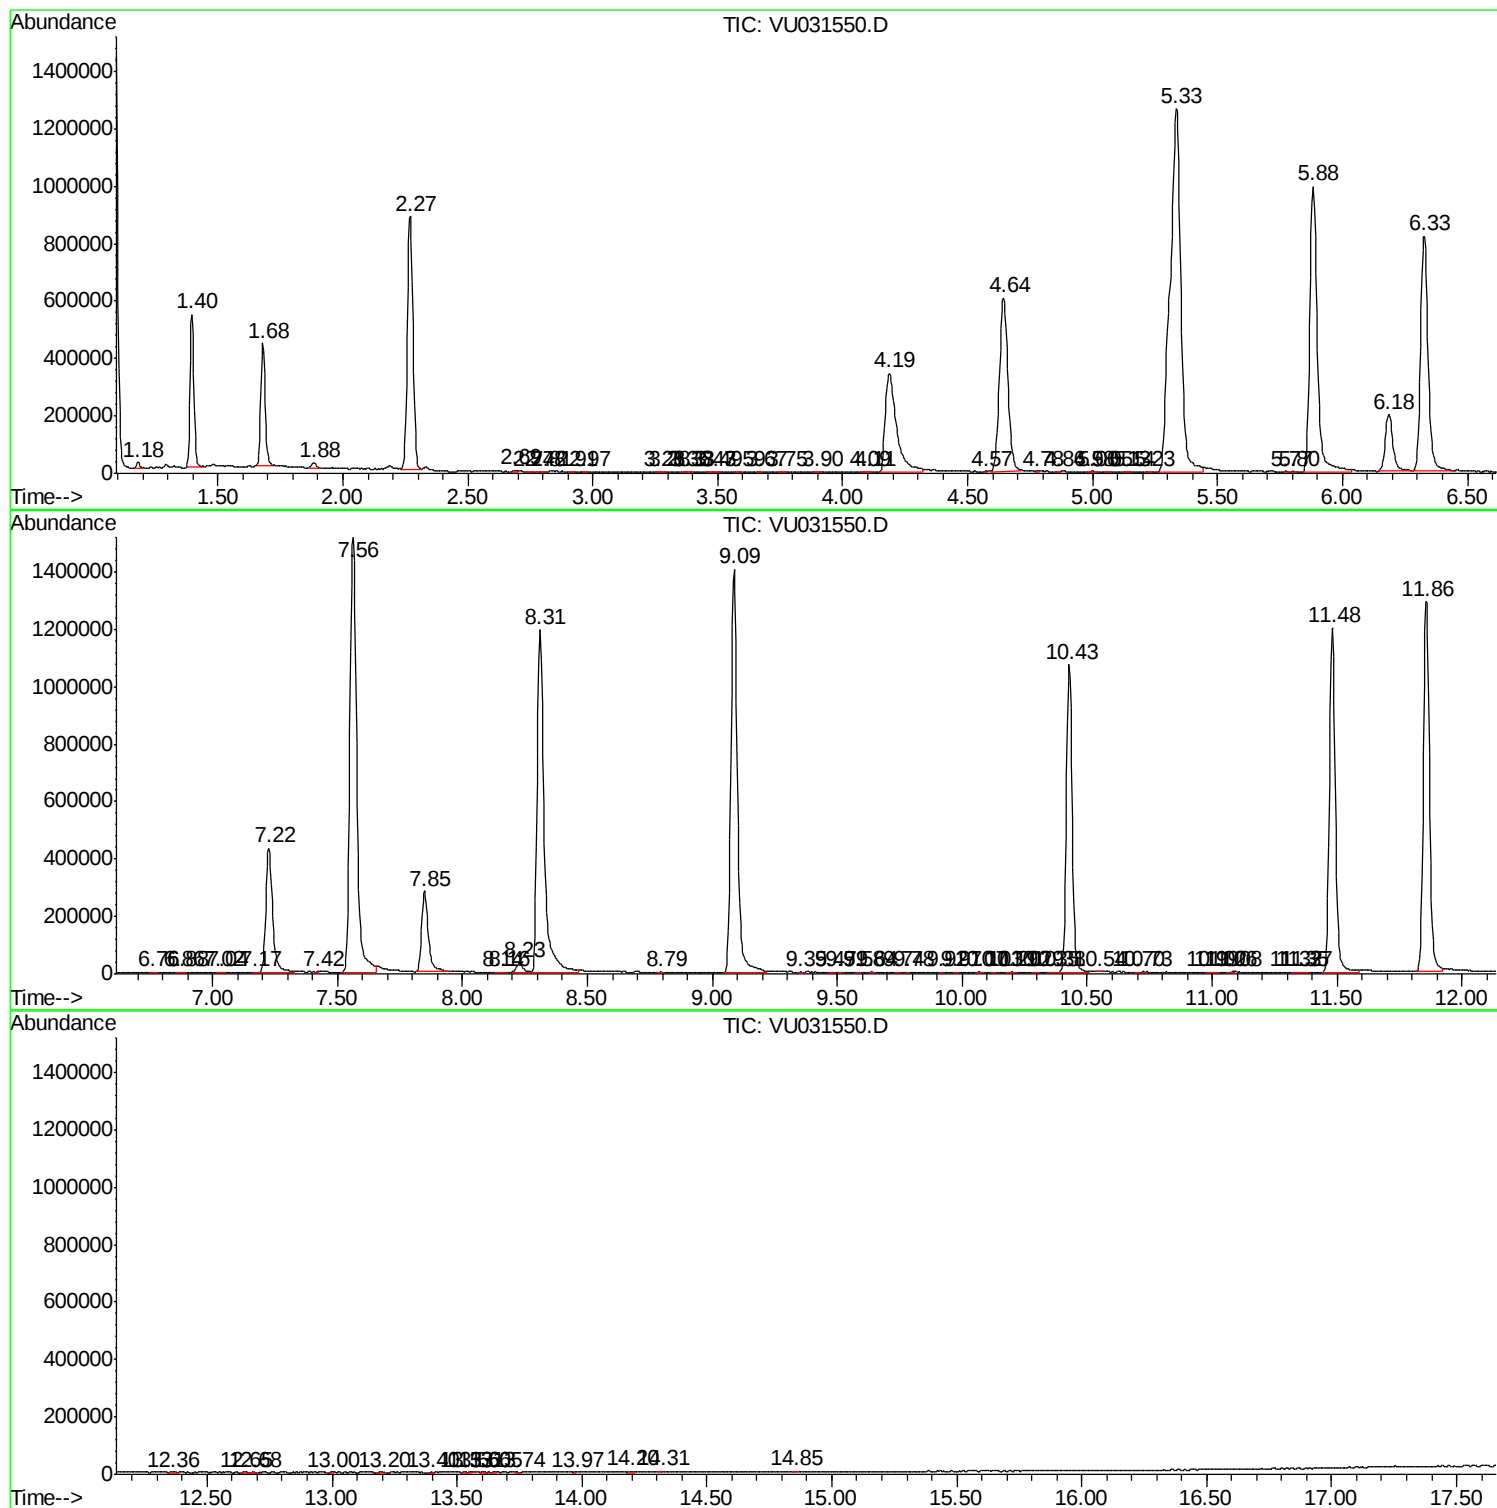

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031550.D
Acq On : 26 Apr 2019 23:06
Operator : JC/SP
Sample : K2536-22 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X10

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031550.D
Acq On : 26 Apr 2019 23:06
Operator : JC/SP
Sample : K2536-22 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X10

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc