

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031553.D
 Acq On : 27 Apr 2019 00:16
 Operator : JC/SP
 Sample : K2592-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rBV	18585	16344	0.43%	0.057%
2	1.395	88	95	109	rBV	539580	585557	15.27%	2.053%
3	1.678	176	183	196	rVB	414229	508285	13.26%	1.782%
4	2.270	356	367	380	rVB	897597	1357908	35.41%	4.760%
5	2.463	425	427	429	rBV3	1377	860	0.02%	0.003%
6	2.675	487	493	494	rBV2	1358	1282	0.03%	0.004%
7	2.701	495	501	507	rVB6	3973	5803	0.15%	0.020%
8	2.772	521	523	526	rVB2	1205	742	0.02%	0.003%
9	2.820	535	538	539	rBV2	1403	783	0.02%	0.003%
10	2.894	555	561	565	rVB6	934	813	0.02%	0.003%
11	2.987	587	590	591	rBV3	959	569	0.01%	0.002%
12	3.093	620	623	625	rBV3	1197	689	0.02%	0.002%
13	3.135	633	636	644	rBV3	1403	1869	0.05%	0.007%
14	3.170	644	647	649	rVV2	1423	900	0.02%	0.003%
15	3.186	649	652	659	rVV5	2141	2223	0.06%	0.008%
16	3.225	662	664	667	rVV3	1280	720	0.02%	0.003%
17	3.251	667	672	676	rVB4	910	792	0.02%	0.003%
18	3.286	680	683	690	rVV4	675	790	0.02%	0.003%
19	3.334	696	698	700	rBV	894	536	0.01%	0.002%
20	3.382	709	713	714	rBV2	1383	1000	0.03%	0.004%
21	3.431	722	728	732	rBV5	1686	1947	0.05%	0.007%
22	3.479	739	743	745	rBV2	941	628	0.02%	0.002%
23	3.553	763	766	767	rBV	929	572	0.01%	0.002%
24	3.694	808	810	815	rVB2	1685	1115	0.03%	0.004%
25	3.723	815	819	821	rBV3	1396	1241	0.03%	0.004%
26	3.945	886	888	890	rBV	918	574	0.01%	0.002%
27	3.997	901	904	906	rBV2	1364	981	0.03%	0.003%
28	4.054	918	922	924	rBV2	564	519	0.01%	0.002%
29	4.128	941	945	950	rBV5	1148	1218	0.03%	0.004%
30	4.183	950	962	1001	rBV	371213	1122494	29.27%	3.935%
31	4.553	1074	1077	1081	rBV3	2005	1610	0.04%	0.006%
32	4.575	1081	1084	1086	rVB4	2284	1365	0.04%	0.005%
33	4.643	1086	1105	1130	rBV	618183	1464278	38.19%	5.133%
34	4.807	1151	1156	1163	rBV7	2153	2428	0.06%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031553.D
 Acq On : 27 Apr 2019 00:16
 Operator : JC/SP
 Sample : K2592-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.958	1200	1203	1205	rBV3	1141	759	0.02%	0.003%
36	5.196	1275	1277	1281	rVB3	1201	697	0.02%	0.002%
37	5.228	1285	1287	1290	rBV	1396	1016	0.03%	0.004%
38	5.334	1295	1320	1351	rBV2	1267535	3834342	100.00%	13.440%
39	5.726	1439	1442	1444	rBV3	1633	895	0.02%	0.003%
40	5.791	1459	1462	1467	rBV4	1342	1285	0.03%	0.005%
41	5.881	1476	1490	1517	rBV	990648	2042891	53.28%	7.161%
42	6.183	1571	1584	1612	rBV	319855	674172	17.58%	2.363%
43	6.328	1615	1629	1663	rVB	838158	1725109	44.99%	6.047%
44	6.675	1735	1737	1745	rVB7	1881	1387	0.04%	0.005%
45	6.710	1745	1748	1754	rVB3	1771	1726	0.05%	0.006%
46	6.736	1754	1756	1757	rBV	1253	524	0.01%	0.002%
47	6.746	1757	1759	1762	rVV2	1180	729	0.02%	0.003%
48	6.775	1765	1768	1772	rBV2	1199	998	0.03%	0.003%
49	6.839	1785	1788	1795	rBV4	1529	1639	0.04%	0.006%
50	6.890	1801	1804	1808	rBV4	1146	1019	0.03%	0.004%
51	6.945	1819	1821	1824	rBV2	814	555	0.01%	0.002%
52	7.061	1853	1857	1859	rBV3	2717	2356	0.06%	0.008%
53	7.225	1896	1908	1931	rBV	434887	819565	21.37%	2.873%
54	7.562	1999	2013	2061	rBV	1547741	2895827	75.52%	10.151%
55	7.848	2091	2102	2126	rBV	285812	521990	13.61%	1.830%
56	8.225	2210	2219	2234	rBV5	22041	42441	1.11%	0.149%
57	8.308	2234	2245	2291	rBV	1223485	2391445	62.37%	8.383%
58	8.713	2369	2371	2379	rVB5	1355	1380	0.04%	0.005%
59	8.807	2398	2400	2403	rBV3	1472	936	0.02%	0.003%
60	8.868	2417	2419	2425	rBV4	1093	953	0.02%	0.003%
61	8.980	2450	2454	2455	rBV2	1697	1099	0.03%	0.004%
62	9.086	2474	2487	2527	rBV	1403969	2489745	64.93%	8.727%
63	9.302	2552	2554	2558	rBV4	1682	1137	0.03%	0.004%
64	9.434	2592	2595	2596	rBV3	952	549	0.01%	0.002%
65	9.517	2617	2621	2624	rBV2	1047	997	0.03%	0.003%
66	9.533	2624	2626	2630	rVV3	798	644	0.02%	0.002%
67	9.601	2645	2647	2651	rBV2	1042	656	0.02%	0.002%
68	9.627	2651	2655	2658	rBV3	1048	782	0.02%	0.003%
69	9.662	2662	2666	2667	rBV2	1526	930	0.02%	0.003%
70	9.729	2682	2687	2689	rBV2	1739	1577	0.04%	0.006%
71	9.768	2696	2699	2703	rBV2	1449	1089	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031553.D
 Acq On : 27 Apr 2019 00:16
 Operator : JC/SP
 Sample : K2592-06 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.861	2724	2728	2730	rBV2	1361	1076	0.03%	0.004%
73	9.900	2737	2740	2744	rBV2	1185	880	0.02%	0.003%
74	9.942	2749	2753	2756	rBV3	1355	992	0.03%	0.003%
75	10.035	2780	2782	2785	rBV5	767	547	0.01%	0.002%
76	10.151	2814	2818	2822	rVB3	1745	1412	0.04%	0.005%
77	10.189	2822	2830	2834	rBV4	2085	2153	0.06%	0.008%
78	10.225	2839	2841	2844	rVV	1089	615	0.02%	0.002%
79	10.324	2866	2872	2873	rBV3	1562	1343	0.04%	0.005%
80	10.363	2882	2884	2888	rVB2	1299	736	0.02%	0.003%
81	10.427	2888	2904	2931	rBV	1089316	1777021	46.34%	6.229%
82	10.749	3001	3004	3006	rBV3	1294	710	0.02%	0.002%
83	10.794	3016	3018	3021	rVB3	1191	669	0.02%	0.002%
84	10.813	3021	3024	3026	rBV2	917	701	0.02%	0.002%
85	10.839	3029	3032	3037	rVB2	1989	1701	0.04%	0.006%
86	10.868	3038	3041	3043	rBV3	1082	551	0.01%	0.002%
87	10.926	3056	3059	3062	rVB2	1556	1042	0.03%	0.004%
88	10.945	3062	3065	3067	rBV2	1309	896	0.02%	0.003%
89	11.215	3147	3149	3151	rBV3	1322	795	0.02%	0.003%
90	11.369	3195	3197	3200	rVB2	1714	944	0.02%	0.003%
91	11.401	3204	3207	3211	rBV3	1394	1349	0.04%	0.005%
92	11.482	3220	3232	3263	rBV	1199035	1972846	51.45%	6.915%
93	11.858	3336	3349	3384	rBV	1292703	2196500	57.28%	7.699%
94	12.212	3457	3459	3466	rVB5	2035	1623	0.04%	0.006%
95	12.771	3630	3633	3637	rBV3	1351	1254	0.03%	0.004%
96	13.028	3711	3713	3715	rBV2	1397	667	0.02%	0.002%
97	13.324	3802	3805	3811	rBV2	1535	1867	0.05%	0.007%
98	13.440	3838	3841	3842	rBV3	1039	625	0.02%	0.002%
99	13.697	3919	3921	3924	rVB	1592	793	0.02%	0.003%
100	14.411	4140	4143	4145	rBV2	2003	1245	0.03%	0.004%


Sum of corrected areas: 28528829

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031553.D
Acq On : 27 Apr 2019 00:16
Operator : JC/SP
Sample : K2592-06 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COWZ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

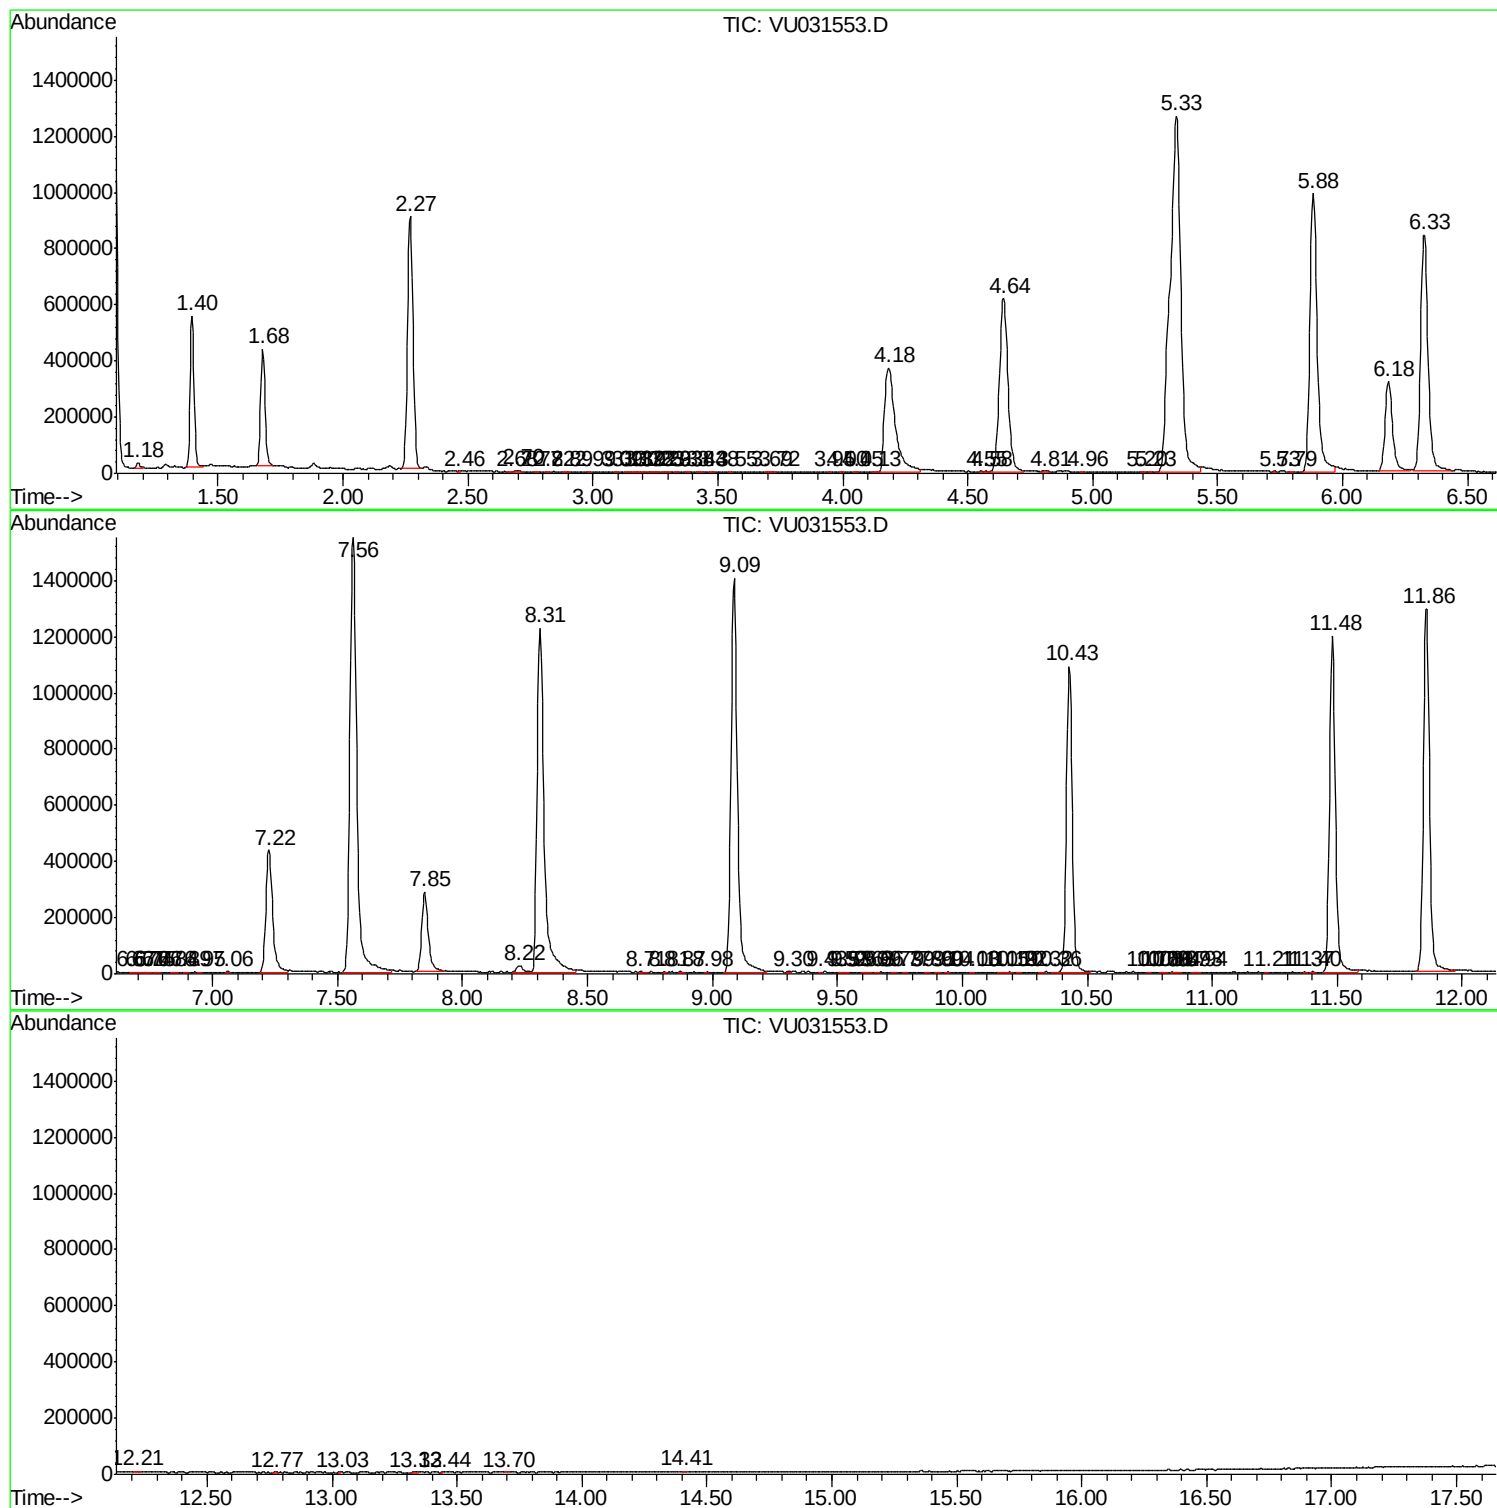

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031553.D
Acq On : 27 Apr 2019 00:16
Operator : JC/SP
Sample : K2592-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031553.D
Acq On : 27 Apr 2019 00:16
Operator : JC/SP
Sample : K2592-06 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
