

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031554.D
 Acq On : 27 Apr 2019 00:39
 Operator : JC/SP
 Sample : K2592-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB2	21211	21995	0.57%	0.077%
2	1.396	88	95	110	rBV	557562	600232	15.61%	2.098%
3	1.679	175	183	195	rBV	424930	535611	13.93%	1.872%
4	2.267	356	366	381	rVB	897866	1389886	36.16%	4.859%
5	2.511	438	442	447	rVB4	2042	1722	0.04%	0.006%
6	2.752	514	517	519	rBV2	1046	753	0.02%	0.003%
7	2.804	530	533	536	rBV5	1948	1586	0.04%	0.006%
8	2.894	557	561	565	rBV4	1124	944	0.02%	0.003%
9	2.942	574	576	580	rVB3	1212	724	0.02%	0.003%
10	2.965	580	583	586	rBV3	1051	913	0.02%	0.003%
11	2.984	586	589	592	rVB3	1635	1009	0.03%	0.004%
12	3.003	592	595	597	rBV2	1195	680	0.02%	0.002%
13	3.055	608	611	613	rBV4	1330	670	0.02%	0.002%
14	3.103	622	626	630	rBV3	1260	1040	0.03%	0.004%
15	3.174	643	648	652	rBV4	1717	1674	0.04%	0.006%
16	3.196	652	655	658	rVB3	1185	688	0.02%	0.002%
17	3.215	658	661	664	rBV2	924	604	0.02%	0.002%
18	3.244	664	670	674	rBV4	1582	1607	0.04%	0.006%
19	3.457	732	736	741	rVB4	1574	1364	0.04%	0.005%
20	3.498	745	749	752	rVB2	1278	914	0.02%	0.003%
21	3.518	752	755	760	rBV4	1788	1476	0.04%	0.005%
22	3.624	780	788	792	rVB4	1376	1785	0.05%	0.006%
23	3.646	792	795	798	rBV2	1428	1194	0.03%	0.004%
24	3.772	827	834	837	rBV3	1038	1517	0.04%	0.005%
25	3.878	862	867	872	rVB3	1078	941	0.02%	0.003%
26	3.923	879	881	884	rVB	1995	1092	0.03%	0.004%
27	3.942	884	887	889	rBV	1369	820	0.02%	0.003%
28	3.997	899	904	910	rBV4	1245	1356	0.04%	0.005%
29	4.061	922	924	931	rBV3	1235	1098	0.03%	0.004%
30	4.100	931	936	937	rBV	824	693	0.02%	0.002%
31	4.113	938	940	945	rVB3	1435	1023	0.03%	0.004%
32	4.186	950	963	1005	rBV	350003	1117220	29.06%	3.906%
33	4.569	1080	1082	1087	rVB3	1106	652	0.02%	0.002%
34	4.643	1087	1105	1137	rBV	620471	1479762	38.49%	5.173%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031554.D
 Acq On : 27 Apr 2019 00:39
 Operator : JC/SP
 Sample : K2592-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.846	1165	1168	1172	rVB3	1686	1132	0.03%	0.004%
36	4.981	1206	1210	1211	rBV3	1778	1160	0.03%	0.004%
37	5.045	1227	1230	1232	rBV2	1291	760	0.02%	0.003%
38	5.112	1247	1251	1258	rBV7	1227	966	0.03%	0.003%
39	5.248	1291	1293	1296	rVB	1096	643	0.02%	0.002%
40	5.334	1296	1320	1345	rBV2	1289130	3844139	100.00%	13.438%
41	5.781	1457	1459	1464	rVB3	1126	755	0.02%	0.003%
42	5.813	1467	1469	1474	rVB3	1561	1073	0.03%	0.004%
43	5.881	1477	1490	1540	rBV	993468	2090857	54.39%	7.309%
44	6.183	1570	1584	1611	rBV	304930	640680	16.67%	2.240%
45	6.325	1615	1628	1666	rVB	840621	1738049	45.21%	6.076%
46	6.608	1714	1716	1718	rVB2	1331	610	0.02%	0.002%
47	6.624	1718	1721	1724	rBV3	1718	894	0.02%	0.003%
48	6.704	1743	1746	1750	rVB2	1121	573	0.01%	0.002%
49	6.736	1754	1756	1760	rVB2	1270	774	0.02%	0.003%
50	6.759	1760	1763	1767	rBV3	1235	992	0.03%	0.003%
51	6.794	1770	1774	1777	rBV3	1015	725	0.02%	0.003%
52	6.813	1777	1780	1783	rBV	1073	717	0.02%	0.003%
53	6.897	1797	1806	1808	rBV5	2339	2632	0.07%	0.009%
54	6.939	1816	1819	1821	rBV2	1376	955	0.02%	0.003%
55	6.968	1824	1828	1832	rVB4	1523	1245	0.03%	0.004%
56	6.987	1832	1834	1837	rBV2	1024	604	0.02%	0.002%
57	7.225	1894	1908	1932	rBV2	432613	829296	21.57%	2.899%
58	7.424	1967	1970	1973	rVB4	1583	972	0.03%	0.003%
59	7.444	1973	1976	1978	rBV2	1017	841	0.02%	0.003%
60	7.563	2000	2013	2055	rBV	1551949	2915303	75.84%	10.191%
61	7.849	2091	2102	2137	rBV	286108	535495	13.93%	1.872%
62	8.157	2195	2198	2201	rBV4	1081	977	0.03%	0.003%
63	8.228	2210	2220	2229	rBV4	24523	41461	1.08%	0.145%
64	8.309	2233	2245	2286	rBV	1196342	2356353	61.30%	8.237%
65	8.736	2376	2378	2383	rBV5	1256	824	0.02%	0.003%
66	8.794	2392	2396	2400	rBV4	1696	1701	0.04%	0.006%
67	8.833	2403	2408	2412	rBV2	2558	3027	0.08%	0.011%
68	8.923	2433	2436	2438	rBV3	1998	1132	0.03%	0.004%
69	8.961	2442	2448	2450	rBV4	1368	1574	0.04%	0.006%
70	8.990	2455	2457	2461	rVB3	1451	859	0.02%	0.003%
71	9.087	2474	2487	2514	rBV	1414700	2466214	64.16%	8.621%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031554.D
 Acq On : 27 Apr 2019 00:39
 Operator : JC/SP
 Sample : K2592-07 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.334	2562	2564	2566	rBV3	1418	879	0.02%	0.003%
73	9.379	2573	2578	2581	rVB4	1967	1495	0.04%	0.005%
74	9.466	2600	2605	2607	rBV4	1685	1476	0.04%	0.005%
75	9.582	2635	2641	2643	rBV5	841	983	0.03%	0.003%
76	9.617	2649	2652	2654	rBV3	1302	720	0.02%	0.003%
77	9.919	2744	2746	2750	rBV	1455	878	0.02%	0.003%
78	9.990	2766	2768	2771	rVB2	1058	614	0.02%	0.002%
79	10.090	2796	2799	2806	rVB5	1419	1633	0.04%	0.006%
80	10.257	2849	2851	2855	rBV5	828	653	0.02%	0.002%
81	10.341	2874	2877	2881	rBV4	1310	1128	0.03%	0.004%
82	10.366	2882	2885	2886	rBV	1090	678	0.02%	0.002%
83	10.427	2892	2904	2932	rBV	1086904	1762349	45.85%	6.161%
84	10.662	2970	2977	2979	rBV6	1509	2095	0.05%	0.007%
85	10.730	2994	2998	3000	rBV2	1629	1125	0.03%	0.004%
86	10.868	3038	3041	3044	rVB2	1983	1184	0.03%	0.004%
87	11.048	3093	3097	3099	rVB3	1094	744	0.02%	0.003%
88	11.067	3099	3103	3105	rBV2	1467	1133	0.03%	0.004%
89	11.080	3105	3107	3112	rVV4	1692	1377	0.04%	0.005%
90	11.180	3135	3138	3143	rVB4	1500	1338	0.03%	0.005%
91	11.479	3219	3231	3256	rBV	1181856	1956574	50.90%	6.840%
92	11.855	3336	3348	3373	rBV	1309090	2192855	57.04%	7.666%
93	12.453	3531	3534	3535	rBV2	1363	730	0.02%	0.003%
94	12.720	3615	3617	3620	rVB3	2066	1141	0.03%	0.004%
95	12.742	3621	3624	3629	rVV4	1456	1269	0.03%	0.004%
96	12.797	3635	3641	3645	rBV5	1641	2153	0.06%	0.008%
97	13.286	3790	3793	3797	rBV3	2043	2039	0.05%	0.007%
98	13.350	3810	3813	3816	rBV2	1866	1301	0.03%	0.005%
99	13.640	3900	3903	3906	rBV4	2026	1614	0.04%	0.006%
100	13.717	3924	3927	3929	rBV3	1821	1346	0.04%	0.005%


Sum of corrected areas: 28605713

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031554.D
Acq On : 27 Apr 2019 00:39
Operator : JC/SP
Sample : K2592-07 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COWZ8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

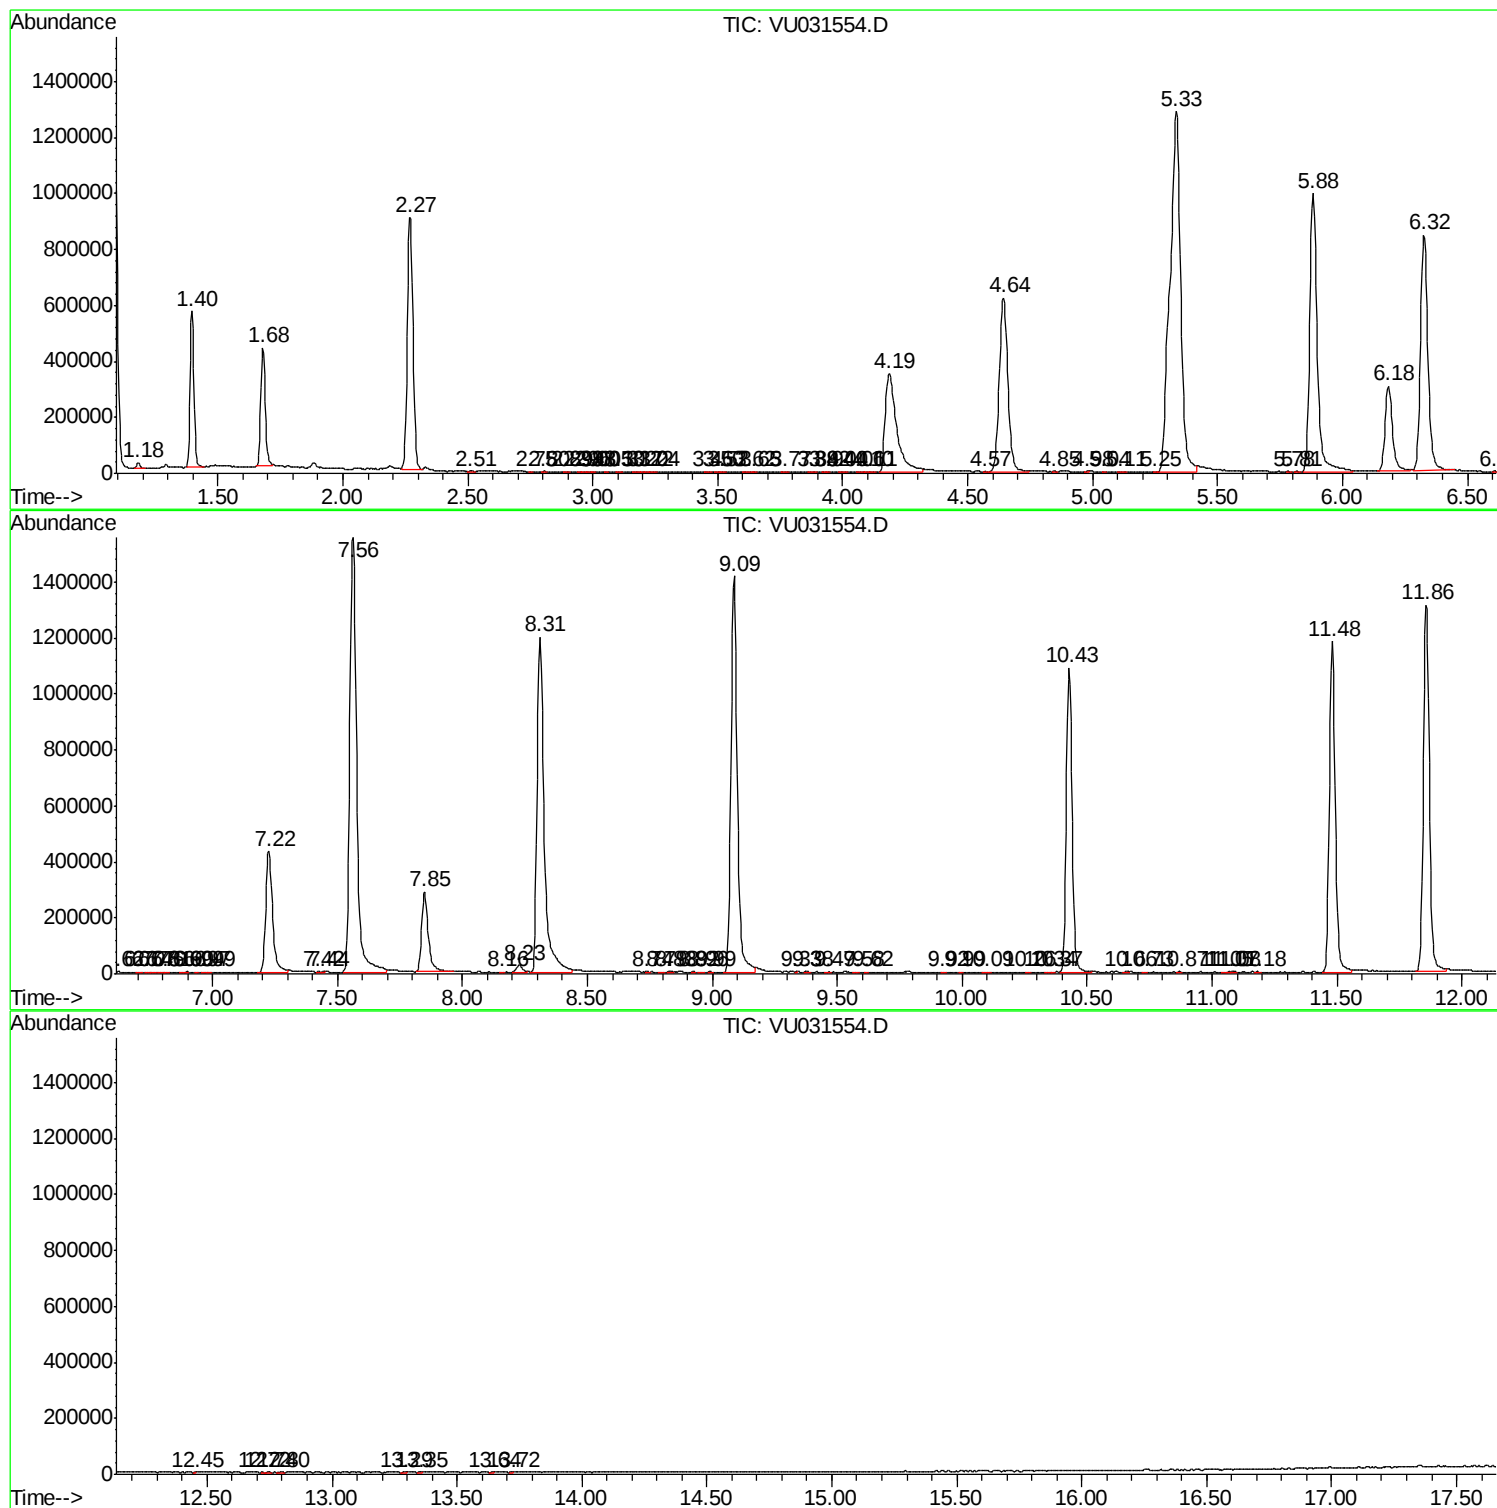

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031554.D
Acq On : 27 Apr 2019 00:39
Operator : JC/SP
Sample : K2592-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031554.D
Acq On : 27 Apr 2019 00:39
Operator : JC/SP
Sample : K2592-07 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc