

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031558.D
 Acq On : 27 Apr 2019 02:13
 Operator : JC/SP
 Sample : K2592-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rBV	16987	15976	0.16%	0.042%
2	1.396	87	95	106	rBV	539132	590730	6.08%	1.553%
3	1.679	176	183	198	rVB	428479	522164	5.37%	1.373%
4	1.881	239	246	258	rVB	82971	115285	1.19%	0.303%
5	2.270	356	367	381	rBV	894623	1371798	14.12%	3.607%
6	2.698	492	500	503	rBV5	3751	4955	0.05%	0.013%
7	2.759	517	519	523	rBV3	1047	922	0.01%	0.002%
8	2.781	523	526	528	rVV3	1503	1061	0.01%	0.003%
9	2.810	532	535	536	rBV2	1371	748	0.01%	0.002%
10	2.888	556	559	563	rBV2	1183	1019	0.01%	0.003%
11	2.962	580	582	585	rBV2	1092	843	0.01%	0.002%
12	3.010	595	597	602	rVB3	1339	1121	0.01%	0.003%
13	3.039	602	606	609	rBV4	1946	1529	0.02%	0.004%
14	3.093	620	623	627	rVB2	1656	1177	0.01%	0.003%
15	3.116	627	630	631	rBV2	1133	698	0.01%	0.002%
16	3.328	693	696	699	rBV2	1634	1051	0.01%	0.003%
17	3.453	730	735	738	rBV3	806	705	0.01%	0.002%
18	3.498	743	749	752	rBV2	1145	1165	0.01%	0.003%
19	3.537	757	761	766	rBV4	1604	2032	0.02%	0.005%
20	3.637	787	792	798	rBV2	1370	1703	0.02%	0.004%
21	3.769	830	833	835	rBV2	1183	800	0.01%	0.002%
22	3.810	843	846	853	rVB3	1070	1281	0.01%	0.003%
23	3.842	853	856	861	rBV4	1577	1311	0.01%	0.003%
24	3.888	867	870	872	rBV3	1563	851	0.01%	0.002%
25	3.990	898	902	906	rVB4	1043	948	0.01%	0.002%
26	4.016	906	910	915	rBV3	1530	1666	0.02%	0.004%
27	4.048	917	920	924	rVB2	1239	949	0.01%	0.002%
28	4.090	928	933	936	rBV4	783	850	0.01%	0.002%
29	4.132	944	946	950	rVB3	923	700	0.01%	0.002%
30	4.187	950	963	993	rBV	358790	1117994	11.50%	2.940%
31	4.550	1071	1076	1078	rBV4	1818	1598	0.02%	0.004%
32	4.643	1088	1105	1131	rBV	614113	1462216	15.05%	3.845%
33	5.100	1244	1247	1251	rVB3	1437	1041	0.01%	0.003%
34	5.334	1296	1320	1351	rBV2	1278030	3838920	39.50%	10.095%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031558.D
 Acq On : 27 Apr 2019 02:13
 Operator : JC/SP
 Sample : K2592-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.752	1447	1450	1454	rVB3	2241	1696	0.02%	0.004%
36	5.781	1454	1459	1461	rBV5	1844	1388	0.01%	0.004%
37	5.801	1461	1465	1468	rBV3	1819	1470	0.02%	0.004%
38	5.881	1476	1490	1522	rBV	1003363	2084026	21.44%	5.480%
39	6.180	1568	1583	1615	rBV	4897294	9718163	100.00%	25.555%
40	6.325	1617	1628	1651	rVB	849659	1745208	17.96%	4.589%
41	6.714	1747	1749	1753	rVB3	1407	874	0.01%	0.002%
42	6.736	1753	1756	1759	rBV3	1223	750	0.01%	0.002%
43	6.858	1790	1794	1797	rBV3	1027	982	0.01%	0.003%
44	6.881	1798	1801	1803	rVV3	1518	754	0.01%	0.002%
45	7.010	1835	1841	1842	rBV3	1450	1405	0.01%	0.004%
46	7.080	1859	1863	1865	rVV4	1074	770	0.01%	0.002%
47	7.106	1868	1871	1874	rVB2	1369	930	0.01%	0.002%
48	7.132	1874	1879	1882	rVB5	1209	1119	0.01%	0.003%
49	7.151	1882	1885	1888	rBV3	961	816	0.01%	0.002%
50	7.225	1895	1908	1930	rBV	435097	819262	8.43%	2.154%
51	7.376	1952	1955	1960	rBV5	1448	1379	0.01%	0.004%
52	7.450	1976	1978	1982	rVB5	2112	1204	0.01%	0.003%
53	7.476	1982	1986	1988	rVB2	1329	802	0.01%	0.002%
54	7.492	1988	1991	1996	rBV4	1198	1161	0.01%	0.003%
55	7.563	1999	2013	2050	rBV	1569096	2918261	30.03%	7.674%
56	7.849	2091	2102	2126	rBV	285763	530135	5.46%	1.394%
57	8.058	2165	2167	2169	rBV	1755	772	0.01%	0.002%
58	8.225	2208	2219	2234	rBV3	158960	274608	2.83%	0.722%
59	8.309	2235	2245	2286	rVV	1231292	2350643	24.19%	6.181%
60	8.781	2389	2392	2395	rBV3	1237	921	0.01%	0.002%
61	8.916	2427	2434	2440	rBV6	2061	3149	0.03%	0.008%
62	8.955	2443	2446	2448	rBV2	1432	758	0.01%	0.002%
63	9.087	2474	2487	2509	rBV	1443097	2490137	25.62%	6.548%
64	9.363	2571	2573	2579	rBV2	1120	1280	0.01%	0.003%
65	9.469	2601	2606	2608	rBV3	1854	1824	0.02%	0.005%
66	9.688	2671	2674	2675	rBV3	1443	822	0.01%	0.002%
67	9.733	2685	2688	2691	rBV3	1065	725	0.01%	0.002%
68	9.778	2699	2702	2705	rBV2	866	676	0.01%	0.002%
69	9.862	2725	2728	2730	rBV3	1422	946	0.01%	0.002%
70	9.935	2746	2751	2758	rVB4	2065	2847	0.03%	0.007%
71	9.971	2758	2762	2763	rBV2	1091	739	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031558.D
 Acq On : 27 Apr 2019 02:13
 Operator : JC/SP
 Sample : K2592-11 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X04

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.000	2768	2771	2777	rVB4	1424	1171	0.01%	0.003%
73	10.038	2778	2783	2786	rBV3	1243	1218	0.01%	0.003%
74	10.054	2786	2788	2791	rVB3	1764	959	0.01%	0.003%
75	10.074	2791	2794	2797	rBV2	1268	794	0.01%	0.002%
76	10.122	2804	2809	2812	rBV6	1450	1330	0.01%	0.003%
77	10.154	2816	2819	2821	rBV3	1556	1077	0.01%	0.003%
78	10.199	2830	2833	2835	rBV4	1313	897	0.01%	0.002%
79	10.427	2890	2904	2927	rBV	1089600	1773083	18.25%	4.663%
80	10.575	2947	2950	2953	rVB4	1295	755	0.01%	0.002%
81	10.775	3008	3012	3017	rVV2	1519	1442	0.01%	0.004%
82	10.871	3039	3042	3045	rVB	1445	898	0.01%	0.002%
83	10.939	3061	3063	3069	rVB5	1385	1314	0.01%	0.003%
84	11.177	3135	3137	3139	rBV	1094	683	0.01%	0.002%
85	11.312	3176	3179	3182	rVB2	1570	928	0.01%	0.002%
86	11.427	3212	3215	3218	rBV2	1587	858	0.01%	0.002%
87	11.482	3219	3232	3260	rBV	1209425	1999232	20.57%	5.257%
88	11.726	3306	3308	3313	rBV5	1708	1320	0.01%	0.003%
89	11.855	3336	3348	3368	rBV	1309310	2194350	22.58%	5.770%
90	12.231	3462	3465	3470	rBV3	2481	1639	0.02%	0.004%
91	12.488	3542	3545	3547	rVB2	1468	866	0.01%	0.002%
92	12.903	3671	3674	3676	rBV2	1891	1189	0.01%	0.003%
93	13.099	3732	3735	3739	rBV2	2285	2405	0.02%	0.006%
94	13.148	3747	3750	3755	rVB5	1614	932	0.01%	0.002%
95	13.173	3755	3758	3761	rBV2	1246	889	0.01%	0.002%
96	13.279	3789	3791	3794	rBV4	1218	829	0.01%	0.002%
97	13.299	3794	3797	3800	rVB2	2114	1329	0.01%	0.003%
98	13.710	3923	3925	3931	rVB4	1383	1000	0.01%	0.003%
99	13.887	3977	3980	3982	rBV3	2462	1567	0.02%	0.004%
100	14.299	4105	4108	4112	rBV3	2026	1717	0.02%	0.005%


Sum of corrected areas: 38027880

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031558.D
Acq On : 27 Apr 2019 02:13
Operator : JC/SP
Sample : K2592-11 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X04

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

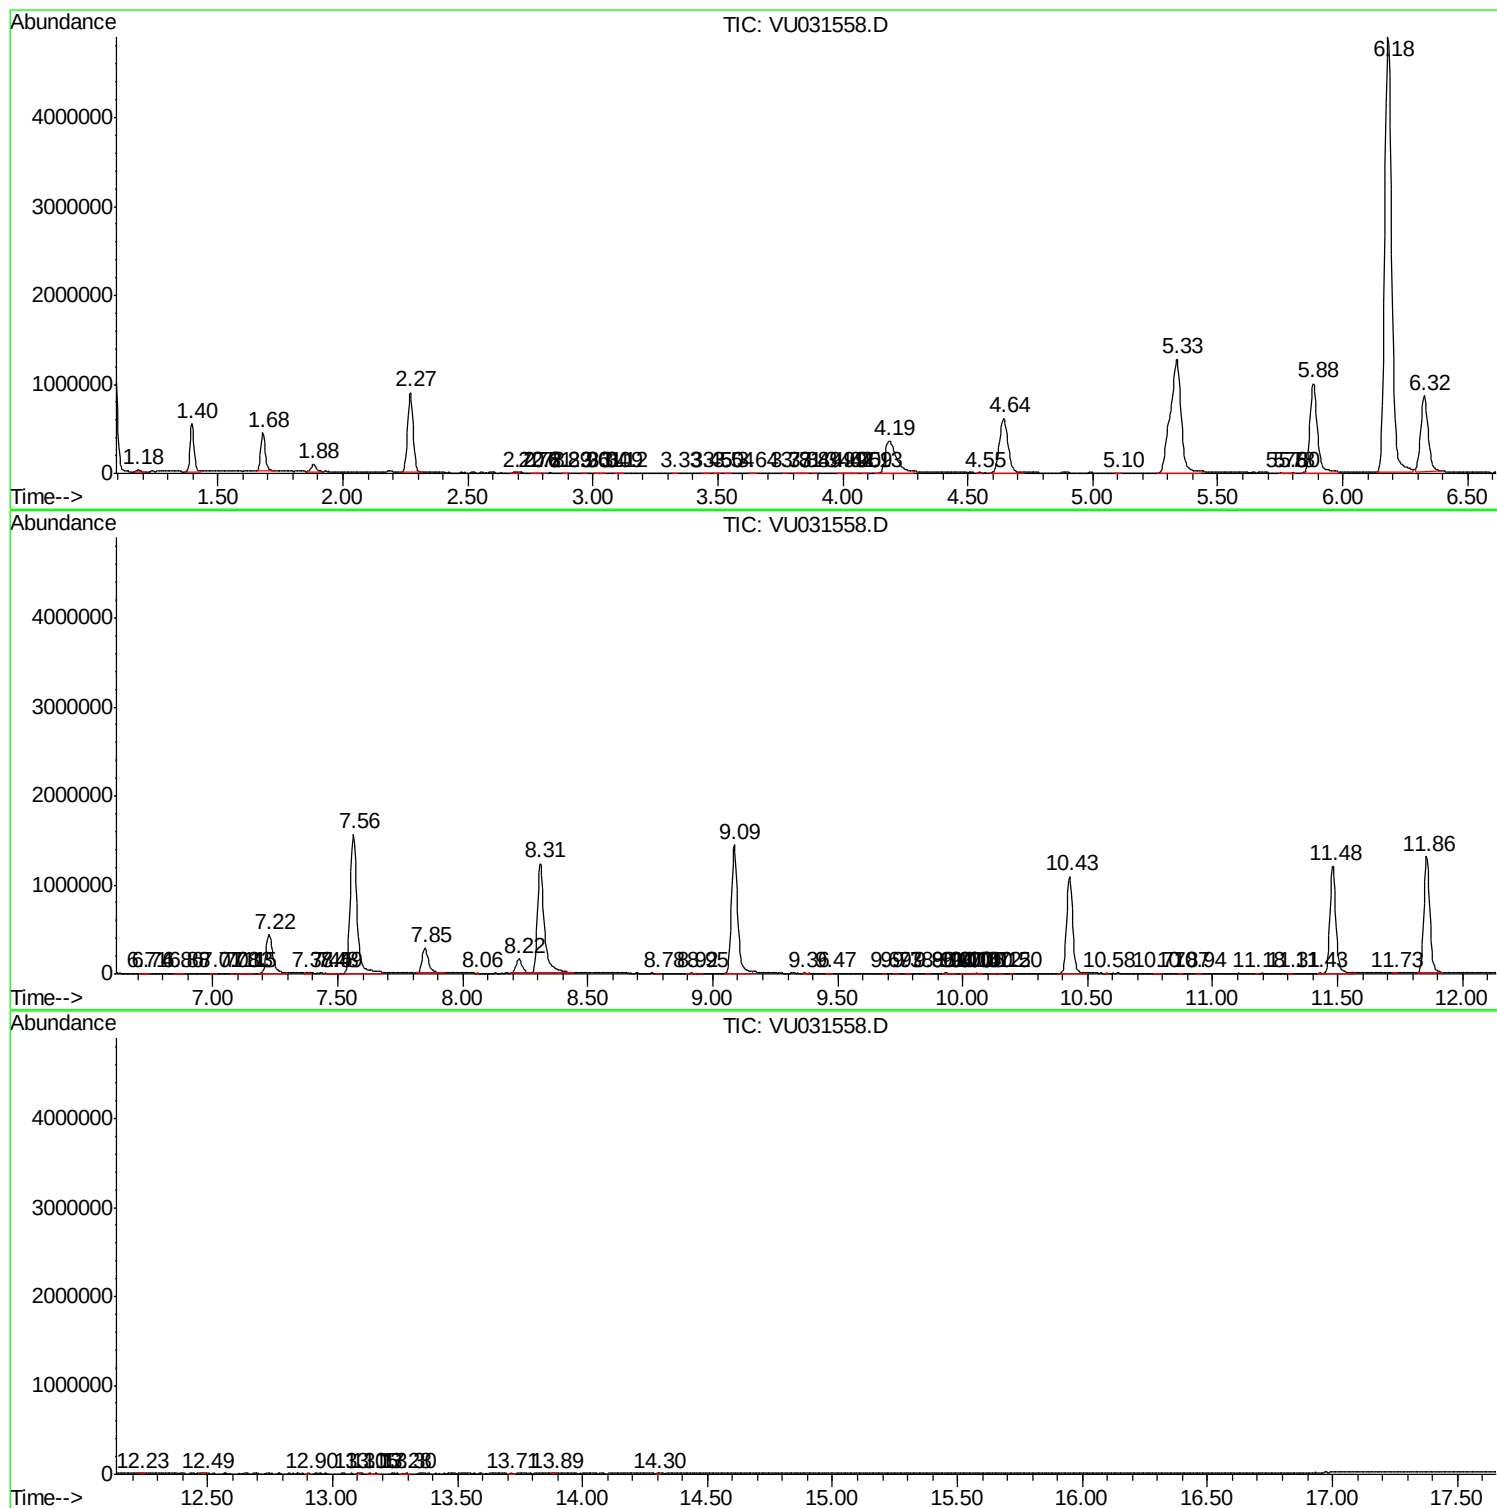

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042719\
Data File : VU031558.D
Acq On : 27 Apr 2019 02:13
Operator : JC/SP
Sample : K2592-11 50X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0X04

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031558.D
Acq On : 27 Apr 2019 02:13
Operator : JC/SP
Sample : K2592-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X04

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc