

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031560.D
 Acq On : 27 Apr 2019 02:59
 Operator : JC/SP
 Sample : K2592-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB2	19437	20260	0.03%	0.020%
2	1.396	88	95	107	rVB	535956	580826	0.86%	0.583%
3	1.679	176	183	200	rVB	435354	537281	0.79%	0.539%
4	1.881	237	246	262	rVB	494591	690437	1.02%	0.693%
5	2.270	355	367	380	rBV	908059	1378638	2.03%	1.383%
6	2.437	416	419	422	rBV2	1168	782	0.00%	0.001%
7	2.701	492	501	507	rBV5	6571	10420	0.02%	0.010%
8	2.807	529	534	536	rBV	1288	1120	0.00%	0.001%
9	2.830	536	541	543	rBV3	1352	1443	0.00%	0.001%
10	2.875	552	555	557	rBV3	1205	892	0.00%	0.001%
11	2.891	557	560	562	rVV2	873	741	0.00%	0.001%
12	2.926	567	571	574	rBV2	974	874	0.00%	0.001%
13	2.974	580	586	587	rBV4	2305	1897	0.00%	0.002%
14	3.103	621	626	629	rBV2	759	772	0.00%	0.001%
15	3.125	630	633	638	rVB3	1632	1516	0.00%	0.002%
16	3.273	676	679	682	rVV3	2098	1484	0.00%	0.001%
17	3.299	685	687	692	rVV3	1347	1037	0.00%	0.001%
18	3.331	694	697	700	rVB3	1239	771	0.00%	0.001%
19	3.354	700	704	708	rVB5	1191	1102	0.00%	0.001%
20	3.383	708	713	716	rBV3	1336	1448	0.00%	0.001%
21	3.492	745	747	753	rBV6	758	770	0.00%	0.001%
22	3.608	779	783	787	rBV4	1075	1092	0.00%	0.001%
23	3.685	799	807	809	rBV3	1139	1500	0.00%	0.002%
24	3.717	814	817	819	rVV	1021	772	0.00%	0.001%
25	3.746	823	826	829	rVV	1695	1063	0.00%	0.001%
26	3.817	844	848	853	rBV3	1264	1524	0.00%	0.002%
27	4.135	944	947	950	rBV4	1166	1063	0.00%	0.001%
28	4.186	950	963	1005	rBV2	357574	1163297	1.72%	1.167%
29	4.540	1069	1073	1075	rBV3	1253	1122	0.00%	0.001%
30	4.643	1088	1105	1131	rBV	626507	1491319	2.20%	1.496%
31	4.881	1172	1179	1185	rBV10	2922	4503	0.01%	0.005%
32	5.048	1228	1231	1235	rVB3	1471	951	0.00%	0.001%
33	5.132	1247	1257	1275	rVB4	11473	28162	0.04%	0.028%
34	5.202	1275	1279	1286	rBV4	1479	1737	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031560.D
 Acq On : 27 Apr 2019 02:59
 Operator : JC/SP
 Sample : K2592-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1296	1320	1354	rBV2	1281779	3872561	5.71%	3.884%
36	5.749	1445	1449	1452	rBV3	2299	1815	0.00%	0.002%
37	5.823	1469	1472	1474	rBV3	1096	745	0.00%	0.001%
38	5.881	1477	1490	1521	rBV	1018260	2114614	3.12%	2.121%
39	6.183	1566	1584	1618	rBV	35174722	67768369	100.00%	67.972%
40	6.325	1620	1628	1659	rVB	902384	1961506	2.89%	1.967%
41	6.727	1750	1753	1759	rBV7	2308	2335	0.00%	0.002%
42	6.755	1760	1762	1765	rBV2	1152	796	0.00%	0.001%
43	6.794	1771	1774	1777	rBV5	1798	1355	0.00%	0.001%
44	6.913	1799	1811	1813	rBV9	2820	5153	0.01%	0.005%
45	7.029	1844	1847	1850	rBV4	1275	819	0.00%	0.001%
46	7.048	1851	1853	1858	rVB3	1427	925	0.00%	0.001%
47	7.106	1868	1871	1873	rBV3	1135	977	0.00%	0.001%
48	7.135	1876	1880	1882	rBV3	1388	1049	0.00%	0.001%
49	7.170	1887	1891	1893	rBV2	1161	943	0.00%	0.001%
50	7.225	1896	1908	1933	rBV2	448006	832762	1.23%	0.835%
51	7.563	1999	2013	2031	rBV	1573132	2850468	4.21%	2.859%
52	7.849	2091	2102	2130	rBV	288772	531055	0.78%	0.533%
53	8.026	2154	2157	2160	rVB3	1985	1208	0.00%	0.001%
54	8.222	2204	2218	2235	rBV	1494680	2648734	3.91%	2.657%
55	8.308	2236	2245	2285	rVB	1241839	2400968	3.54%	2.408%
56	8.672	2349	2358	2364	rBV8	2885	4442	0.01%	0.004%
57	8.755	2381	2384	2388	rBV5	1065	786	0.00%	0.001%
58	8.833	2406	2408	2414	rVB6	1390	795	0.00%	0.001%
59	8.907	2426	2431	2435	rBV4	2089	2334	0.00%	0.002%
60	9.025	2464	2468	2472	rVB4	1946	1916	0.00%	0.002%
61	9.087	2473	2487	2520	rBV	1457609	2582343	3.81%	2.590%
62	9.373	2571	2576	2584	rVB4	12178	16483	0.02%	0.017%
63	9.472	2604	2607	2611	rVB4	1481	1111	0.00%	0.001%
64	9.508	2611	2618	2622	rBV6	1528	1657	0.00%	0.002%
65	9.572	2636	2638	2643	rVB4	1731	1043	0.00%	0.001%
66	9.611	2647	2650	2653	rBV2	1415	834	0.00%	0.001%
67	9.781	2694	2703	2719	rBV4	17236	30908	0.05%	0.031%
68	9.929	2744	2749	2752	rBV4	1886	1344	0.00%	0.001%
69	9.955	2752	2757	2760	rBV4	1443	1108	0.00%	0.001%
70	9.977	2760	2764	2767	rBV4	888	852	0.00%	0.001%
71	10.058	2785	2789	2795	rBV2	1783	1839	0.00%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031560.D
 Acq On : 27 Apr 2019 02:59
 Operator : JC/SP
 Sample : K2592-13 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X76

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.087	2795	2798	2803	rBV3	1149	959	0.00%	0.001%
73	10.119	2805	2808	2811	rVV2	1301	1017	0.00%	0.001%
74	10.170	2818	2824	2832	rVB6	3233	4420	0.01%	0.004%
75	10.209	2834	2836	2841	rVB4	1309	973	0.00%	0.001%
76	10.247	2845	2848	2853	rVB4	1654	1096	0.00%	0.001%
77	10.279	2855	2858	2861	rBV3	1148	880	0.00%	0.001%
78	10.321	2868	2871	2874	rVB	1535	860	0.00%	0.001%
79	10.427	2891	2904	2934	rBV	1099059	1793945	2.65%	1.799%
80	10.646	2969	2972	2976	rVB	1211	840	0.00%	0.001%
81	10.688	2976	2985	2990	rBV7	6950	11821	0.02%	0.012%
82	10.768	3008	3010	3019	rVB7	2925	3271	0.00%	0.003%
83	10.804	3019	3021	3023	rBV2	1394	885	0.00%	0.001%
84	10.836	3028	3031	3033	rVB3	1423	804	0.00%	0.001%
85	10.977	3065	3075	3081	rBV4	10039	16430	0.02%	0.016%
86	11.025	3087	3090	3094	rBV3	1889	1711	0.00%	0.002%
87	11.080	3103	3107	3110	rVB5	2415	1799	0.00%	0.002%
88	11.151	3122	3129	3136	rBV4	8871	12117	0.02%	0.012%
89	11.212	3145	3148	3157	rVB4	1663	2410	0.00%	0.002%
90	11.263	3157	3164	3167	rBV2	1520	2145	0.00%	0.002%
91	11.318	3177	3181	3184	rBV3	1868	1842	0.00%	0.002%
92	11.479	3219	3231	3251	rBV	1226362	2035481	3.00%	2.042%
93	11.855	3336	3348	3372	rBV	1335195	2213864	3.27%	2.221%
94	12.254	3470	3472	3475	rBV3	1945	1329	0.00%	0.001%
95	13.106	3731	3737	3739	rBV5	1521	1435	0.00%	0.001%
96	13.241	3776	3779	3784	rBV2	1659	1459	0.00%	0.001%
97	13.614	3892	3895	3899	rVB3	1498	1067	0.00%	0.001%
98	13.967	4003	4005	4008	rBV4	1346	967	0.00%	0.001%
99	13.996	4011	4014	4018	rBV	1589	1121	0.00%	0.001%
100	14.913	4296	4299	4305	rBV6	2163	1816	0.00%	0.002%


Sum of corrected areas: 99700332

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031560.D
Acq On : 27 Apr 2019 02:59
Operator : JC/SP
Sample : K2592-13 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X76

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

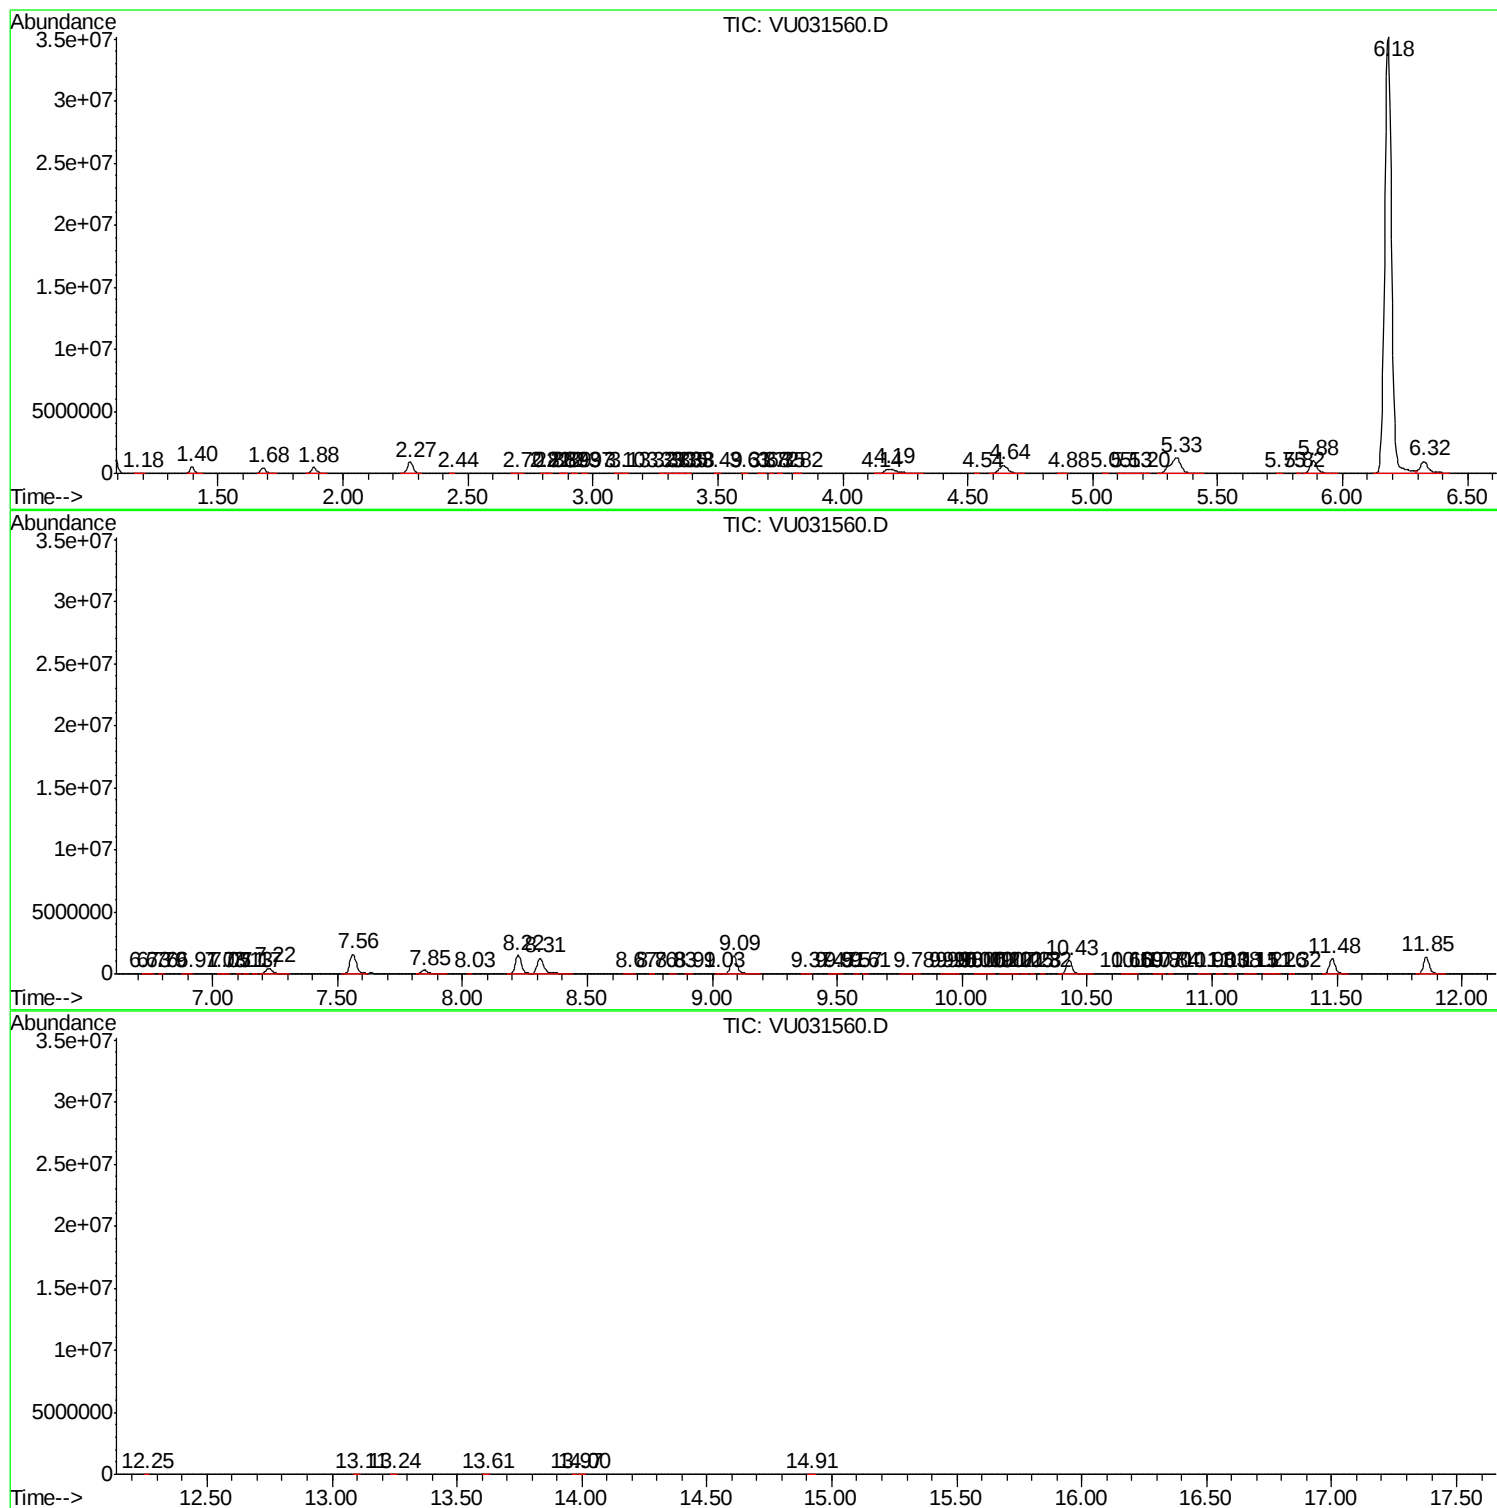

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031560.D
Acq On : 27 Apr 2019 02:59
Operator : JC/SP
Sample : K2592-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X76

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031560.D
Acq On : 27 Apr 2019 02:59
Operator : JC/SP
Sample : K2592-13 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X76

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc