

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031561.D
 Acq On : 27 Apr 2019 03:22
 Operator : JC/SP
 Sample : K2592-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rBV	19225	18412	0.01%	0.011%
2	1.395	88	95	108	rBV	548116	586080	0.46%	0.361%
3	1.678	176	183	197	rBV	432694	533769	0.42%	0.329%
4	1.881	237	246	263	rVB	800819	1137120	0.89%	0.701%
5	2.270	355	367	381	rBV	899111	1376101	1.08%	0.848%
6	2.421	410	414	420	rBV6	1435	1682	0.00%	0.001%
7	2.633	476	480	482	rBV4	1401	992	0.00%	0.001%
8	2.698	491	500	510	rBV6	7745	15202	0.01%	0.009%
9	2.829	537	541	545	rVB4	1868	1475	0.00%	0.001%
10	2.952	574	579	580	rBV3	1163	798	0.00%	0.000%
11	3.186	649	652	655	rVB2	1024	683	0.00%	0.000%
12	3.215	655	661	662	rBV3	1299	973	0.00%	0.001%
13	3.280	676	681	685	rBV5	1450	1336	0.00%	0.001%
14	3.315	690	692	697	rVB2	989	672	0.00%	0.000%
15	3.366	705	708	710	rBV2	876	624	0.00%	0.000%
16	3.415	720	723	727	rBV3	823	581	0.00%	0.000%
17	3.633	783	791	793	rBV3	1346	1336	0.00%	0.001%
18	3.701	807	812	818	rBV3	1027	1341	0.00%	0.001%
19	3.791	838	840	846	rVB5	811	741	0.00%	0.000%
20	3.820	846	849	851	rBV2	812	560	0.00%	0.000%
21	3.874	862	866	869	rBV3	1457	1362	0.00%	0.001%
22	3.993	899	903	907	rVB3	1503	974	0.00%	0.001%
23	4.016	907	910	913	rBV3	1435	1393	0.00%	0.001%
24	4.103	934	937	939	rBV	1248	940	0.00%	0.001%
25	4.183	950	962	1006	rBV	363503	1183712	0.93%	0.730%
26	4.505	1057	1062	1063	rBV3	2021	1872	0.00%	0.001%
27	4.643	1086	1105	1134	rBV	629860	1493307	1.17%	0.921%
28	5.058	1232	1234	1238	rVV3	1037	829	0.00%	0.001%
29	5.135	1242	1258	1273	rVB4	18572	48943	0.04%	0.030%
30	5.193	1273	1276	1279	rBV2	1109	911	0.00%	0.001%
31	5.334	1293	1320	1360	rBV2	1281194	3904422	3.05%	2.407%
32	5.733	1441	1444	1446	rBV3	1119	740	0.00%	0.000%
33	5.881	1476	1490	1533	rBV	1014427	2135325	1.67%	1.316%
34	6.186	1563	1585	1618	rBV3	65608411	127929637	100.00%	78.863%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031561.D
 Acq On : 27 Apr 2019 03:22
 Operator : JC/SP
 Sample : K2592-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.324	1621	1628	1666	rVB	943940	2103309	1.64%	1.297%
36	6.791	1771	1773	1775	rBV3	1592	773	0.00%	0.000%
37	7.019	1841	1844	1846	rBV5	1319	819	0.00%	0.001%
38	7.225	1895	1908	1935	rBV	458626	852904	0.67%	0.526%
39	7.508	1994	1996	1998	rBV2	1480	664	0.00%	0.000%
40	7.562	1998	2013	2029	rBV	1576258	2861403	2.24%	1.764%
41	7.848	2091	2102	2128	rBV	296729	534081	0.42%	0.329%
42	8.067	2165	2170	2184	rVB	5449	10879	0.01%	0.007%
43	8.221	2205	2218	2235	rBV	2302207	3963544	3.10%	2.443%
44	8.308	2236	2245	2288	rVB	1243494	2483893	1.94%	1.531%
45	8.636	2344	2347	2351	rVB4	2078	1758	0.00%	0.001%
46	8.826	2399	2406	2408	rBV4	2234	2836	0.00%	0.002%
47	8.987	2449	2456	2462	rVB6	1802	2359	0.00%	0.001%
48	9.012	2462	2464	2469	rBV4	664	665	0.00%	0.000%
49	9.086	2474	2487	2530	rVV	1464857	2578039	2.02%	1.589%
50	9.254	2530	2539	2553	rVB2	12843	26363	0.02%	0.016%
51	9.373	2567	2576	2593	rBV2	44514	79128	0.06%	0.049%
52	9.501	2613	2616	2618	rBV2	1258	795	0.00%	0.000%
53	9.533	2623	2626	2630	rBV3	946	812	0.00%	0.001%
54	9.598	2642	2646	2648	rBV3	1832	1149	0.00%	0.001%
55	9.614	2648	2651	2653	rBV3	1856	949	0.00%	0.001%
56	9.704	2677	2679	2682	rVB2	1211	626	0.00%	0.000%
57	9.729	2682	2687	2689	rBV3	1009	942	0.00%	0.001%
58	9.781	2693	2703	2714	rVV3	33766	59372	0.05%	0.037%
59	9.938	2744	2752	2754	rBV7	2137	2777	0.00%	0.002%
60	9.974	2759	2763	2766	rBV2	1917	1517	0.00%	0.001%
61	10.086	2795	2798	2802	rBV2	750	612	0.00%	0.000%
62	10.122	2806	2809	2811	rBV2	922	550	0.00%	0.000%
63	10.138	2811	2814	2816	rBV	999	682	0.00%	0.000%
64	10.237	2842	2845	2846	rBV3	1463	776	0.00%	0.000%
65	10.254	2847	2850	2853	rVV4	2462	1840	0.00%	0.001%
66	10.270	2853	2855	2859	rVB3	1046	591	0.00%	0.000%
67	10.331	2871	2874	2877	rVB3	1129	785	0.00%	0.000%
68	10.427	2891	2904	2927	rBV	1103249	1788558	1.40%	1.103%
69	10.594	2951	2956	2967	rVB7	5206	7206	0.01%	0.004%
70	10.681	2976	2983	2989	rBV2	15347	25129	0.02%	0.015%
71	10.771	3005	3011	3018	rVB5	5626	7552	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031561.D
 Acq On : 27 Apr 2019 03:22
 Operator : JC/SP
 Sample : K2592-14 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.852	3033	3036	3039	rBV2	1400	889	0.00%	0.001%
73	10.919	3051	3057	3059	rBV4	1664	1541	0.00%	0.001%
74	10.938	3060	3063	3065	rVV	2456	1821	0.00%	0.001%
75	10.967	3065	3072	3085	rVV	16190	27761	0.02%	0.017%
76	11.032	3089	3092	3096	rBV3	1545	1042	0.00%	0.001%
77	11.051	3096	3098	3101	rBV2	1257	776	0.00%	0.000%
78	11.147	3118	3128	3138	rBV	28991	48070	0.04%	0.030%
79	11.237	3152	3156	3160	rBV3	1485	1227	0.00%	0.001%
80	11.276	3166	3168	3171	rBV2	1033	623	0.00%	0.000%
81	11.366	3193	3196	3201	rVB3	1542	1132	0.00%	0.001%
82	11.408	3205	3209	3210	rBV3	1797	1138	0.00%	0.001%
83	11.479	3219	3231	3251	rBV	1239891	2031483	1.59%	1.252%
84	11.569	3253	3259	3271	rVB2	38354	63519	0.05%	0.039%
85	11.855	3336	3348	3372	rBV	1335745	2223918	1.74%	1.371%
86	12.434	3525	3528	3531	rBV4	1174	966	0.00%	0.001%
87	12.479	3537	3542	3546	rBV7	3576	3910	0.00%	0.002%
88	12.552	3562	3565	3567	rBV3	1546	867	0.00%	0.001%
89	12.823	3644	3649	3652	rBV4	1916	1697	0.00%	0.001%
90	12.993	3699	3702	3708	rVB5	1493	1263	0.00%	0.001%
91	13.022	3708	3711	3715	rBV3	1667	1217	0.00%	0.001%
92	13.070	3723	3726	3729	rBV3	1330	935	0.00%	0.001%
93	13.134	3744	3746	3748	rBV3	1507	640	0.00%	0.000%
94	13.176	3755	3759	3764	rBV6	2043	2046	0.00%	0.001%
95	13.241	3777	3779	3782	rVB3	1266	576	0.00%	0.000%
96	13.527	3864	3868	3869	rBV2	1999	1340	0.00%	0.001%
97	13.829	3959	3962	3964	rBV3	1612	1079	0.00%	0.001%
98	13.980	4006	4009	4011	rBV4	1321	983	0.00%	0.001%
99	14.623	4206	4209	4212	rBV3	2042	1250	0.00%	0.001%
100	14.707	4232	4235	4239	rVB3	2497	1969	0.00%	0.001%


Sum of corrected areas: 162217160

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031561.D
Acq On : 27 Apr 2019 03:22
Operator : JC/SP
Sample : K2592-14 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0X77

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

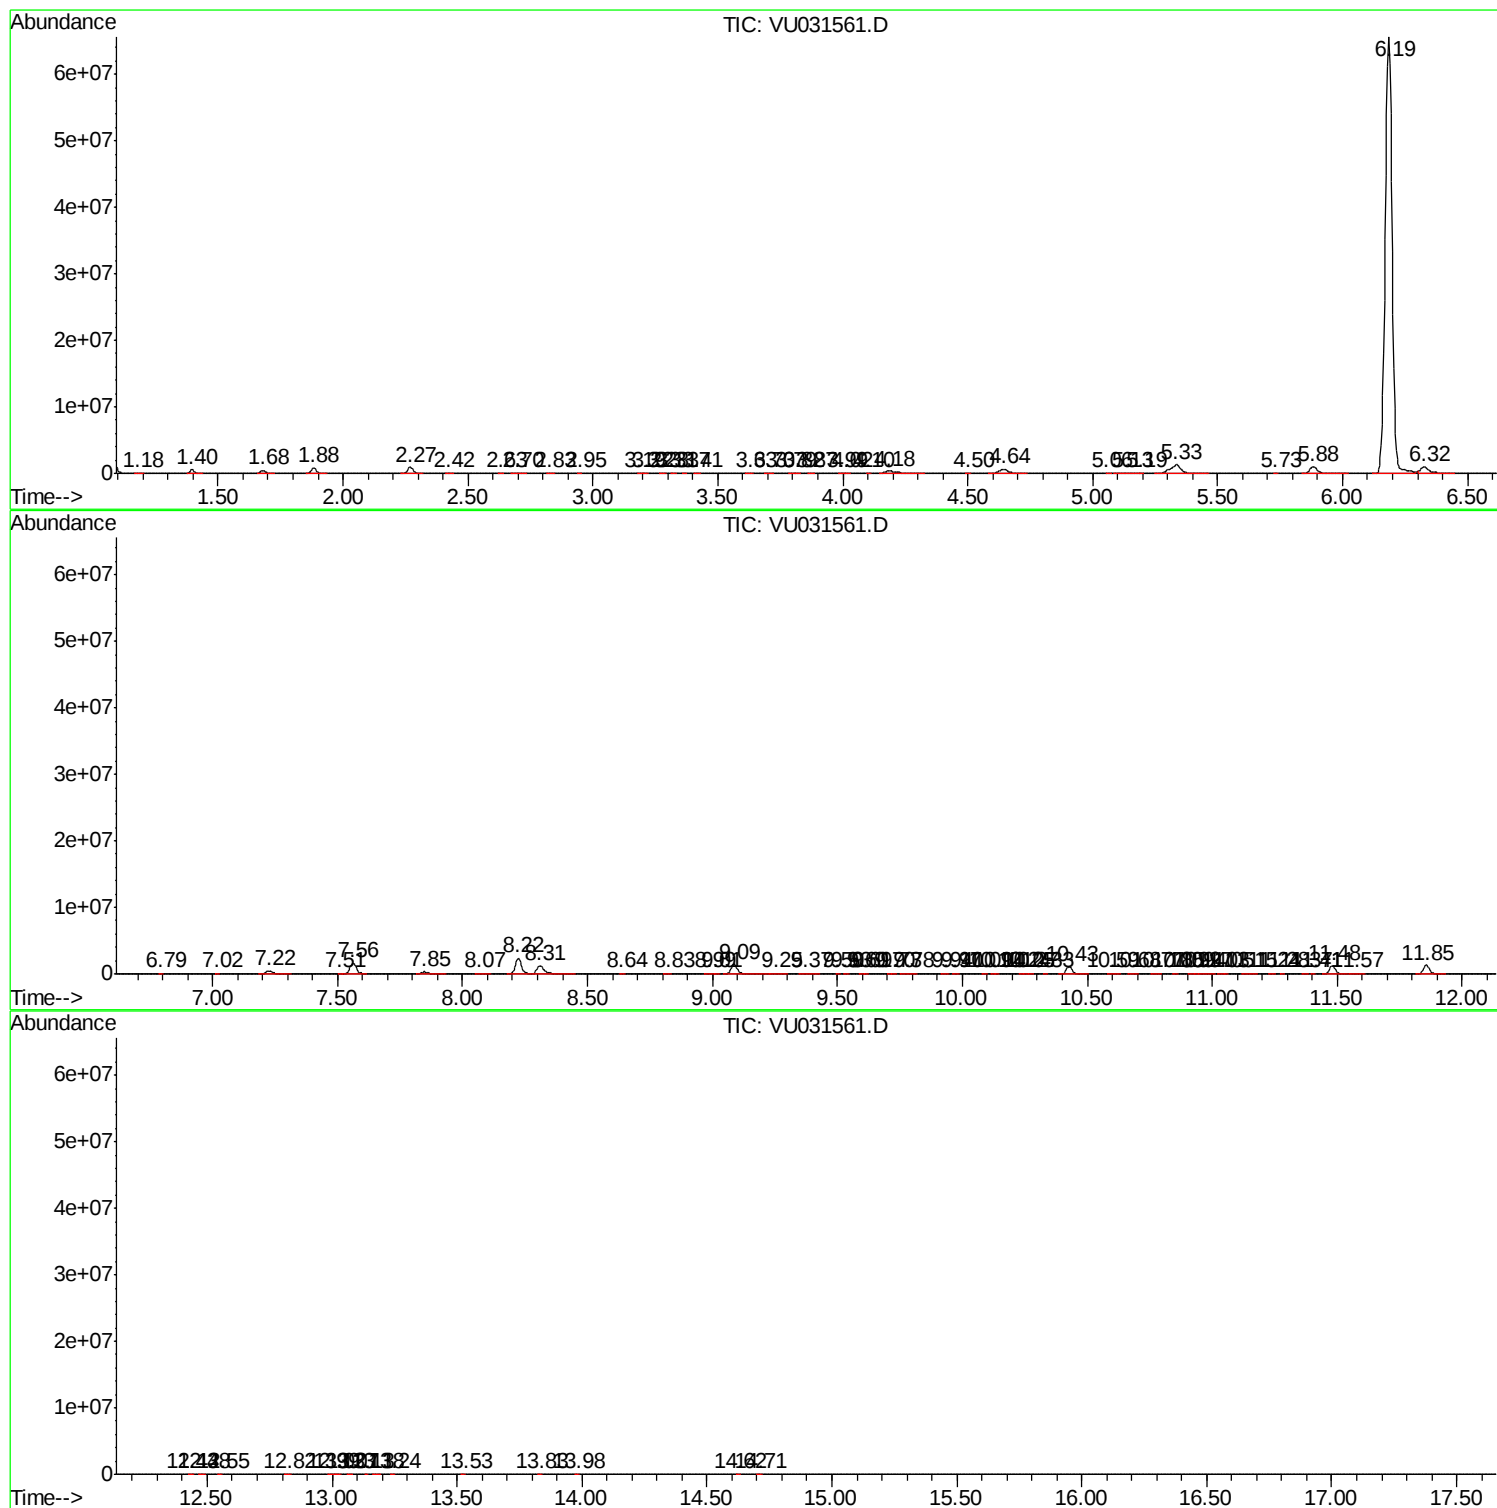

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031561.D
Acq On : 27 Apr 2019 03:22
Operator : JC/SP
Sample : K2592-14 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X77

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031561.D
Acq On : 27 Apr 2019 03:22
Operator : JC/SP
Sample : K2592-14 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X77

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc