

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031563.D
 Acq On : 27 Apr 2019 04:09
 Operator : JC/SP
 Sample : K2592-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB2	19427	19188	0.50%	0.068%
2	1.396	88	95	106	rBV	525509	569152	14.77%	2.026%
3	1.678	176	183	202	rVB	430234	530217	13.76%	1.888%
4	2.267	355	366	380	rBV	887639	1358719	35.26%	4.837%
5	2.473	428	430	434	rVB3	2175	1415	0.04%	0.005%
6	2.878	553	556	561	rBV4	1328	1251	0.03%	0.004%
7	2.952	577	579	584	rVB4	1420	1105	0.03%	0.004%
8	3.003	591	595	598	rBV3	1952	1790	0.05%	0.006%
9	3.100	622	625	630	rBV3	1278	1330	0.03%	0.005%
10	3.164	642	645	650	rBV4	1169	1071	0.03%	0.004%
11	3.354	701	704	706	rBV	2036	1100	0.03%	0.004%
12	3.392	713	716	720	rBV	928	805	0.02%	0.003%
13	3.434	725	729	733	rBV3	1019	815	0.02%	0.003%
14	3.514	749	754	758	rBV4	1788	1792	0.05%	0.006%
15	3.537	758	761	763	rVV2	1053	768	0.02%	0.003%
16	3.575	771	773	776	rVB	1592	830	0.02%	0.003%
17	3.624	784	788	793	rBV3	1667	1813	0.05%	0.006%
18	3.649	793	796	799	rVV3	1493	995	0.03%	0.004%
19	3.704	811	813	821	rVB5	1143	1168	0.03%	0.004%
20	3.762	828	831	836	rBV3	1062	831	0.02%	0.003%
21	3.836	848	854	855	rBV2	1017	922	0.02%	0.003%
22	3.932	881	884	885	rBV	1486	872	0.02%	0.003%
23	3.942	885	887	891	rVB3	1534	776	0.02%	0.003%
24	3.997	902	904	910	rVB3	1077	889	0.02%	0.003%
25	4.186	948	963	996	rBV	350205	1107062	28.73%	3.941%
26	4.534	1067	1071	1076	rVB4	1855	1988	0.05%	0.007%
27	4.643	1088	1105	1127	rBV2	613818	1468017	38.10%	5.226%
28	4.817	1155	1159	1167	rBV8	1602	1827	0.05%	0.007%
29	4.987	1209	1212	1216	rVB2	1836	1403	0.04%	0.005%
30	5.055	1229	1233	1238	rVB5	1592	1574	0.04%	0.006%
31	5.087	1238	1243	1245	rBV3	1453	1312	0.03%	0.005%
32	5.122	1250	1254	1257	rBV3	1075	765	0.02%	0.003%
33	5.334	1296	1320	1345	rBV2	1288996	3853282	100.00%	13.718%
34	5.714	1434	1438	1439	rBV4	1100	783	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031563.D
 Acq On : 27 Apr 2019 04:09
 Operator : JC/SP
 Sample : K2592-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.881	1476	1490	1519	rBV	1000212	2072422	53.78%	7.378%
36	6.183	1569	1584	1598	rBV6	67538	149207	3.87%	0.531%
37	6.325	1614	1628	1659	rBV	860174	1764543	45.79%	6.282%
38	6.759	1761	1763	1768	rBV4	1311	918	0.02%	0.003%
39	6.781	1768	1770	1775	rVB2	1345	869	0.02%	0.003%
40	6.807	1775	1778	1781	rBV2	1591	1124	0.03%	0.004%
41	6.887	1799	1803	1807	rBV3	1683	1296	0.03%	0.005%
42	7.006	1837	1840	1846	rBV5	1798	1647	0.04%	0.006%
43	7.083	1862	1864	1866	rBV2	1548	851	0.02%	0.003%
44	7.177	1888	1893	1895	rVB3	1385	941	0.02%	0.003%
45	7.225	1895	1908	1938	rBV	430631	811430	21.06%	2.889%
46	7.427	1967	1971	1974	rBV4	1837	1490	0.04%	0.005%
47	7.489	1985	1990	1994	rBV7	1284	1352	0.04%	0.005%
48	7.562	1998	2013	2046	rBV	1537395	2865217	74.36%	10.200%
49	7.849	2091	2102	2130	rBV	281928	525396	13.64%	1.870%
50	8.016	2151	2154	2158	rBV4	1458	1194	0.03%	0.004%
51	8.045	2161	2163	2166	rVB2	2215	1149	0.03%	0.004%
52	8.170	2200	2202	2208	rVB6	1280	1306	0.03%	0.005%
53	8.225	2208	2219	2234	rBV5	21841	43559	1.13%	0.155%
54	8.312	2234	2246	2291	rBV	1206095	2423756	62.90%	8.629%
55	8.720	2370	2373	2377	rVB3	1290	951	0.02%	0.003%
56	8.993	2454	2458	2462	rBV6	1379	1184	0.03%	0.004%
57	9.087	2474	2487	2527	rBV	1426647	2522153	65.45%	8.979%
58	9.296	2549	2552	2555	rVB3	1724	1200	0.03%	0.004%
59	9.321	2557	2560	2566	rVB4	2158	2316	0.06%	0.008%
60	9.707	2676	2680	2685	rBV3	1285	1416	0.04%	0.005%
61	9.749	2690	2693	2695	rBV2	1722	1121	0.03%	0.004%
62	9.784	2700	2704	2707	rBV3	2064	1552	0.04%	0.006%
63	9.855	2721	2726	2730	rBV4	1421	1357	0.04%	0.005%
64	9.958	2755	2758	2761	rBV4	1119	1056	0.03%	0.004%
65	10.025	2777	2779	2785	rVB3	1746	1179	0.03%	0.004%
66	10.067	2785	2792	2794	rBV4	1525	1859	0.05%	0.007%
67	10.080	2794	2796	2799	rVV	1317	876	0.02%	0.003%
68	10.125	2806	2810	2813	rVB3	986	787	0.02%	0.003%
69	10.302	2861	2865	2870	rBV3	1240	1370	0.04%	0.005%
70	10.328	2870	2873	2876	rBV	1148	1080	0.03%	0.004%
71	10.369	2883	2886	2889	rBV2	1395	1078	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031563.D
 Acq On : 27 Apr 2019 04:09
 Operator : JC/SP
 Sample : K2592-16 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X82

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.427	2889	2904	2931	rVV	1095151	1784414	46.31%	6.353%
73	10.556	2940	2944	2947	rBV3	1301	1350	0.04%	0.005%
74	10.614	2958	2962	2968	rVB6	2319	2379	0.06%	0.008%
75	10.646	2968	2972	2973	rBV3	1361	852	0.02%	0.003%
76	10.678	2980	2982	2989	rBV4	1284	1267	0.03%	0.005%
77	10.784	3011	3015	3018	rVB2	1886	1451	0.04%	0.005%
78	10.810	3018	3023	3028	rVB2	1561	1783	0.05%	0.006%
79	10.842	3028	3033	3036	rBV3	1221	1266	0.03%	0.005%
80	10.871	3038	3042	3046	rBV	2833	2683	0.07%	0.010%
81	10.977	3072	3075	3078	rBV2	1389	1047	0.03%	0.004%
82	11.051	3096	3098	3102	rBV3	1077	854	0.02%	0.003%
83	11.074	3102	3105	3109	rVB3	1470	1200	0.03%	0.004%
84	11.125	3115	3121	3124	rBV6	2159	2436	0.06%	0.009%
85	11.157	3129	3131	3136	rVV5	829	764	0.02%	0.003%
86	11.202	3141	3145	3146	rBV	1797	1047	0.03%	0.004%
87	11.263	3160	3164	3168	rBV3	1212	988	0.03%	0.004%
88	11.289	3168	3172	3175	rBV4	1399	1194	0.03%	0.004%
89	11.398	3202	3206	3211	rBV3	2145	2401	0.06%	0.009%
90	11.482	3219	3232	3251	rBV	1169124	1939064	50.32%	6.903%
91	11.855	3336	3348	3378	rBV	1279032	2173589	56.41%	7.738%
92	12.183	3447	3450	3452	rBV2	1636	999	0.03%	0.004%
93	12.520	3552	3555	3558	rBV2	1568	1009	0.03%	0.004%
94	12.578	3568	3573	3579	rBV3	2178	2730	0.07%	0.010%
95	12.794	3637	3640	3649	rVB5	2275	3099	0.08%	0.011%
96	12.839	3649	3654	3657	rBV5	1844	1895	0.05%	0.007%
97	13.154	3749	3752	3757	rBV4	1649	1444	0.04%	0.005%
98	13.196	3762	3765	3770	rBV4	1332	1229	0.03%	0.004%
99	14.491	4165	4168	4172	rBV4	1841	1455	0.04%	0.005%
100	15.022	4330	4333	4340	rBV3	2537	3514	0.09%	0.013%


Sum of corrected areas: 28089232

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031563.D
Acq On : 27 Apr 2019 04:09
Operator : JC/SP
Sample : K2592-16 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

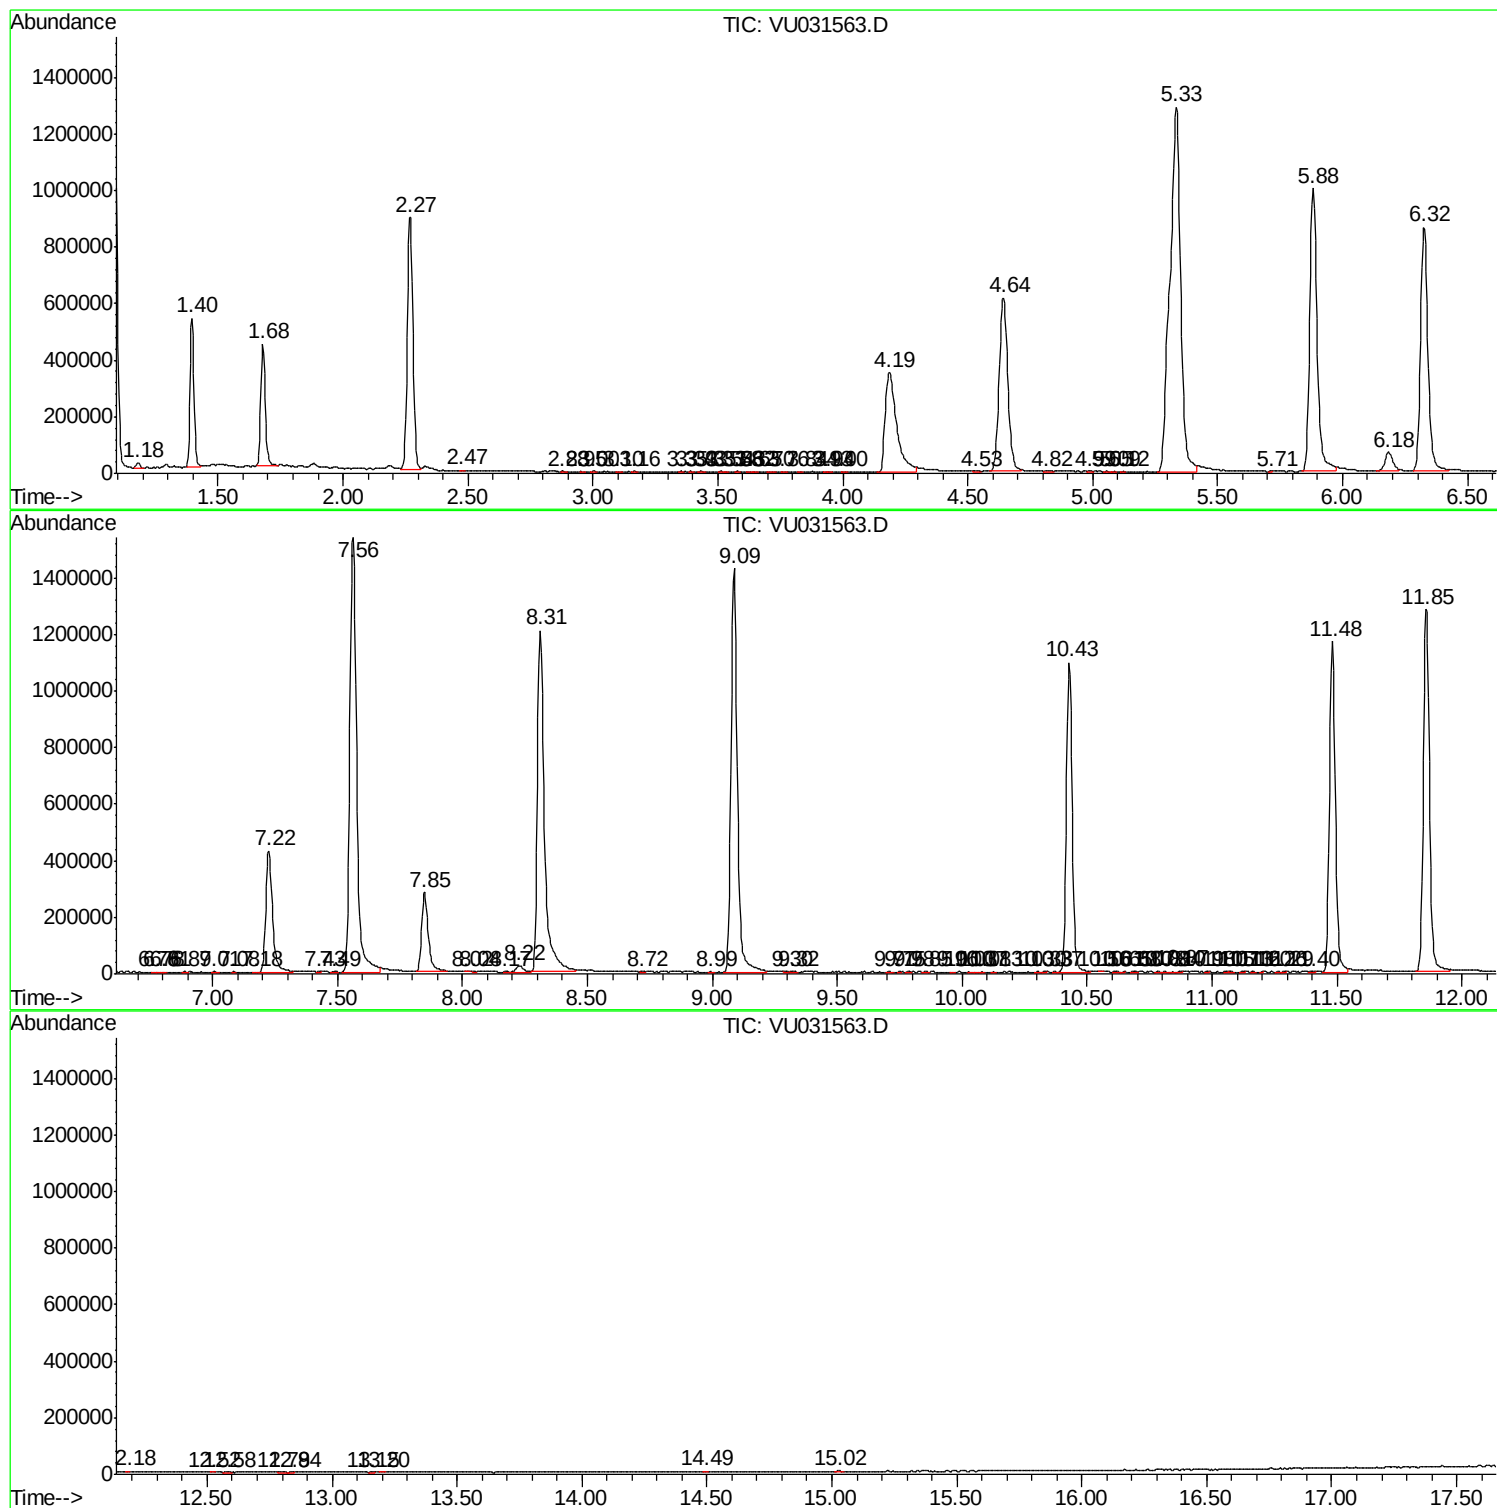

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031563.D
Acq On : 27 Apr 2019 04:09
Operator : JC/SP
Sample : K2592-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031563.D
Acq On : 27 Apr 2019 04:09
Operator : JC/SP
Sample : K2592-16 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X82

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc