

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031564.D
 Acq On : 27 Apr 2019 04:32
 Operator : JC/SP
 Sample : K2592-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB	15802	13892	0.36%	0.050%
2	1.395	88	95	110	rBV	538712	585277	15.10%	2.093%
3	1.678	176	183	197	rVB	414756	511975	13.21%	1.830%
4	2.270	356	367	381	rBV	890880	1368683	35.31%	4.893%
5	2.434	416	418	421	rBV3	1323	778	0.02%	0.003%
6	2.492	433	436	441	rBV3	1634	1276	0.03%	0.005%
7	2.518	441	444	449	rBV4	1486	1558	0.04%	0.006%
8	2.646	479	484	486	rBV6	916	1020	0.03%	0.004%
9	2.694	496	499	502	rBV5	2709	2439	0.06%	0.009%
10	2.829	536	541	543	rBV3	1577	1260	0.03%	0.005%
11	2.865	547	552	557	rBV5	2161	1957	0.05%	0.007%
12	2.939	573	575	578	rBV2	1171	800	0.02%	0.003%
13	2.987	587	590	595	rVB5	1079	1010	0.03%	0.004%
14	3.029	601	603	611	rVB5	1271	1525	0.04%	0.005%
15	3.096	621	624	629	rBV4	1222	1193	0.03%	0.004%
16	3.161	640	644	647	rVB4	1095	892	0.02%	0.003%
17	3.444	727	732	734	rBV	1278	1226	0.03%	0.004%
18	3.456	734	736	742	rVB3	1509	1129	0.03%	0.004%
19	3.534	756	760	763	rVB3	1110	806	0.02%	0.003%
20	3.659	796	799	806	rVB3	1098	900	0.02%	0.003%
21	3.720	814	818	822	rVB4	1294	1148	0.03%	0.004%
22	3.775	827	835	839	rVB4	1196	1206	0.03%	0.004%
23	3.984	896	900	903	rVB3	1196	957	0.02%	0.003%
24	4.112	937	940	945	rVB2	1628	1299	0.03%	0.005%
25	4.186	950	963	996	rBV2	357035	1104254	28.49%	3.948%
26	4.572	1080	1083	1086	rBV3	1727	1353	0.03%	0.005%
27	4.643	1087	1105	1131	rVV2	618248	1483201	38.26%	5.303%
28	4.945	1195	1199	1204	rVB6	1067	1107	0.03%	0.004%
29	4.974	1204	1208	1209	rBV3	1162	806	0.02%	0.003%
30	5.064	1232	1236	1241	rBV3	1438	1273	0.03%	0.005%
31	5.144	1258	1261	1266	rVB5	2152	1458	0.04%	0.005%
32	5.177	1266	1271	1274	rBV4	1583	1319	0.03%	0.005%
33	5.334	1297	1320	1345	rBV2	1305810	3876602	100.00%	13.860%
34	5.630	1410	1412	1416	rVB4	1482	831	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031564.D
 Acq On : 27 Apr 2019 04:32
 Operator : JC/SP
 Sample : K2592-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.672	1420	1425	1427	rBV4	2540	2169	0.06%	0.008%
36	5.881	1475	1490	1524	rBV	1013270	2094488	54.03%	7.488%
37	6.135	1565	1569	1571	rBV4	1656	1239	0.03%	0.004%
38	6.183	1573	1584	1597	rVV5	44634	100526	2.59%	0.359%
39	6.324	1615	1628	1652	rBV	849098	1743850	44.98%	6.235%
40	6.527	1688	1691	1694	rBV3	2028	1593	0.04%	0.006%
41	6.595	1707	1712	1716	rBV4	1987	2343	0.06%	0.008%
42	6.742	1755	1758	1764	rVB4	1558	1639	0.04%	0.006%
43	6.791	1771	1773	1778	rVV2	990	906	0.02%	0.003%
44	6.829	1780	1785	1788	rVV4	1689	1163	0.03%	0.004%
45	6.894	1802	1805	1808	rBV4	1669	1041	0.03%	0.004%
46	6.993	1832	1836	1840	rBV3	1276	1469	0.04%	0.005%
47	7.016	1840	1843	1847	rVV3	1291	1201	0.03%	0.004%
48	7.157	1884	1887	1890	rBV3	1028	891	0.02%	0.003%
49	7.225	1896	1908	1936	rVV	416681	796017	20.53%	2.846%
50	7.363	1948	1951	1956	rBV3	1862	1783	0.05%	0.006%
51	7.414	1963	1967	1969	rBV5	1085	857	0.02%	0.003%
52	7.562	2000	2013	2054	rBV	1537658	2880317	74.30%	10.298%
53	7.848	2091	2102	2124	rBV	281178	519975	13.41%	1.859%
54	8.112	2179	2184	2185	rBV2	1186	1177	0.03%	0.004%
55	8.183	2201	2206	2208	rBV3	1441	1129	0.03%	0.004%
56	8.228	2209	2220	2231	rVV5	27005	49494	1.28%	0.177%
57	8.311	2235	2246	2291	rBV	1213753	2388353	61.61%	8.539%
58	8.868	2417	2419	2423	rVV3	1761	1445	0.04%	0.005%
59	8.890	2424	2426	2433	rVB6	2009	1729	0.04%	0.006%
60	8.964	2447	2449	2453	rVB4	1650	945	0.02%	0.003%
61	9.000	2455	2460	2463	rVB4	1552	1459	0.04%	0.005%
62	9.086	2474	2487	2524	rBV	1416221	2501006	64.52%	8.942%
63	9.273	2543	2545	2550	rVB5	1485	898	0.02%	0.003%
64	9.434	2592	2595	2598	rVB3	1394	789	0.02%	0.003%
65	9.466	2598	2605	2606	rBV6	1433	1355	0.03%	0.005%
66	9.575	2633	2639	2640	rBV2	1240	991	0.03%	0.004%
67	9.627	2651	2655	2659	rBV2	1015	1083	0.03%	0.004%
68	9.652	2659	2663	2664	rBV2	1229	919	0.02%	0.003%
69	9.848	2719	2724	2726	rBV3	1736	1773	0.05%	0.006%
70	9.945	2749	2754	2755	rBV2	1086	849	0.02%	0.003%
71	10.147	2813	2817	2820	rBV4	916	940	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031564.D
 Acq On : 27 Apr 2019 04:32
 Operator : JC/SP
 Sample : K2592-17 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X83

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.250	2846	2849	2852	rBV3	1283	853	0.02%	0.003%
73	10.295	2861	2863	2867	rVB	1382	877	0.02%	0.003%
74	10.331	2871	2874	2877	rVV3	1220	776	0.02%	0.003%
75	10.363	2881	2884	2886	rBV2	1215	865	0.02%	0.003%
76	10.427	2890	2904	2927	rBV	1083362	1769943	45.66%	6.328%
77	10.607	2956	2960	2963	rBV3	1358	1241	0.03%	0.004%
78	10.752	3002	3005	3008	rBV5	1298	1103	0.03%	0.004%
79	11.051	3095	3098	3099	rBV	1371	839	0.02%	0.003%
80	11.138	3120	3125	3126	rBV3	1074	870	0.02%	0.003%
81	11.186	3138	3140	3145	rVB5	1438	910	0.02%	0.003%
82	11.395	3203	3205	3213	rVB3	2023	1718	0.04%	0.006%
83	11.482	3219	3232	3259	rBV	1181983	1940937	50.07%	6.939%
84	11.800	3327	3331	3332	rBV3	1104	896	0.02%	0.003%
85	11.855	3336	3348	3372	rVV	1268439	2142148	55.26%	7.659%
86	12.530	3554	3558	3562	rVB5	1354	965	0.02%	0.003%
87	12.630	3585	3589	3591	rBV2	1282	1082	0.03%	0.004%
88	12.643	3591	3593	3596	rVV2	1881	1101	0.03%	0.004%
89	12.662	3597	3599	3603	rVB2	1548	929	0.02%	0.003%
90	12.745	3620	3625	3629	rBV2	1458	1472	0.04%	0.005%
91	12.810	3642	3645	3647	rBV3	1749	1350	0.03%	0.005%
92	12.884	3663	3668	3672	rBV4	2356	2688	0.07%	0.010%
93	13.048	3716	3719	3722	rBV2	1245	1049	0.03%	0.004%
94	13.331	3805	3807	3812	rVB3	1522	1127	0.03%	0.004%
95	13.356	3812	3815	3817	rBV3	1334	1029	0.03%	0.004%
96	13.562	3876	3879	3882	rBV	1449	1111	0.03%	0.004%
97	13.713	3922	3926	3933	rBV6	2222	2709	0.07%	0.010%
98	13.964	4001	4004	4007	rBV3	1548	1375	0.04%	0.005%
99	14.282	4101	4103	4107	rBV2	1754	980	0.03%	0.004%
100	14.610	4201	4205	4206	rBV3	1352	1014	0.03%	0.004%


Sum of corrected areas: 27970168

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031564.D
Acq On : 27 Apr 2019 04:32
Operator : JC/SP
Sample : K2592-17 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

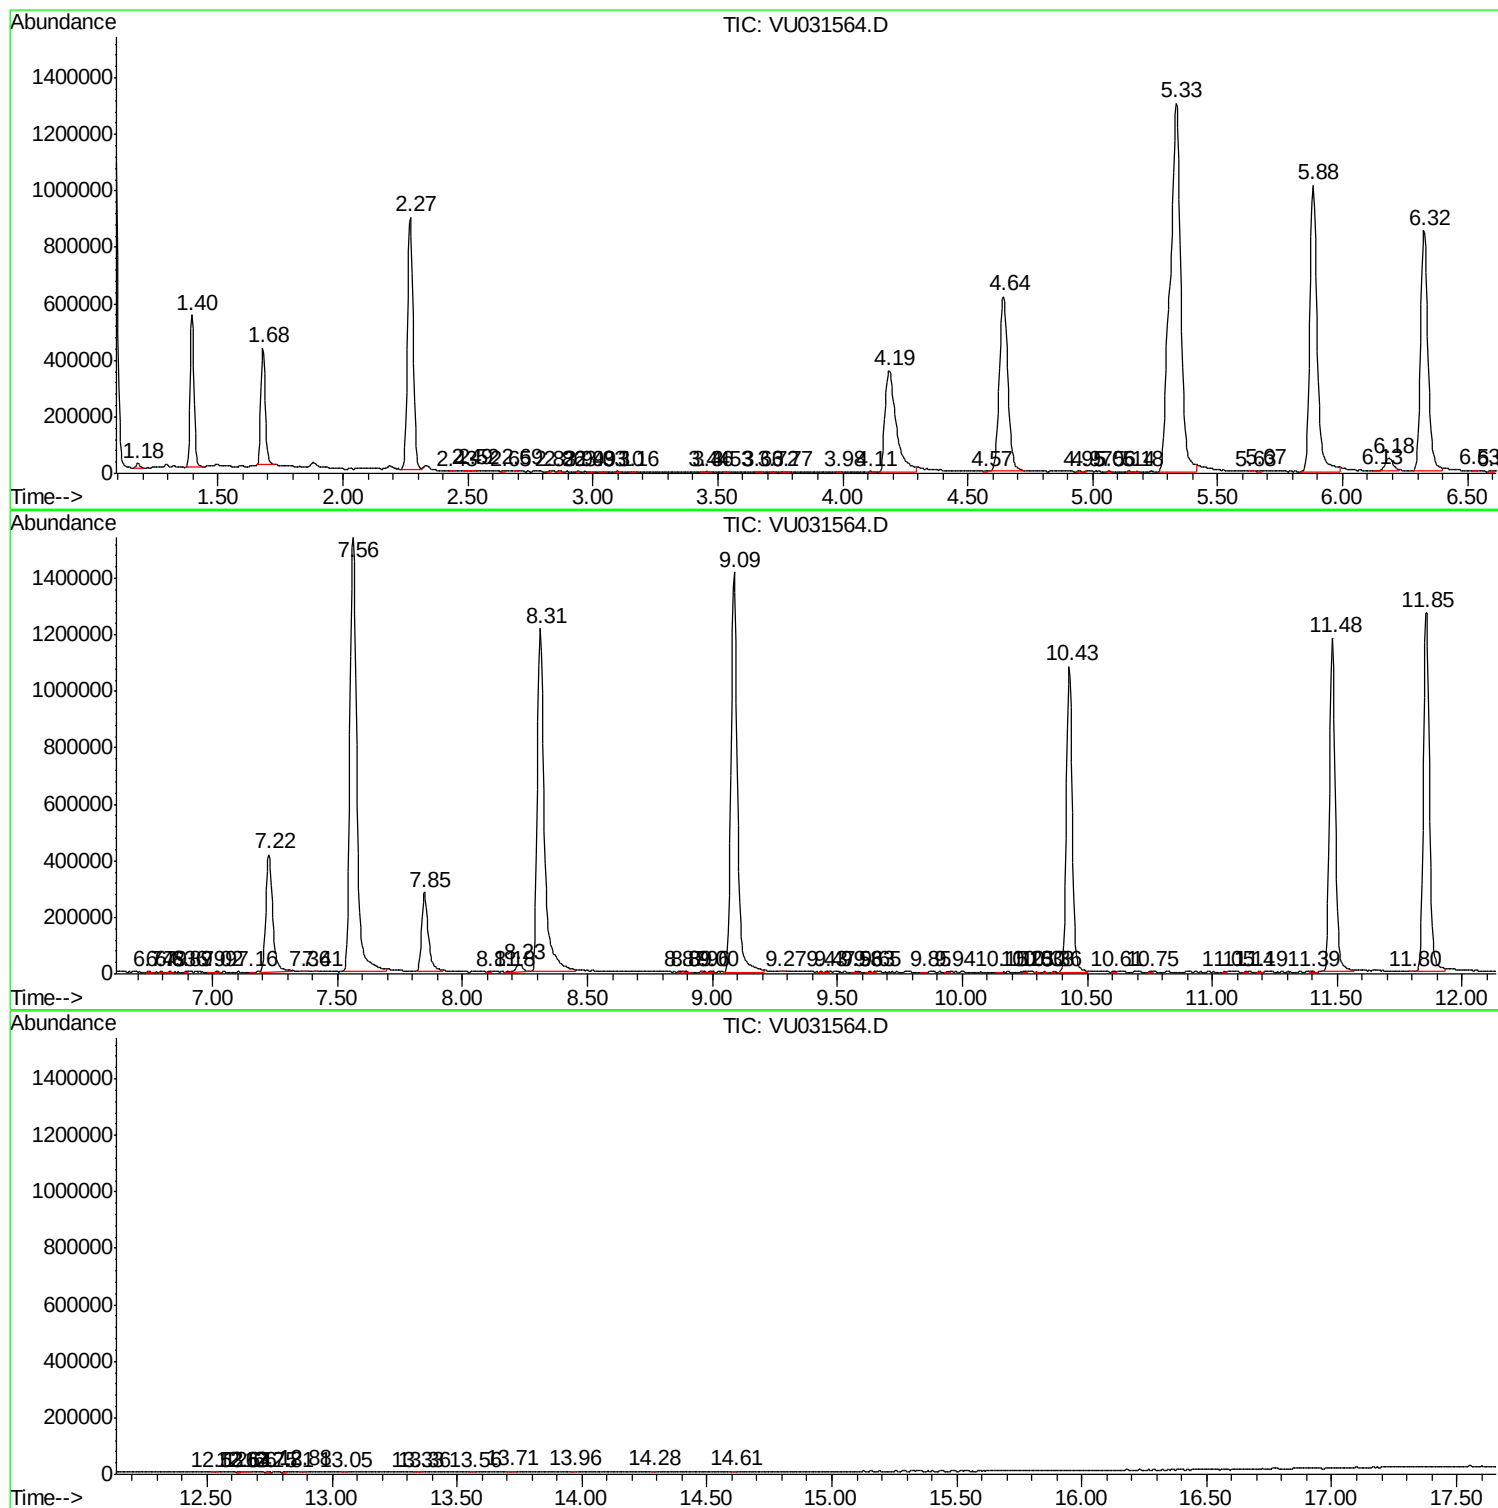

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031564.D
Acq On : 27 Apr 2019 04:32
Operator : JC/SP
Sample : K2592-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031564.D
Acq On : 27 Apr 2019 04:32
Operator : JC/SP
Sample : K2592-17 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X83

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc